




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019851.D
 Acq On : 19 May 2022 09:20
 Operator : CG/JU
 Sample : PB144854BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK854

Manual IntegrationsAPPROVED

Quant Time: May 19 17:58:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :mohammad ahmed 05/25/2022

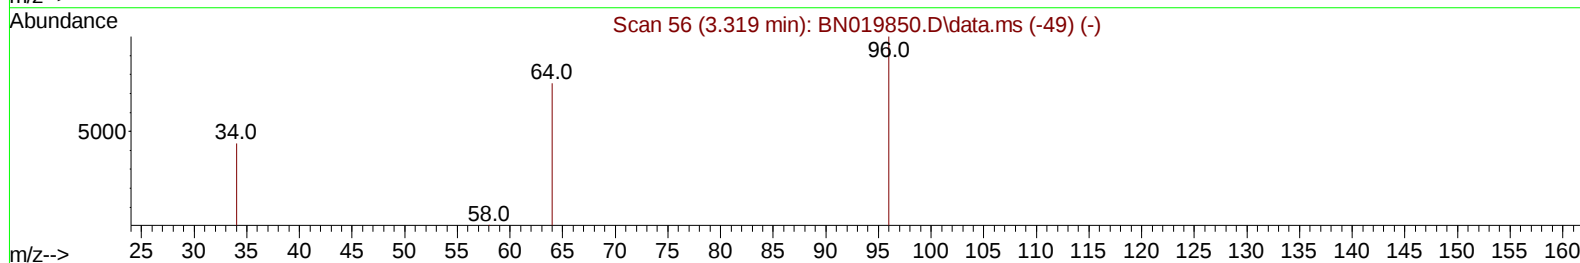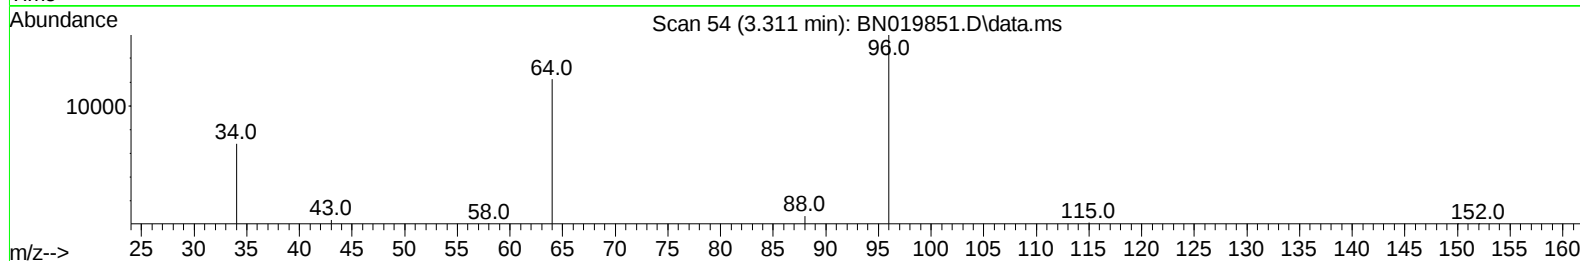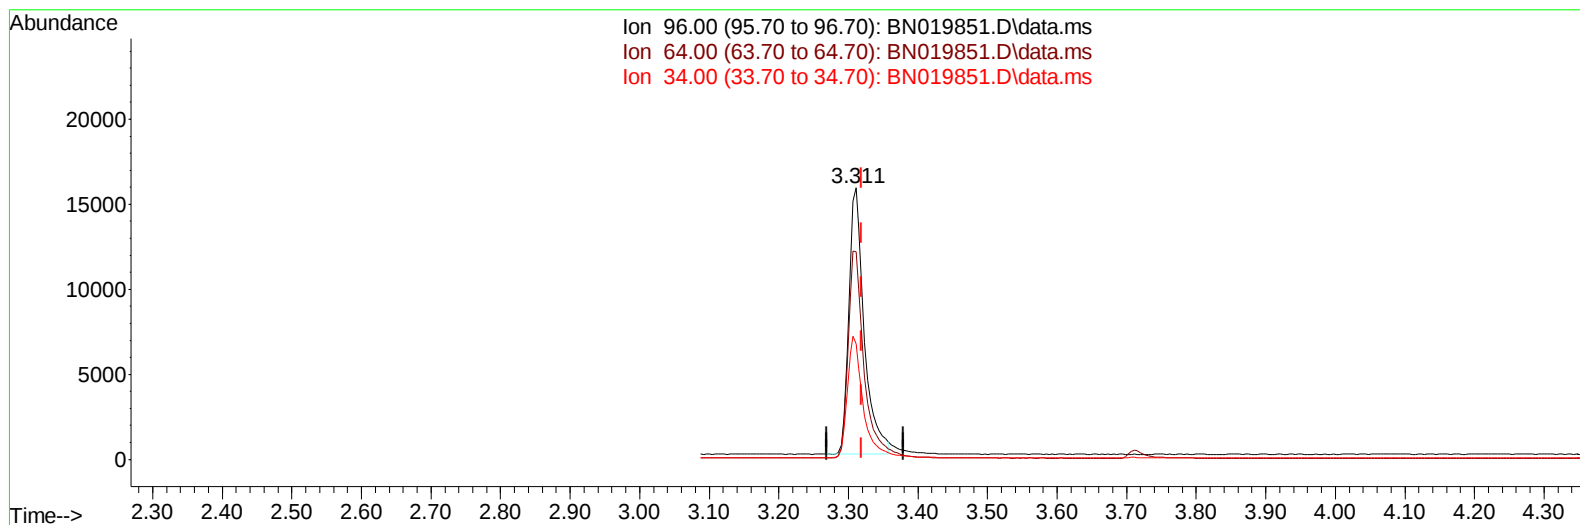

TIC: BN019851.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.311min (-0.008) 5.23 ng/u1

response 24043

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.57#
34.00	22.70	42.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019851.D
Acq On : 19 May 2022 09:20
Operator : CG/JU
Sample : PB144854BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK854

Manual IntegrationsAPPROVED

Quant Time: May 19 17:58:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :mohammad ahmed 05/25/2022

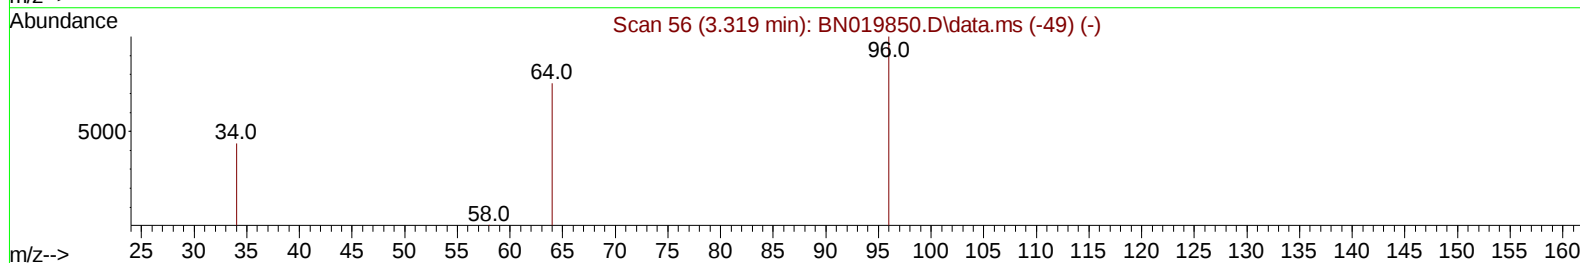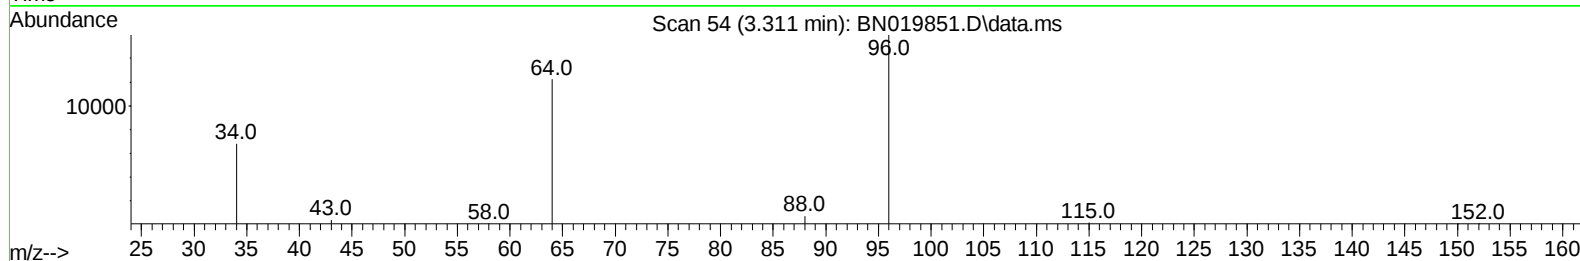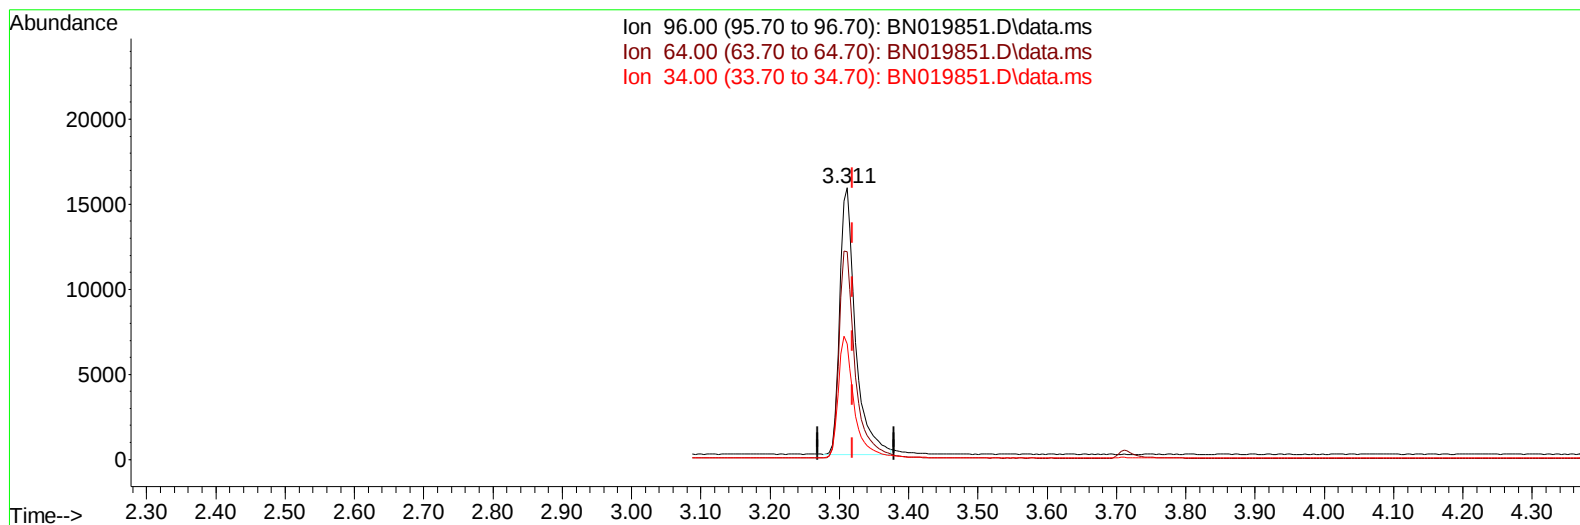

TIC: BN019851.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.311min (-0.008) 5.37 ng/ul m

response 24652

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	76.57#
34.00	22.70	42.46#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019851.D
 Acq On : 19 May 2022 09:20
 Operator : CG/JU
 Sample : PB144854BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK854

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 17:58:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.838	152		3881	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.628	136		13411	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.469	164		9097	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		20757	0.400	ng/ul	0.00
17) Chrysene-d12	21.406	240		17804	0.400	ng/ul	0.00
23) Perylene-d12	23.747	264		16587	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.311	96		24652m	5.367	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152		6342	0.313	ng/ul	-0.01
18) Fluoranthene-d10	19.244	212		15386	0.273	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019851.D
Acq On : 19 May 2022 09:20
Operator : CG/JU
Sample : PB144854BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK854

Manual IntegrationsAPPROVED

Quant Time: May 19 17:58:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :mohammad ahmed 05/25/2022

