




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019852.D
Acq On : 19 May 2022 10:22
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 11:00:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :mohammad ahmed 05/25/2022

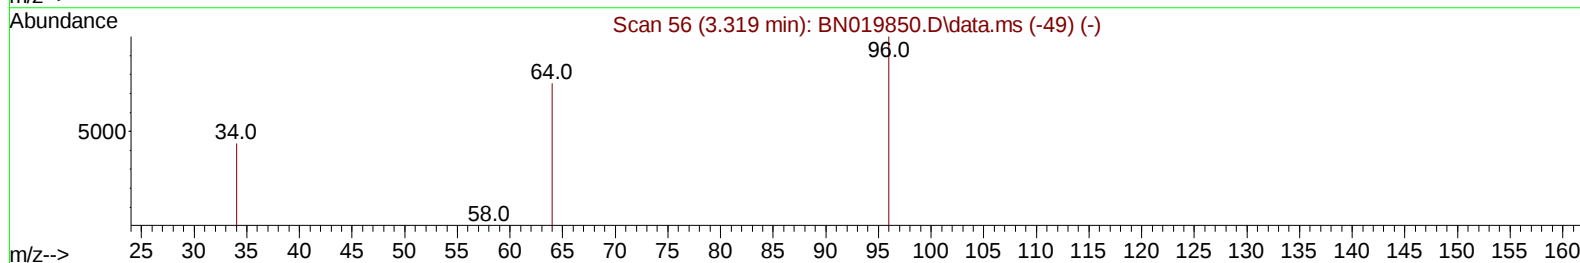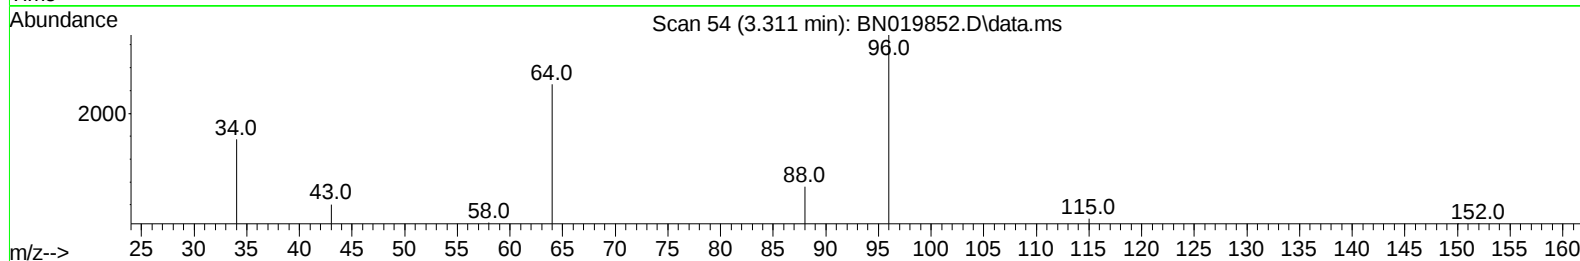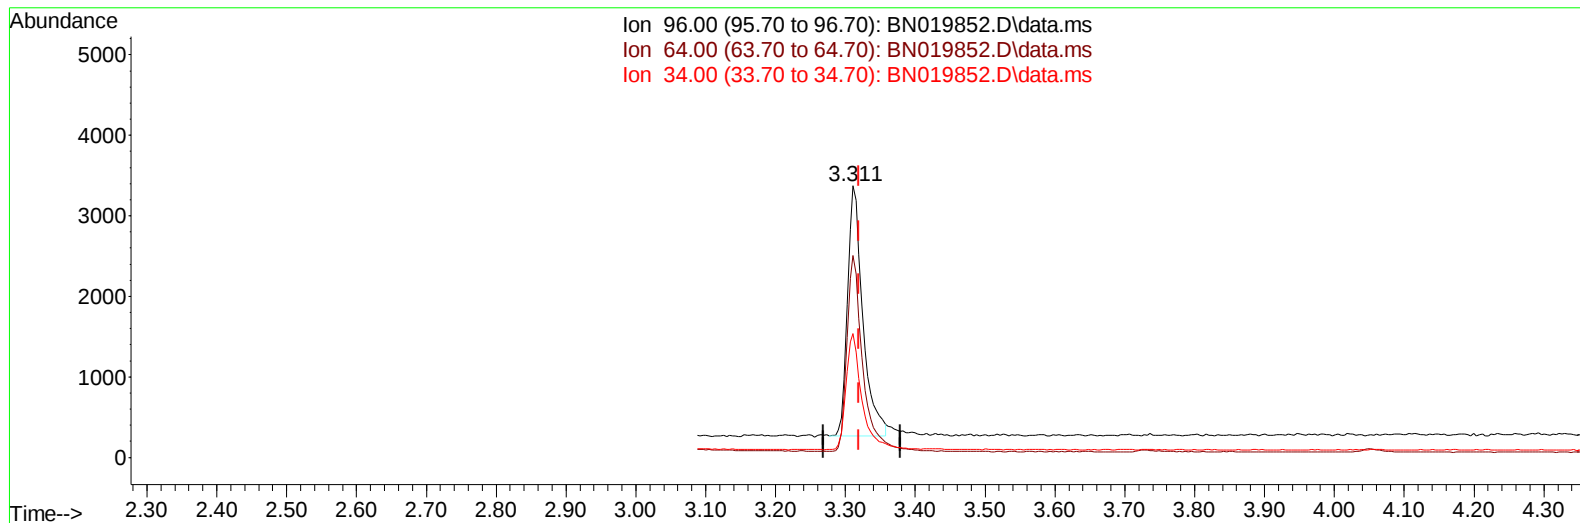

TIC: BN019852.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.311min (-0.008) 0.98 ng/u1

response 4724

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	74.43#
34.00	22.70	45.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019852.D
Acq On : 19 May 2022 10:22
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 11:00:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :mohammad ahmed 05/25/2022

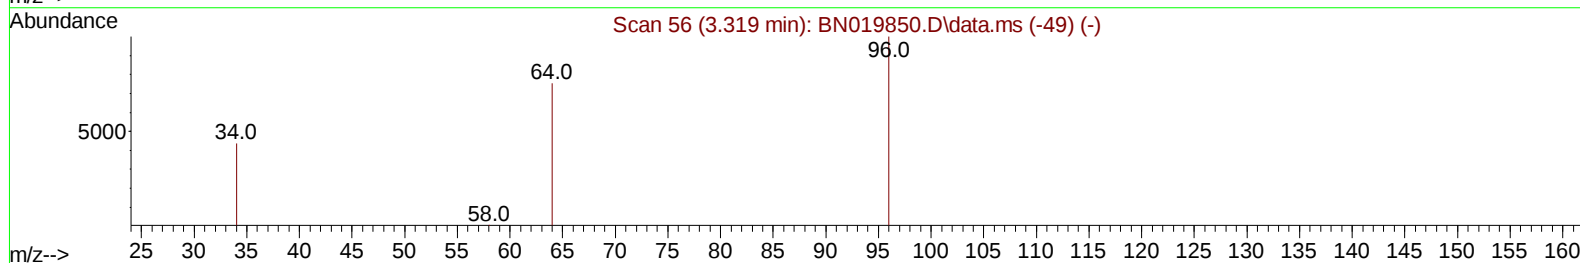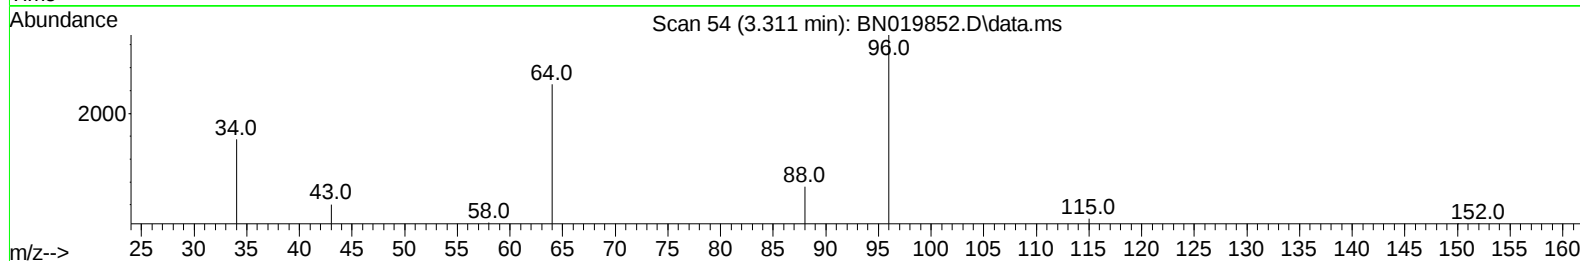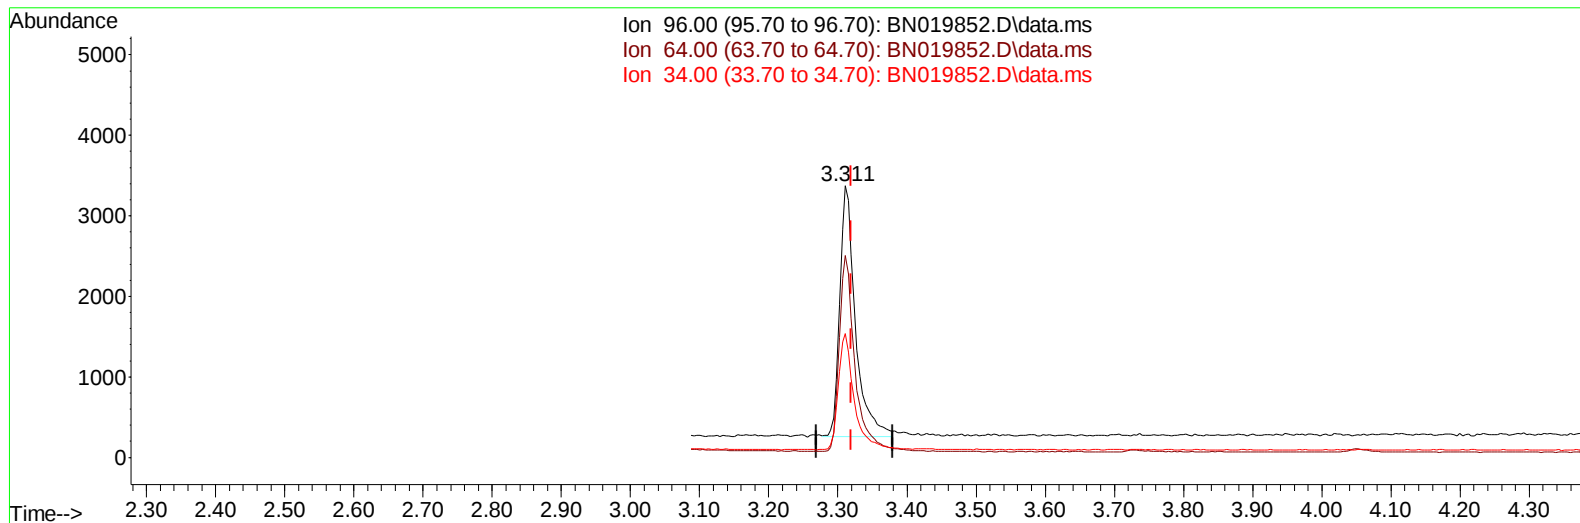

TIC: BN019852.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.311min (-0.008) 1.01 ng/ul m

response 4865

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	40.10	74.43#
34.00	22.70	45.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
 Data File : BN019852.D
 Acq On : 19 May 2022 10:22
 Operator : CG/JU
 Sample : N2766-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4F9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :mohammad ahmed 05/25/2022

Quant Time: May 19 11:00:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 17 01:41:05 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.842	152		4060	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.634	136		14180	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.469	164		9223	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188		20272	0.400	ng/ul	0.00
17) Chrysene-d12	21.404	240		17650	0.400	ng/ul	0.00
23) Perylene-d12	23.746	264		15524	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.311	96		4865m	1.012	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152		4164	0.194	ng/ul	-0.01
18) Fluoranthene-d10	19.244	212		10443	0.187	ng/ul	0.00
Target Compounds							Qvalue
7) 2-Methylnaphthalene	12.300	142		580	0.021	ng/ul#	100
8) 1-Methylnaphthalene	12.514	142		574	0.022	ng/ul#	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN051822\
Data File : BN019852.D
Acq On : 19 May 2022 10:22
Operator : CG/JU
Sample : N2766-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4F9

Manual IntegrationsAPPROVED

Quant Time: May 19 11:00:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN042922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 17 01:41:05 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :mohammad ahmed 05/25/2022

