

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019926.D
 Acq On : 24 May 2022 16:57
 Operator : CG/JU
 Sample : PB144964BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK964

Quant Time: May 25 01:45:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.850	152	4119	0.400	ng/ul	0.00
4) Naphthalene-d8	10.638	136	14362	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	8782	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.211	188	18215	0.400	ng/ul	0.00
17) Chrysene-d12	21.402	240	13362	0.400	ng/ul	0.00
23) Perylene-d12	23.744	264	11035	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	20781	5.411	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.227	152	6557	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.242	212	14464	0.303	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.467	166	2040	0.054	ng/ul#	14
20) Pyrene	19.609	202	1790	0.026	ng/ul#	1
26) Benzo(a)pyrene	23.592	252	3053	0.066	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019926.D
Acq On : 24 May 2022 16:57
Operator : CG/JU
Sample : PB144964BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK964

Quant Time: May 25 01:45:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration




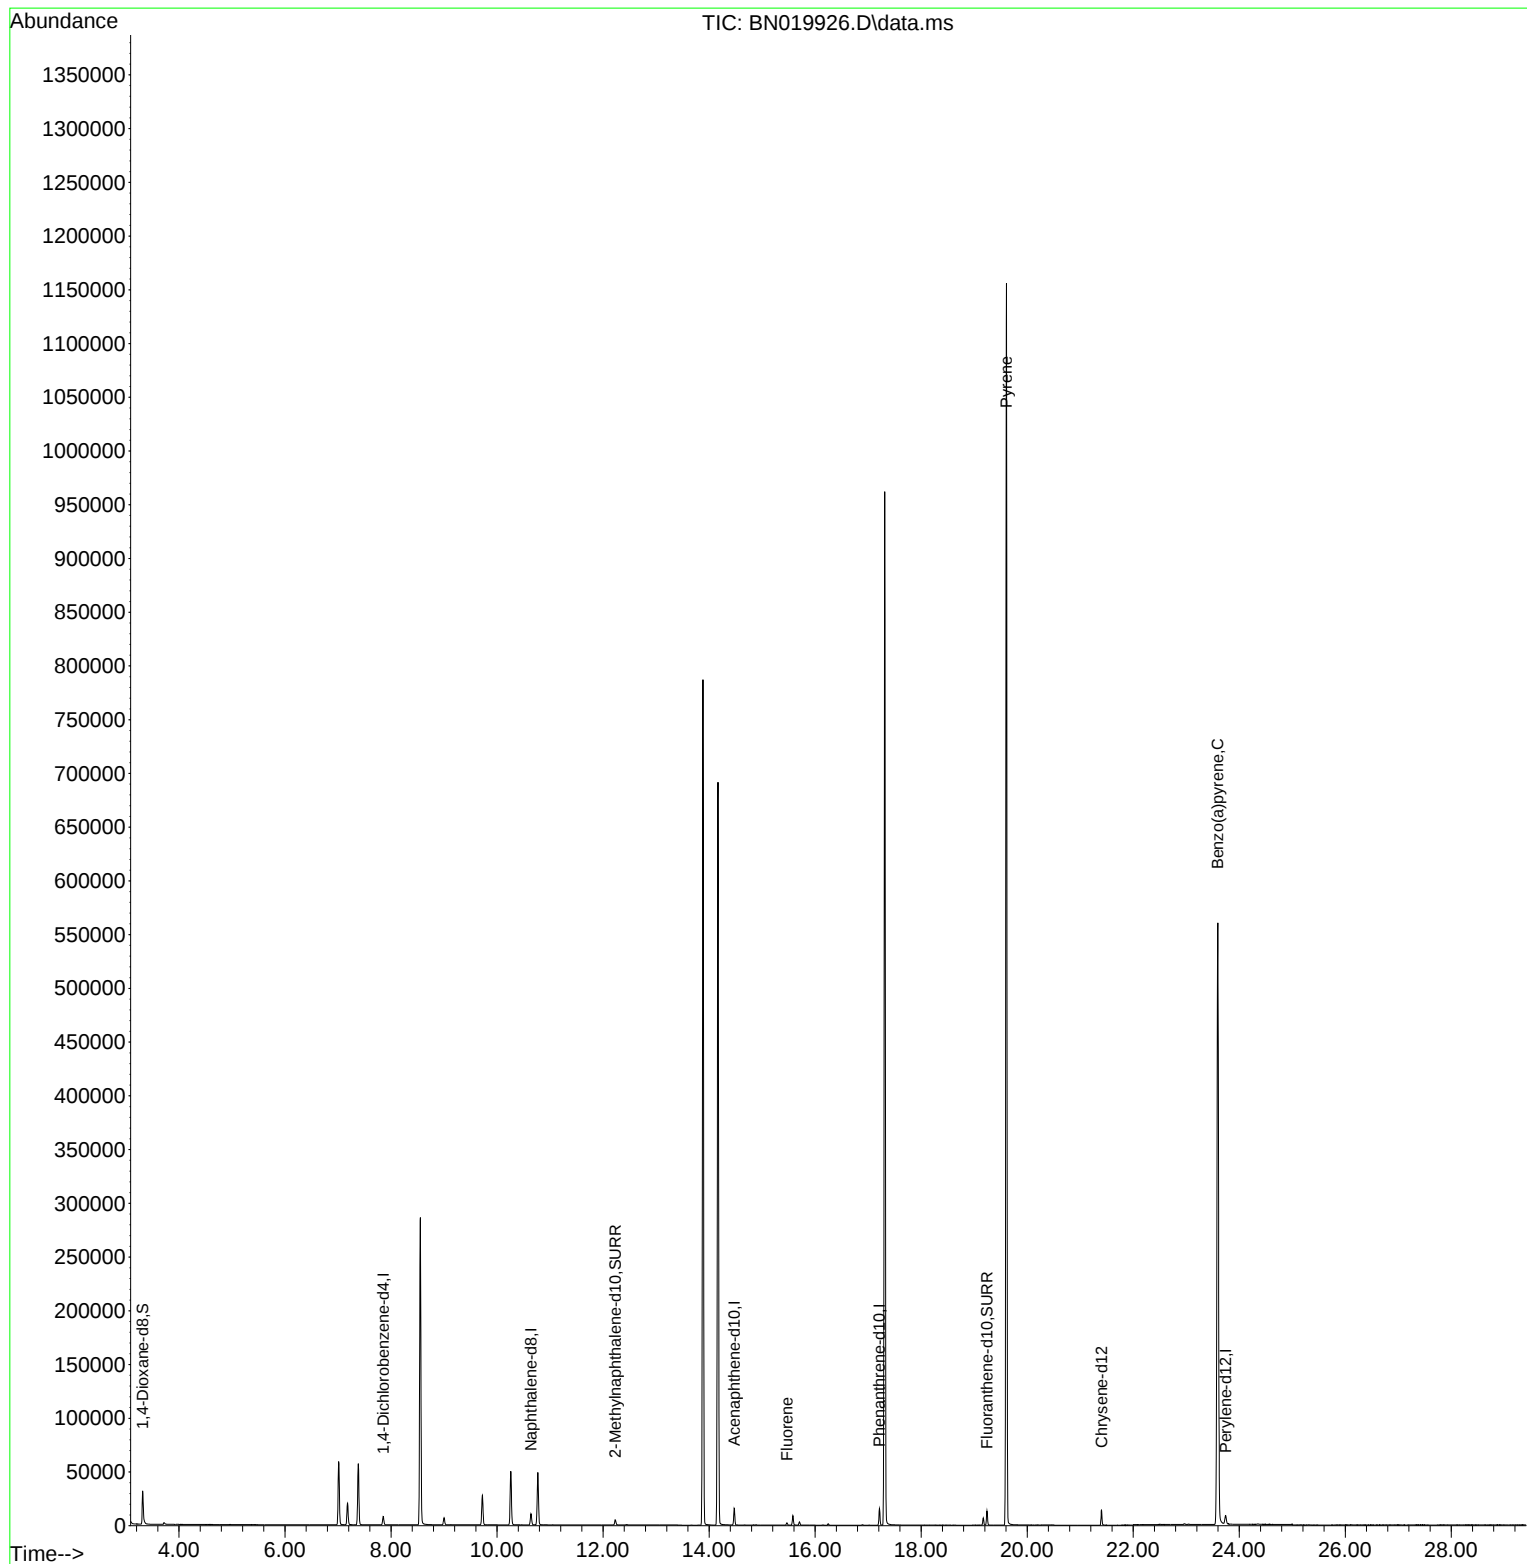


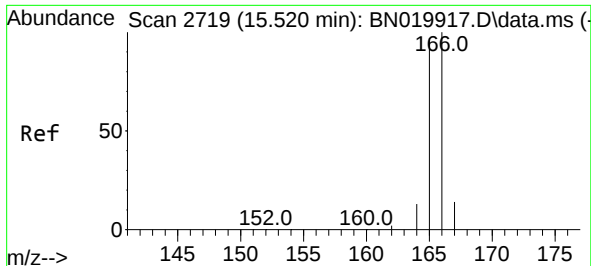

#12
Fluorene
Concen: 0.054 ng/ul
RT: 15.467 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN019926.D
Acq: 24 May 2022 16:57




Instrument :
BNA_N
ClientSampleId :
SBLK964


Tgt Ion:166 Resp: 2040
Ion Ratio Lower Upper
166 100
165 8.2 78.2 117.2#
167 35.3 11.3 16.9#

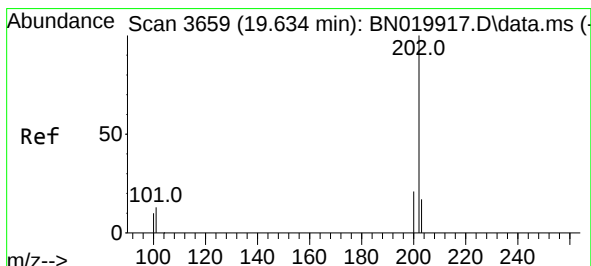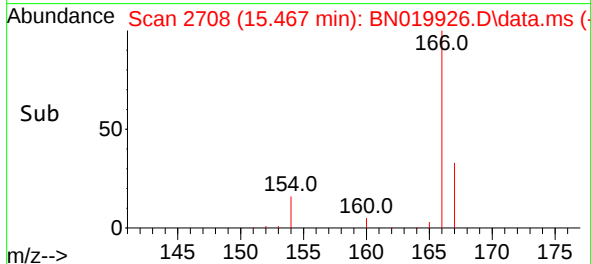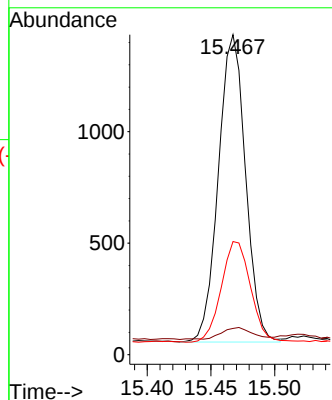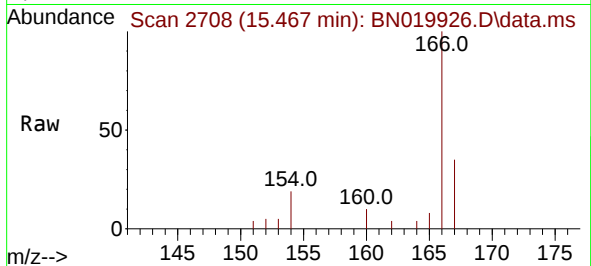

#20
Pyrene
Concen: 0.026 ng/ul
RT: 19.609 min Scan# 3654
Delta R.T. -0.028 min
Lab File: BN019926.D
Acq: 24 May 2022 16:57

Tgt Ion:202 Resp: 1790
Ion Ratio Lower Upper
202 100
101 162.8 11.4 17.0#
100 1172.0 9.0 13.4#

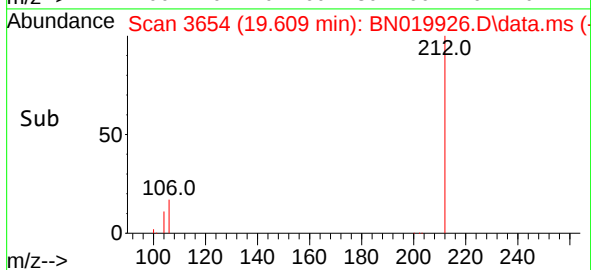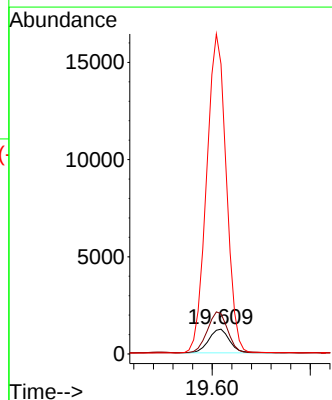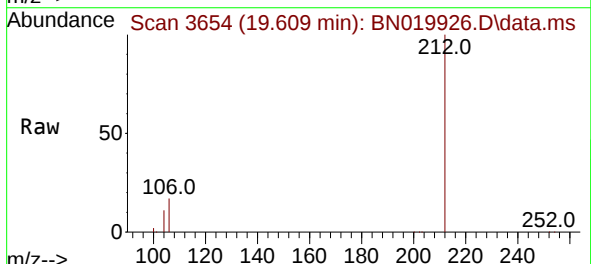

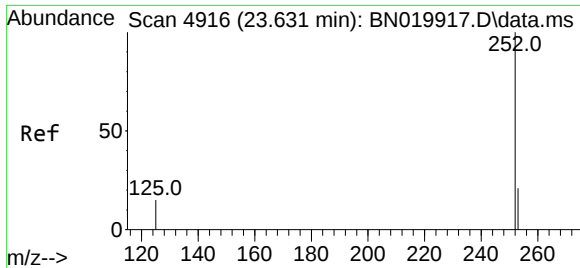

#26

Benzo(a)pyrene

Concen: 0.066 ng/ul

RT: 23.592 min Scan# 4903

Delta R.T. -0.047 min

Lab File: BN019926.D


Acq: 24 May 2022 16:57

Instrument :

BNA_N

ClientSampleId :

SBLK964

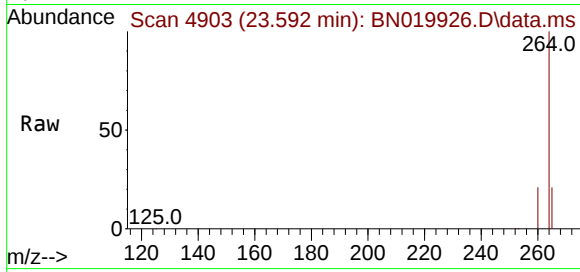

Tgt Ion:252 Resp: 3053

Ion Ratio Lower Upper

252 100

253 40.5 23.4 35.0#

125 36.7 28.3 42.5

