

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019927.D
 Acq On : 24 May 2022 17:33
 Operator : CG/JU
 Sample : PB145005BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK005

Quant Time: May 25 01:45:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3066	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	10929	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	6832	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	14415	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	12571	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264	10862	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	16495	5.770	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	5350	0.300	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	12295	0.274	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.606	202	1720	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.589	252	3111	0.069	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019927.D
Acq On : 24 May 2022 17:33
Operator : CG/JU
Sample : PB145005BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK005

Quant Time: May 25 01:45:39 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration

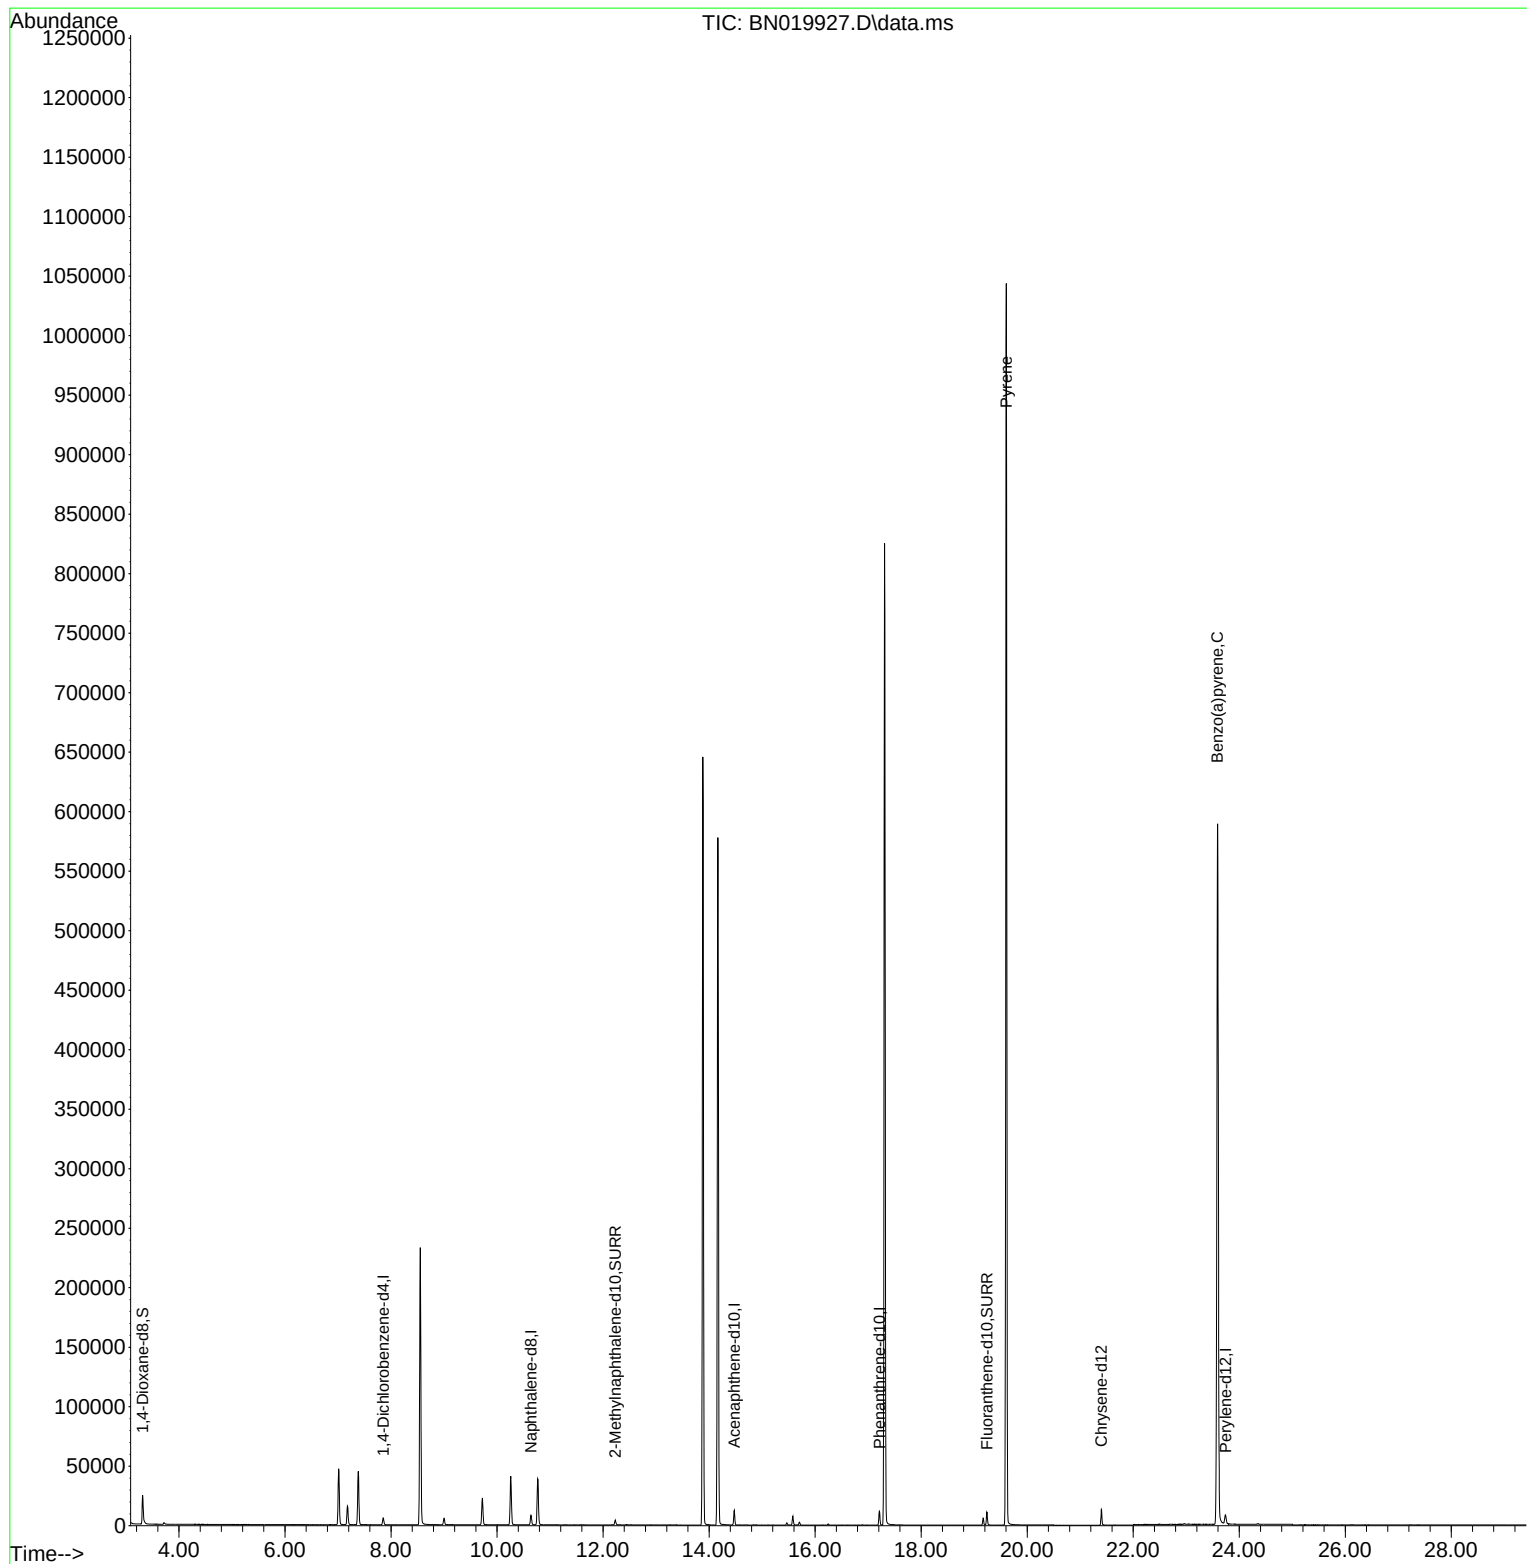

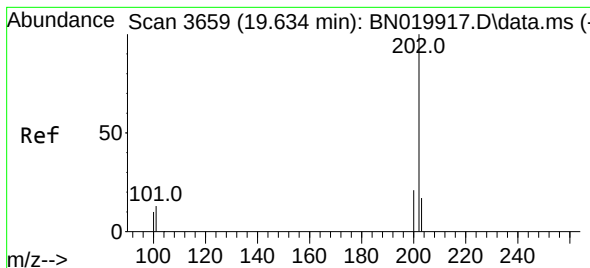

#20

Pyrene

Concen: 0.027 ng/ul

RT: 19.606 min Scan# 30

Delta R.T. -0.031 min

Lab File: BN019927.D

Acq: 24 May 2022 17:33

Instrument :





BNA_N

ClientSampleId :

SBLK005

Tgt Ion:202 Resp: 1720

Ion	Ratio	Lower	Upper
202	100		
101	167.0	11.4	17.0#
100	1196.4	9.0	13.4#

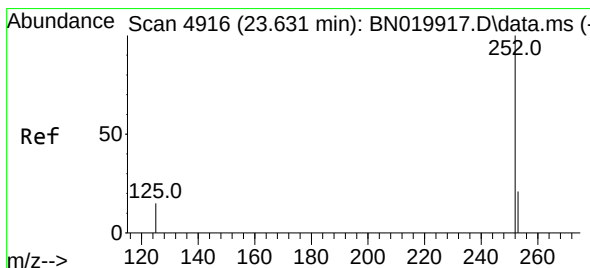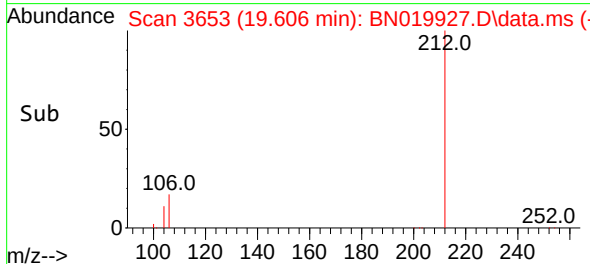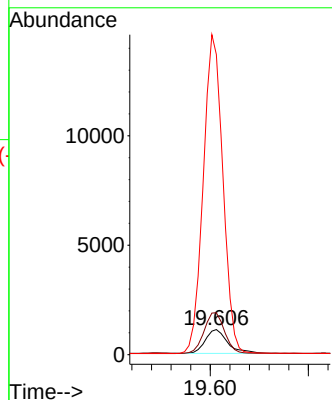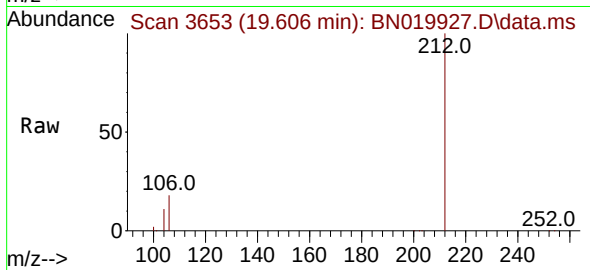

#26

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.589 min Scan# 4902

Delta R.T. -0.050 min

Lab File: BN019927.D

Acq: 24 May 2022 17:33

Tgt Ion:252 Resp: 3111

Ion	Ratio	Lower	Upper
252	100		
253	41.6	23.4	35.0#
125	35.5	28.3	42.5

