

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019928.D
 Acq On : 24 May 2022 18:09
 Operator : CG/JU
 Sample : PB145035BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK035

Quant Time: May 25 01:45:43 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3017	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	10717	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164	6694	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	13838	0.400	ng/ul	0.00
17) Chrysene-d12	21.403	240	11197	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264	9612	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	18969	6.743	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	6096	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.244	212	13975	0.349	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.606	202	1869	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.592	252	3322	0.083	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019928.D
Acq On : 24 May 2022 18:09
Operator : CG/JU
Sample : PB145035BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK035

Quant Time: May 25 01:45:43 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration




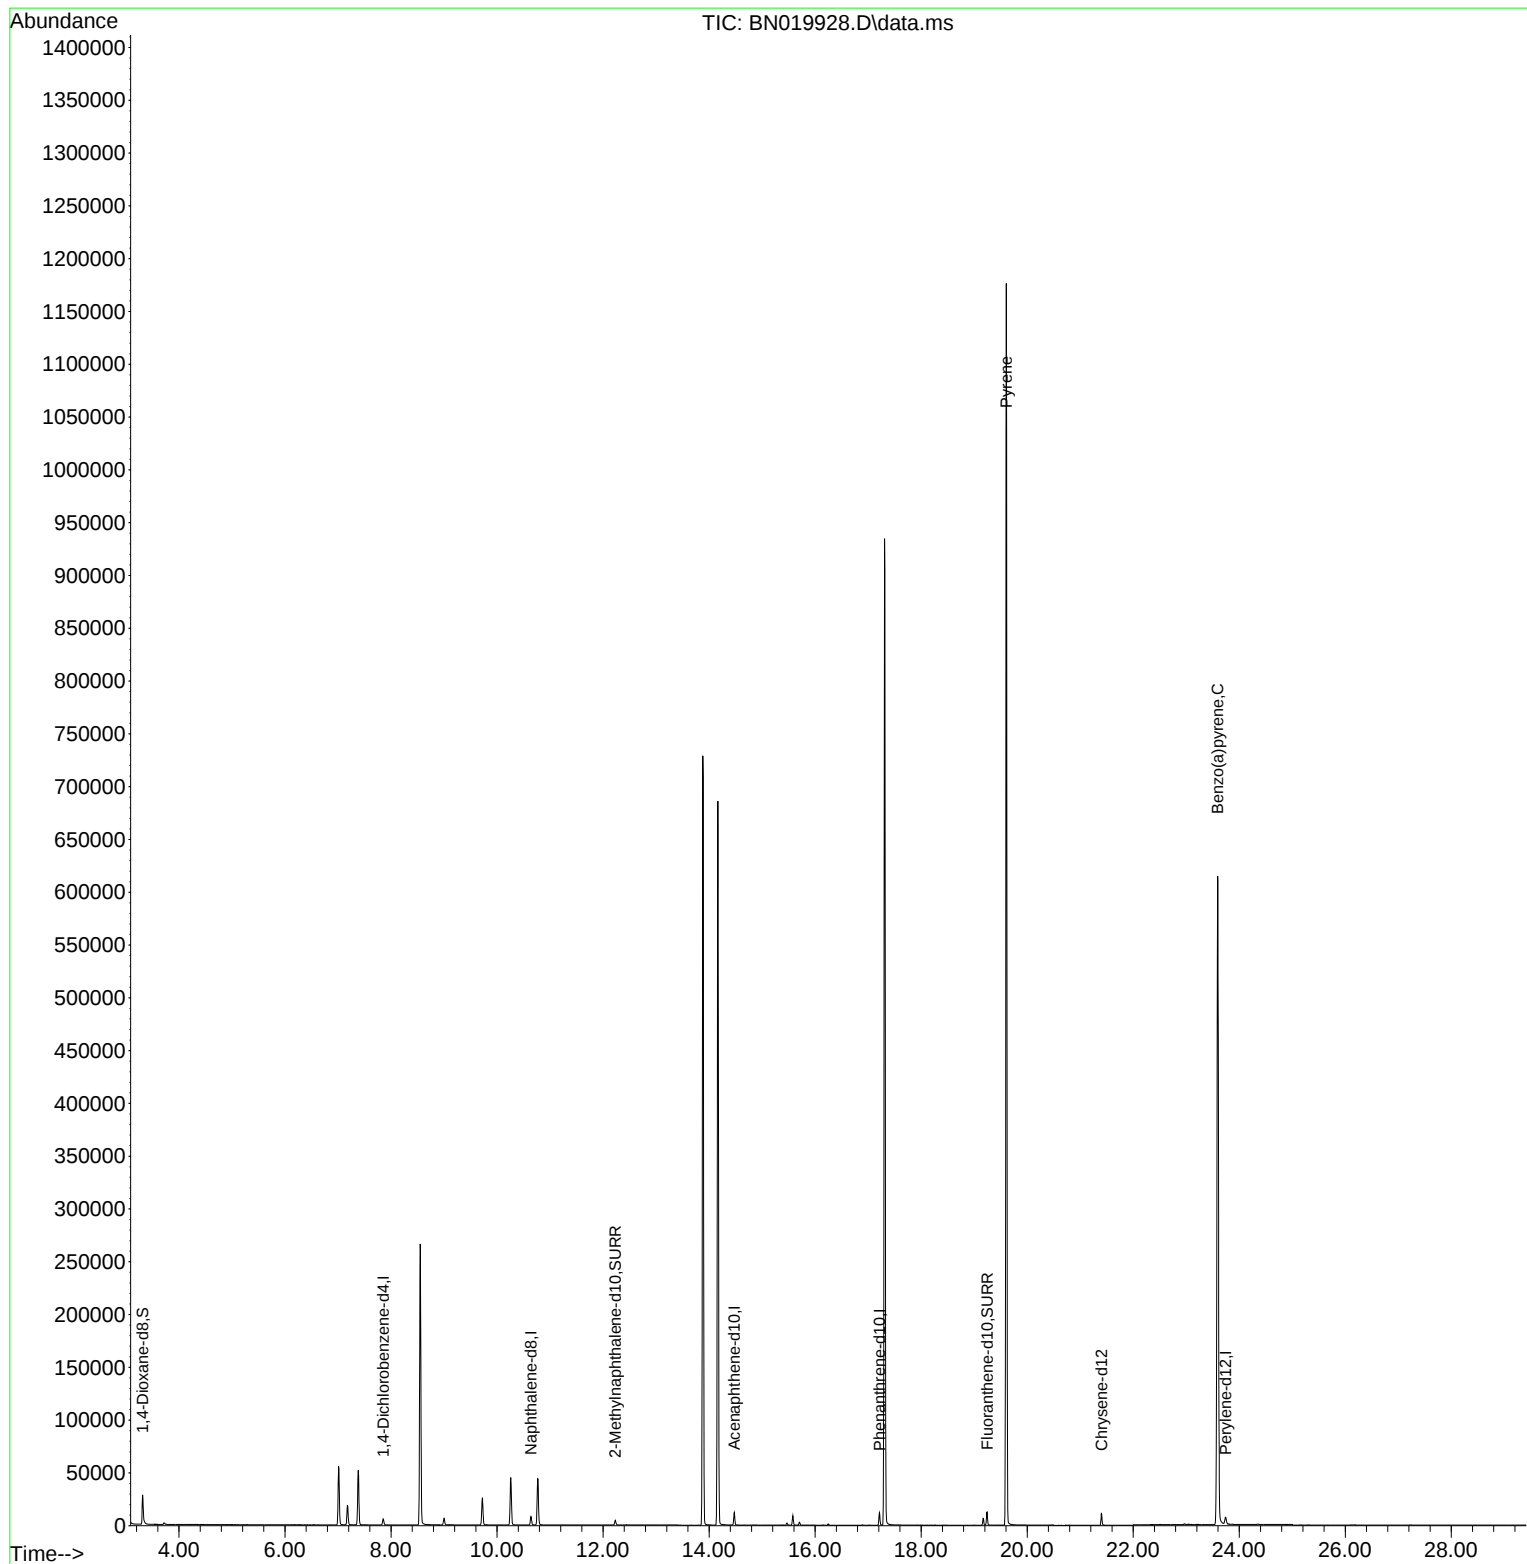


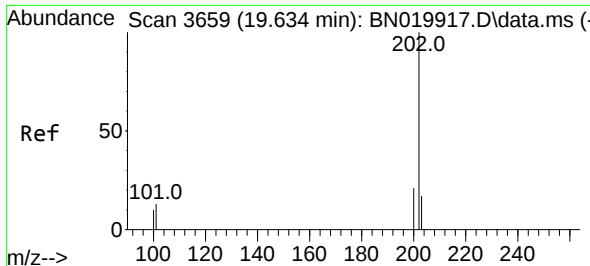

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.606 min Scan# 3653
Delta R.T. -0.031 min
Lab File: BN019928.D
Acq: 24 May 2022 18:09

Instrument :
BNA_N
ClientSampleId :
SBLK035

Tgt Ion:202 Resp: 1869
Ion Ratio Lower Upper
202 100
101 173.6 11.4 17.0#
100 1268.6 9.0 13.4#

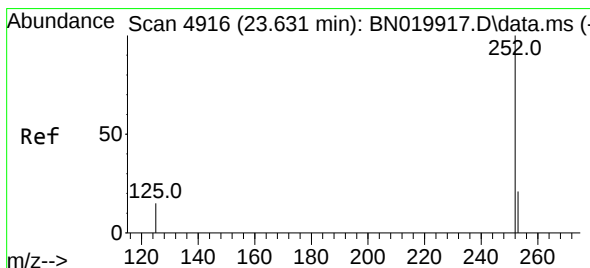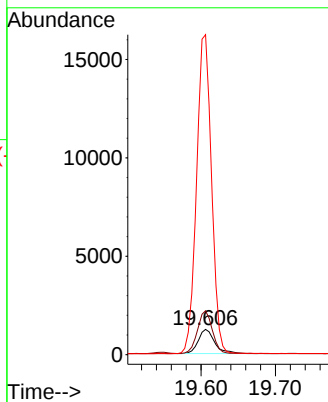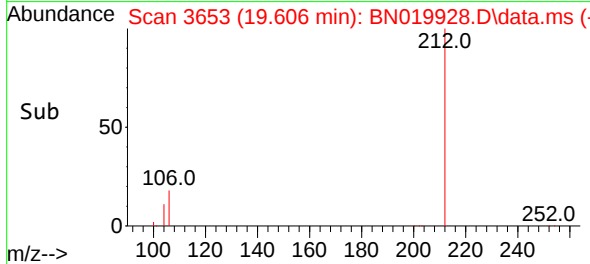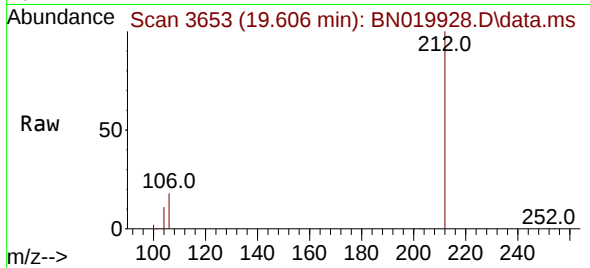

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.592 min Scan# 4903
Delta R.T. -0.047 min
Lab File: BN019928.D
Acq: 24 May 2022 18:09

Tgt Ion:252 Resp: 3322
Ion Ratio Lower Upper
252 100
253 38.8 23.4 35.0#
125 35.4 28.3 42.5

