

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019959.D
 Acq On : 25 May 2022 19:44
 Operator : CG/JU
 Sample : N2883-09
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4K9

Quant Time: May 26 01:16:01 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4014	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	14085	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.474	164	8995	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	18964	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240	13126	0.400	ng/ul	0.00
23) Perylene-d12	23.732	264	10835	0.400	ng/ul #-	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	25734	6.876	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	9257	0.403	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	20842	0.444	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.606	202	2449	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.586	252	3966	0.088	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019959.D
Acq On : 25 May 2022 19:44
Operator : CG/JU
Sample : N2883-09
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4K9

Quant Time: May 26 01:16:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration

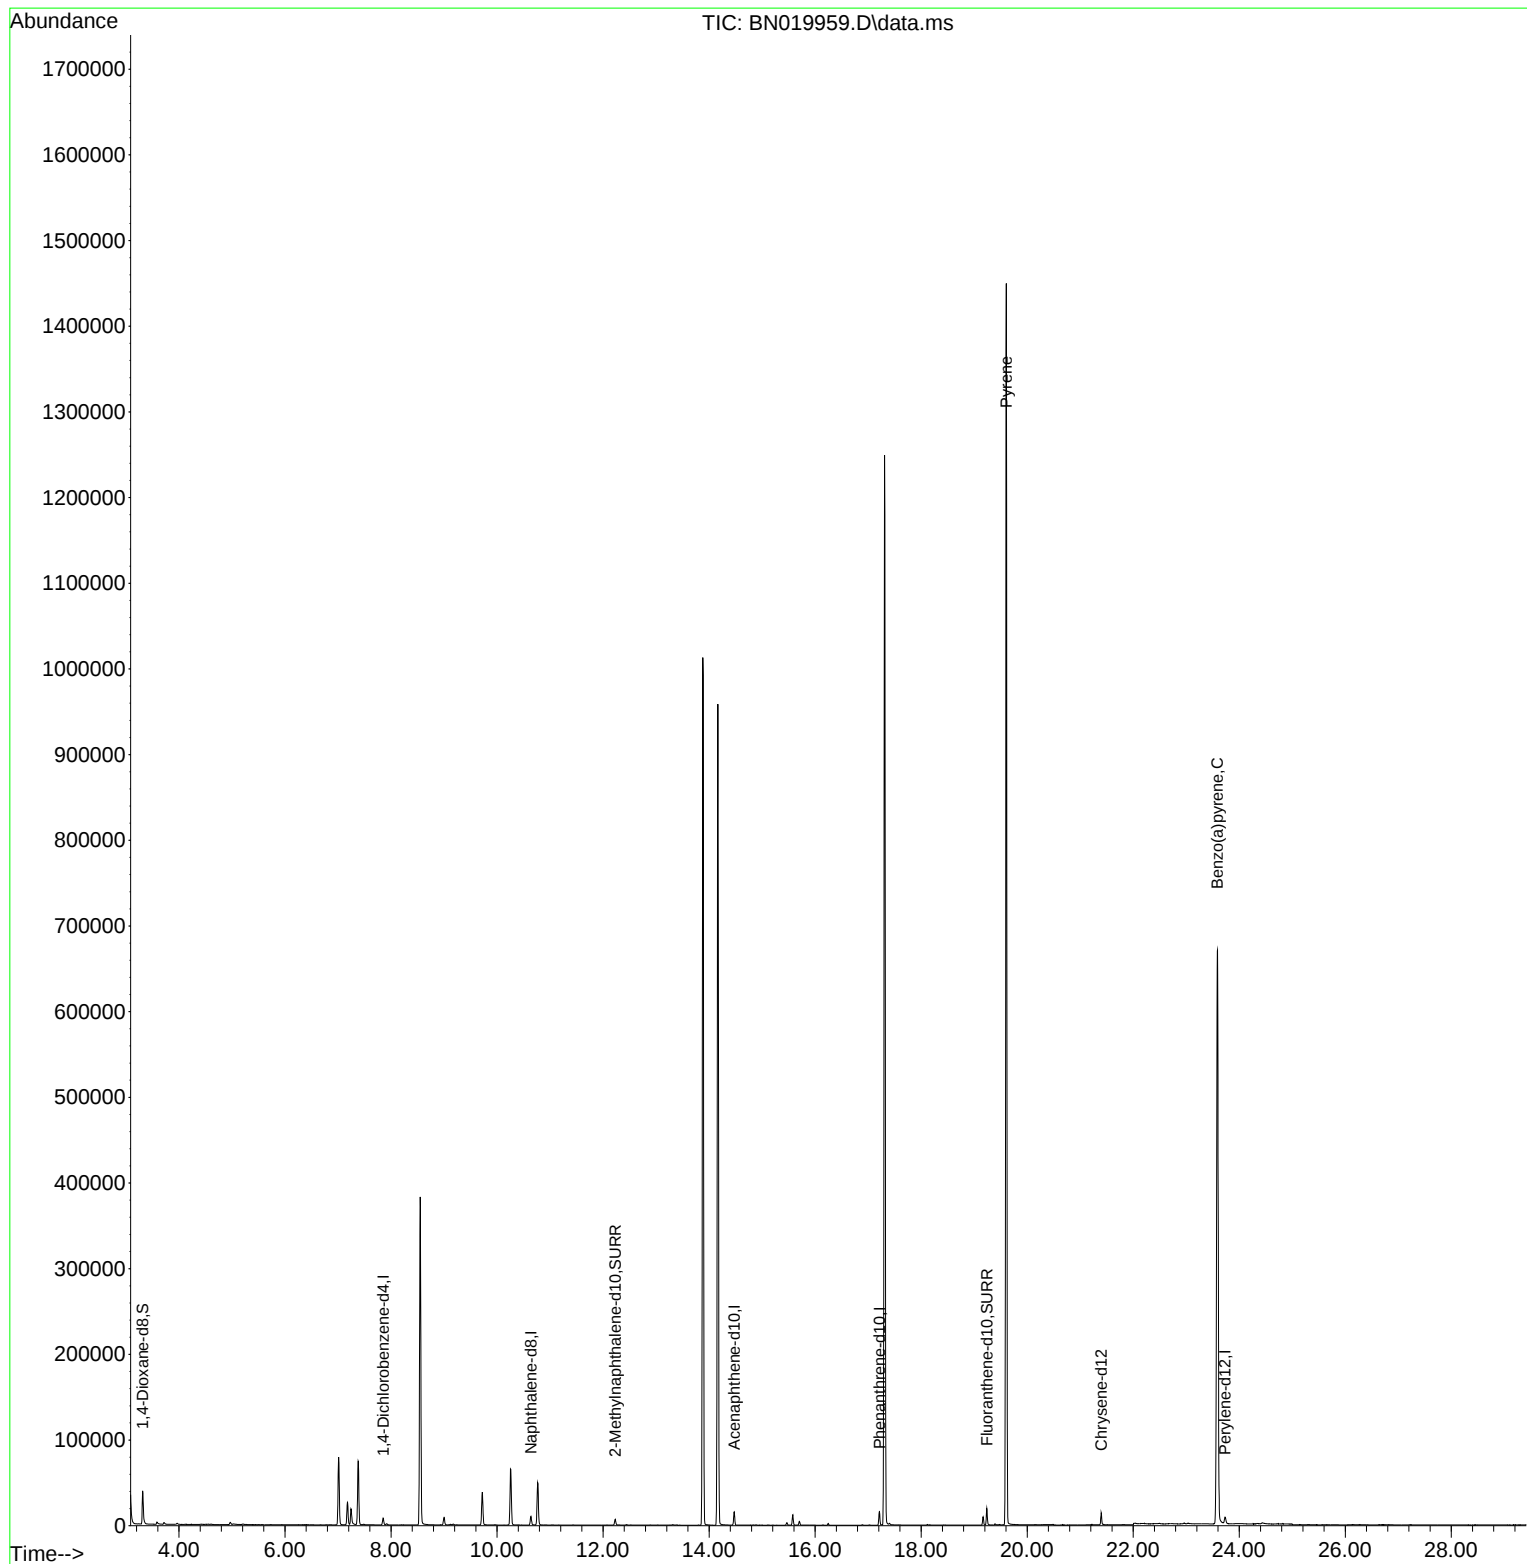

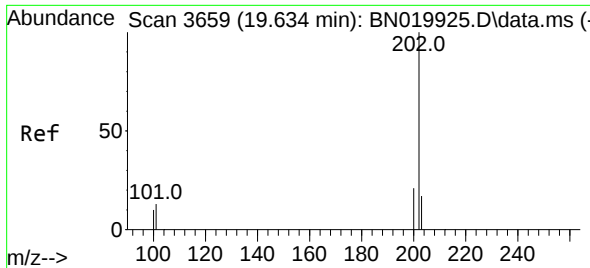

#20

Pyrene

Concen: 0.037 ng/ul

RT: 19.606 min Scan# 3

Delta R.T. -0.031 min

Lab File: BN019959.D

Acq: 25 May 2022 19:44

Instrument :

BNA_N

ClientSampleId :

EW4K9





Tgt Ion:202 Resp: 2449

Ion Ratio Lower Upper

202 100

101 168.8 11.4 17.0#

100 1191.9 9.0 13.4#

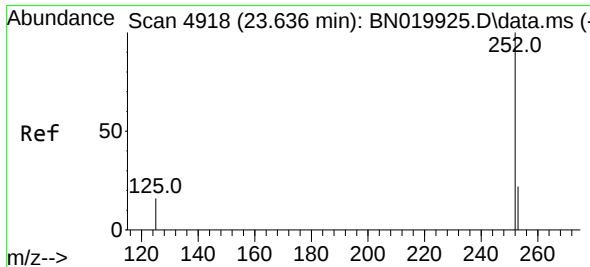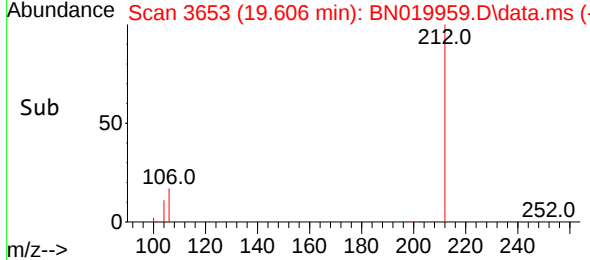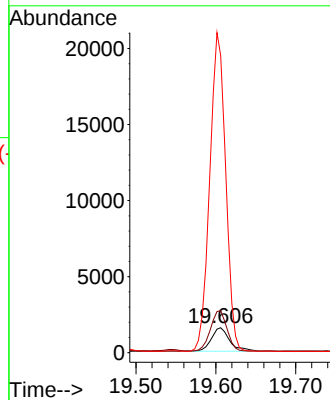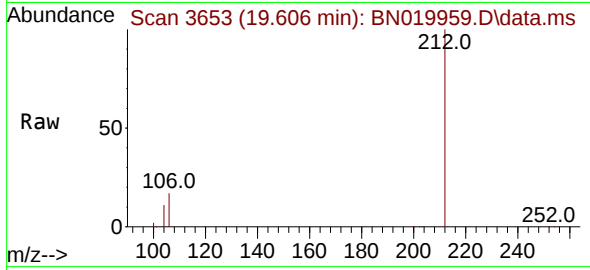

#26

Benzo(a)pyrene

Concen: 0.088 ng/ul

RT: 23.586 min Scan# 4901

Delta R.T. -0.053 min

Lab File: BN019959.D

Acq: 25 May 2022 19:44

Tgt Ion:252 Resp: 3966

Ion Ratio Lower Upper

252 100

253 41.2 23.4 35.0#

125 79.2 28.3 42.5#

