

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019962.D
 Acq On : 25 May 2022 21:32
 Operator : CG/JU
 Sample : N2883-08
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4K8

Quant Time: May 26 01:16:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3802	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	13501	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.474	164	8575	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.213	188	18089	0.400	ng/ul	0.00
17) Chrysene-d12	21.400	240	12694	0.400	ng/ul	0.00
23) Perylene-d12	23.738	264	10134	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	25653	7.237	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	9611	0.436	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	20921	0.461	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.606	202	2753	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.592	252	4134	0.098	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019962.D
Acq On : 25 May 2022 21:32
Operator : CG/JU
Sample : N2883-08
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4K8

Quant Time: May 26 01:16:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration




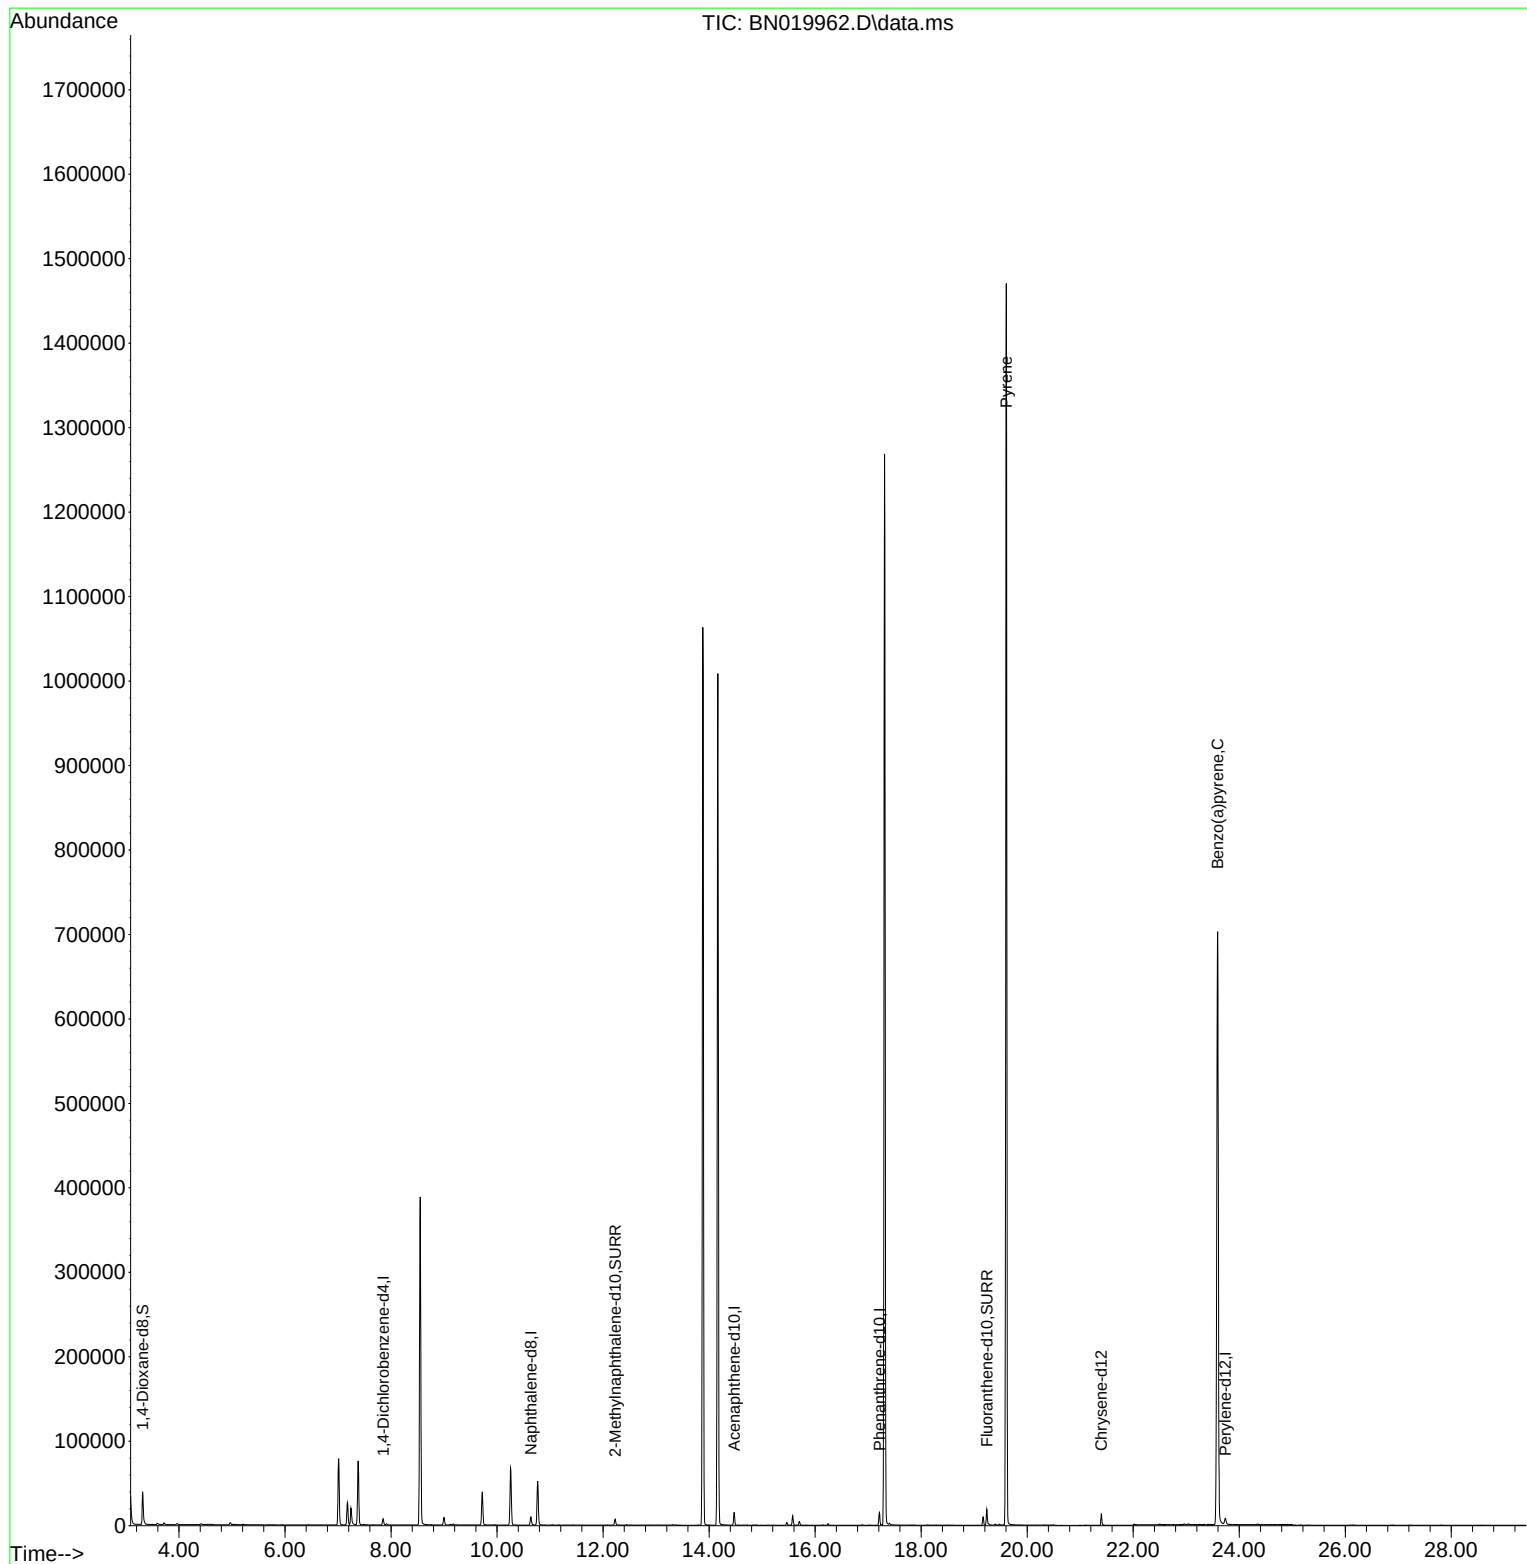


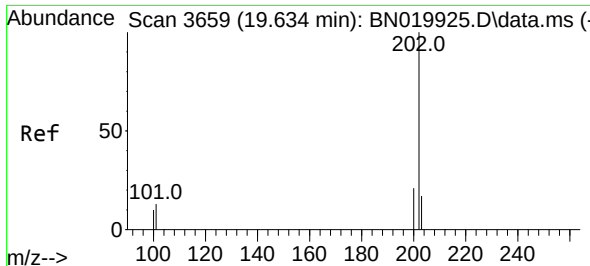

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.606 min Scan# 3653
Delta R.T. -0.031 min
Lab File: BN019962.D
Acq: 25 May 2022 21:32

Instrument :
BNA_N
ClientSampleId :
EW4K8

Tgt Ion:202 Resp: 2753
Ion Ratio Lower Upper
202 100
101 173.6 11.4 17.0#
100 1252.4 9.0 13.4#

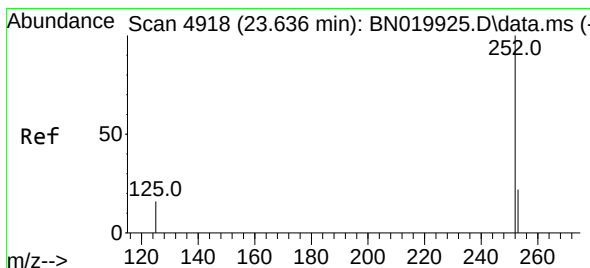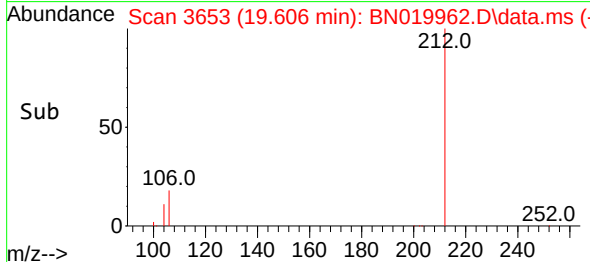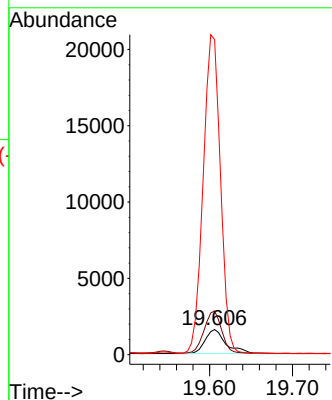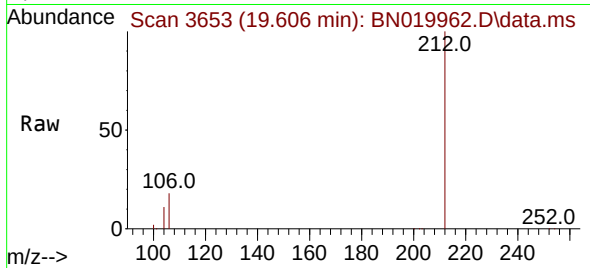

#26
Benzo(a)pyrene
Concen: 0.098 ng/ul
RT: 23.592 min Scan# 4903
Delta R.T. -0.047 min
Lab File: BN019962.D
Acq: 25 May 2022 21:32

Tgt Ion:252 Resp: 4134
Ion Ratio Lower Upper
252 100
253 39.8 23.4 35.0#
125 39.4 28.3 42.5

