

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019963.D
 Acq On : 25 May 2022 22:08
 Operator : CG/JU
 Sample : N2883-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4K4

Quant Time: May 26 01:16:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4155	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	14688	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.474	164	9803	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.209	188	20158	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240	13920	0.400	ng/ul	0.00
23) Perylene-d12	23.738	264	11180	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	48226	12.449	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	16693	0.696	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	35428	0.712	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.606	202	4308	0.061	ng/ul#	1
26) Benzo(a)pyrene	23.592	252	6395	0.137	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019963.D
Acq On : 25 May 2022 22:08
Operator : CG/JU
Sample : N2883-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4K4

Quant Time: May 26 01:16:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration




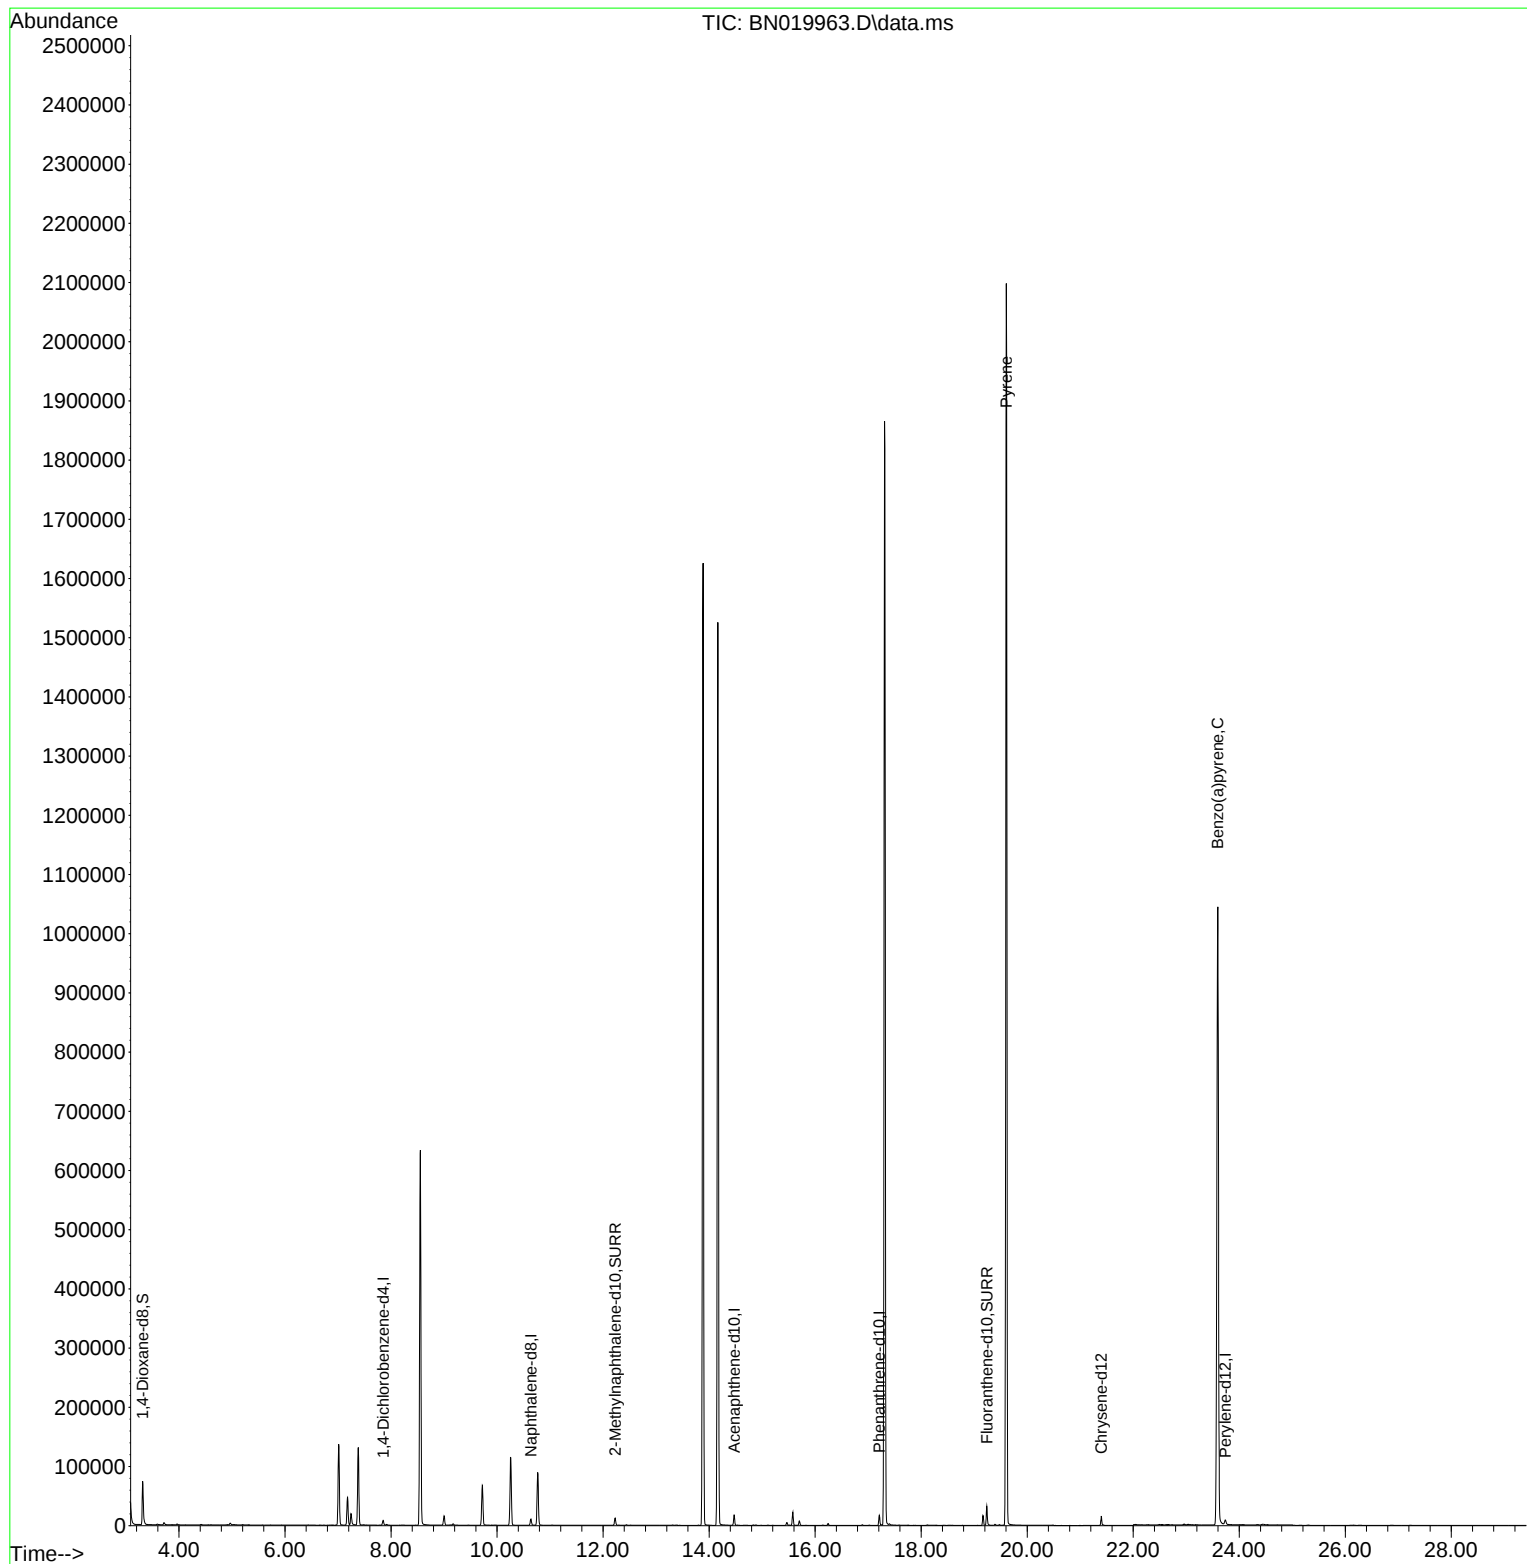


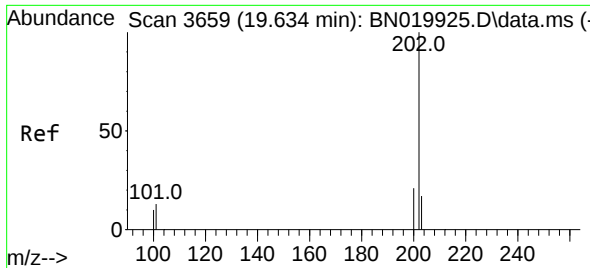

#20
Pyrene
Concen: 0.061 ng/ul
RT: 19.606 min Scan# 30
Delta R.T. -0.031 min
Lab File: BN019963.D
Acq: 25 May 2022 22:08

Instrument :
BNA_N
ClientSampleId :
EW4K4

Tgt Ion:202 Resp: 4308
Ion Ratio Lower Upper
202 100
101 177.8 11.4 17.0#
100 1336.8 9.0 13.4#

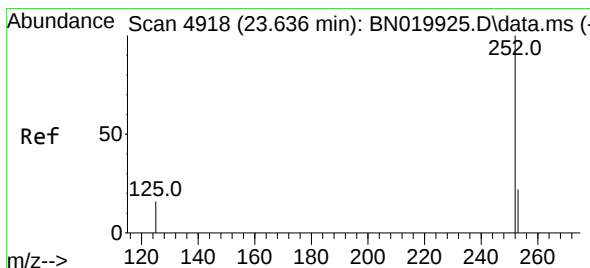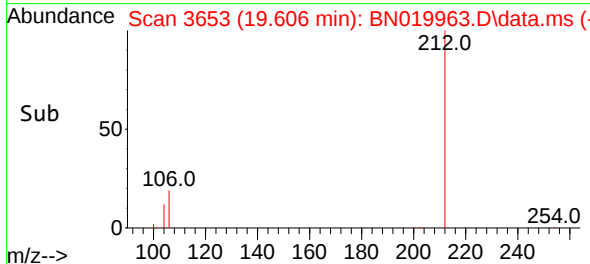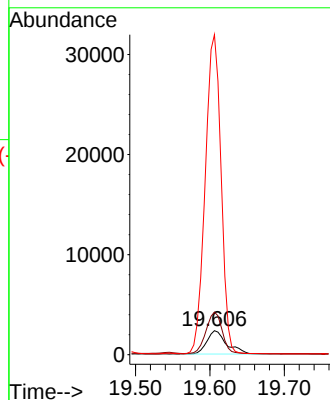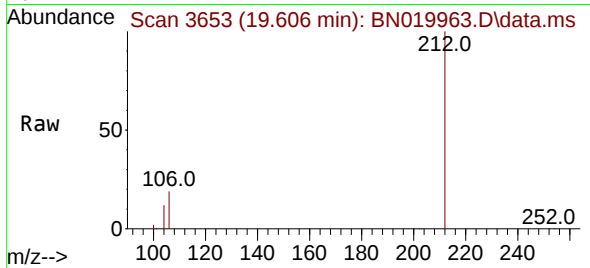

#26
Benzo(a)pyrene
Concen: 0.137 ng/ul
RT: 23.592 min Scan# 4903
Delta R.T. -0.047 min
Lab File: BN019963.D
Acq: 25 May 2022 22:08

Tgt Ion:252 Resp: 6395
Ion Ratio Lower Upper
252 100
253 36.7 23.4 35.0#
125 38.1 28.3 42.5

