




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019934.D
 Acq On : 24 May 2022 22:56
 Operator : CG/JU
 Sample : N2950-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBTE2

Manual IntegrationsAPPROVED

Quant Time: May 25 08:39:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :mohammad ahmed 05/27/2022

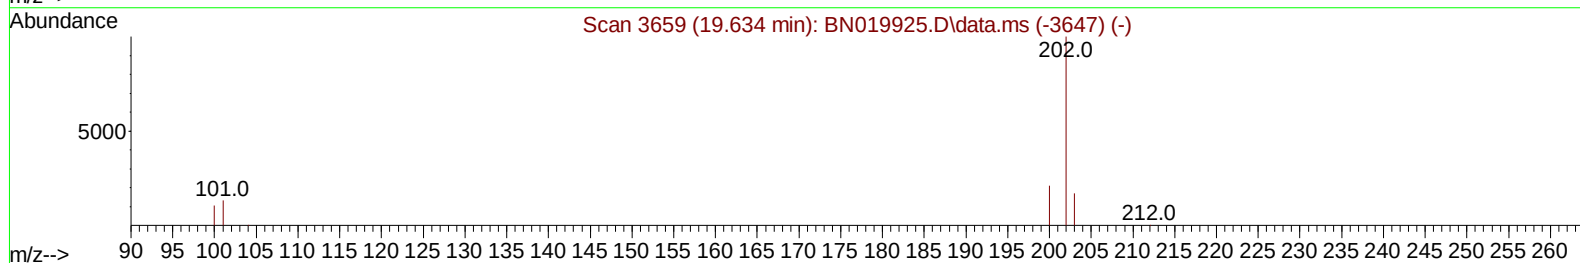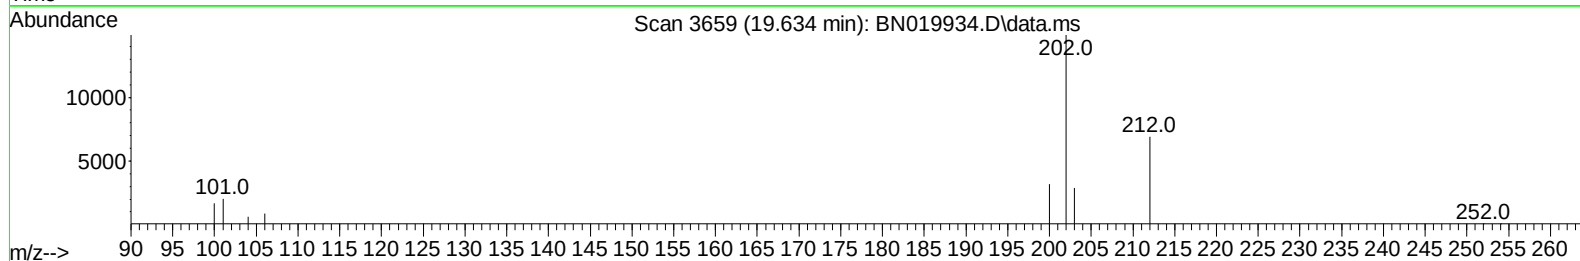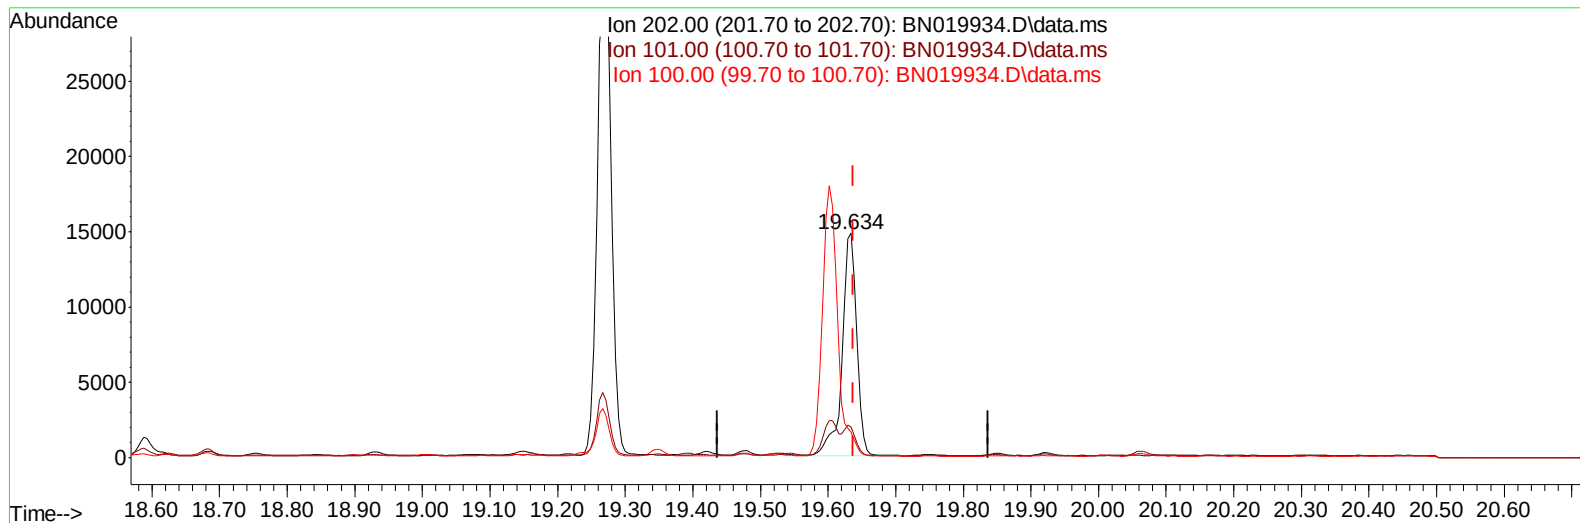

TIC: BN019934.D\data.ms

(20) Pyrene

19.634min (-0.003) 0.32 ng/u1

response 21872

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	13.52
100.00	11.20	11.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019934.D
 Acq On : 24 May 2022 22:56
 Operator : CG/JU
 Sample : N2950-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBTE2

Manual IntegrationsAPPROVED

Quant Time: May 25 08:39:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :mohammad ahmed 05/27/2022

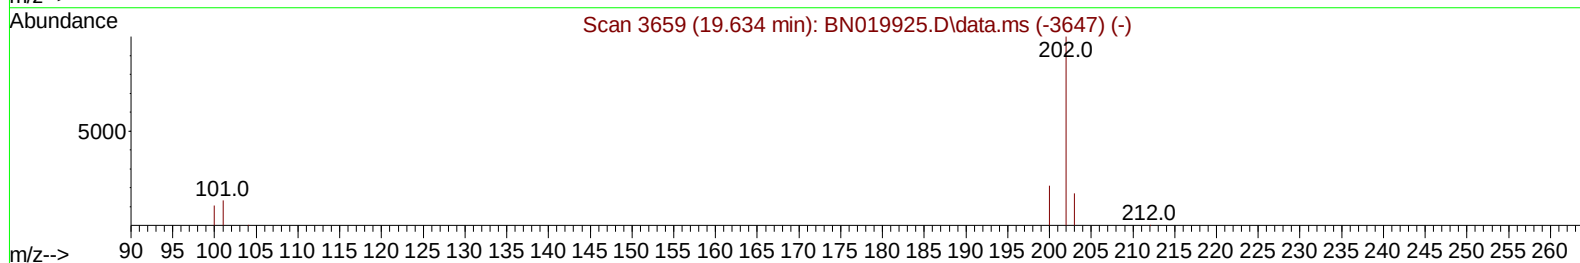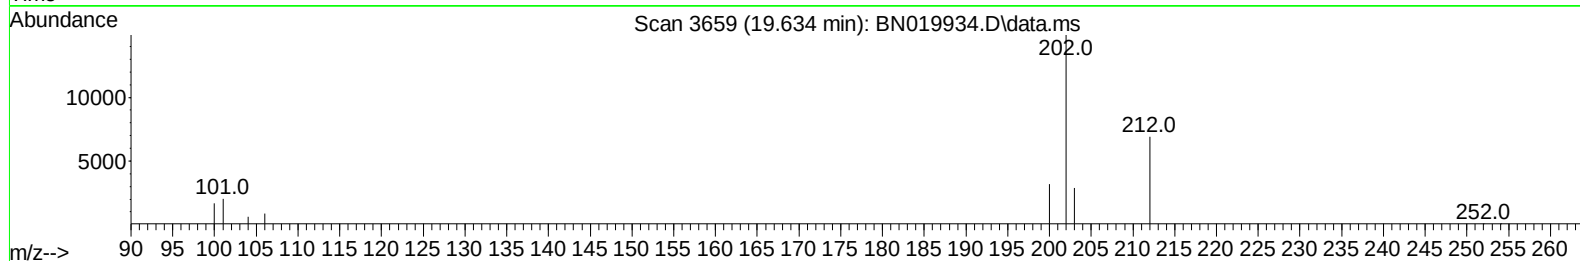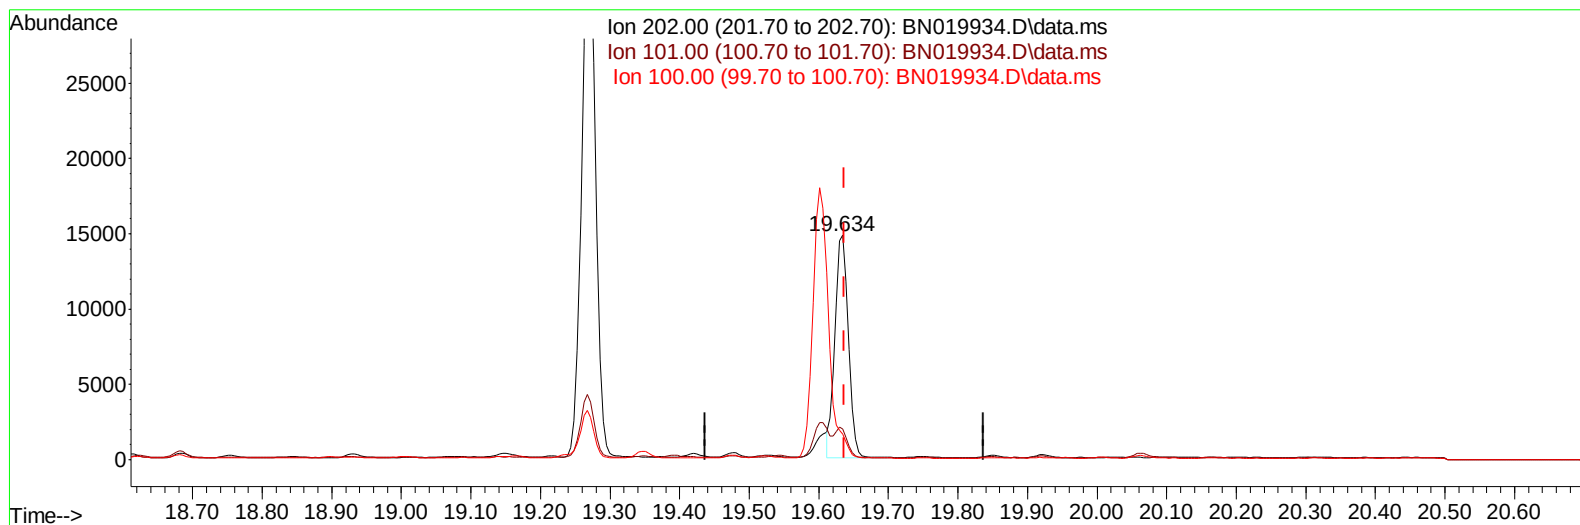

TIC: BN019934.D\data.ms

(20) Pyrene

19.634min (-0.003) 0.29 ng/ul m

response 20006

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.20	13.52
100.00	11.20	11.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019934.D
 Acq On : 24 May 2022 22:56
 Operator : CG/JU
 Sample : N2950-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBTE2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/25/2022
 Supervised By :mohammad ahmed 05/27/2022

Quant Time: May 25 08:39:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.851	152		3600	0.400	ng/ul	0.00
4) Naphthalene-d8	10.650	136		12254	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.474	164		9784	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.213	188		17132	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240		13674	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264		10838	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.315	96		14684	4.375	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152		7105	0.355	ng/ul	0.00
18) Fluoranthene-d10	19.239	212		16475	0.337	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.722	128	16598493	431.891	ng/ul		100
7) 2-Methylnaphthalene	12.306	142	1702564	66.856	ng/ul#		100
8) 1-Methylnaphthalene	12.520	142	1399630	59.038	ng/ul#		100
10) Acenaphthylene	14.192	152	184847	3.315	ng/ul		99
11) Acenaphthene	14.539	153	1803086	47.726	ng/ul		99
12) Fluorene	15.520	166	804440	19.042	ng/ul		99
14) Pentachlorophenol	16.867	266	52558	18.419	ng/ul		90
15) Phenanthrene	17.251	178	469000	7.785	ng/ul		99
16) Anthracene	17.344	178	53142	0.941	ng/ul		99
19) Fluoranthene	19.267	202	49003	0.718	ng/ul		100
20) Pyrene	19.634	202	20006m	0.289	ng/ul		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019934.D
Acq On : 24 May 2022 22:56
Operator : CG/JU
Sample : N2950-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBTE2

Manual IntegrationsAPPROVED

Quant Time: May 25 08:39:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/25/2022
Supervised By :mohammad ahmed 05/27/2022

