

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
 Data File : BN019947.D
 Acq On : 25 May 2022 12:33
 Operator : CG/JU
 Sample : N2950-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBTD1

Quant Time: May 26 01:15:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 23 14:58:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3807	0.400	ng/ul	0.00
4) Naphthalene-d8	10.639	136	13221	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.474	164	8038	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.209	188	16669	0.400	ng/ul	0.00
17) Chrysene-d12	21.397	240	11076	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	9282	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	17102	4.818	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.229	152	6520	0.302	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	15532	0.392	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.867	266	552	0.199	ng/ul	87
16) Anthracene	17.344	178	3650	0.066	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052422\
Data File : BN019947.D
Acq On : 25 May 2022 12:33
Operator : CG/JU
Sample : N2950-11
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBTD1

Quant Time: May 26 01:15:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN052322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 23 14:58:28 2022
Response via : Initial Calibration

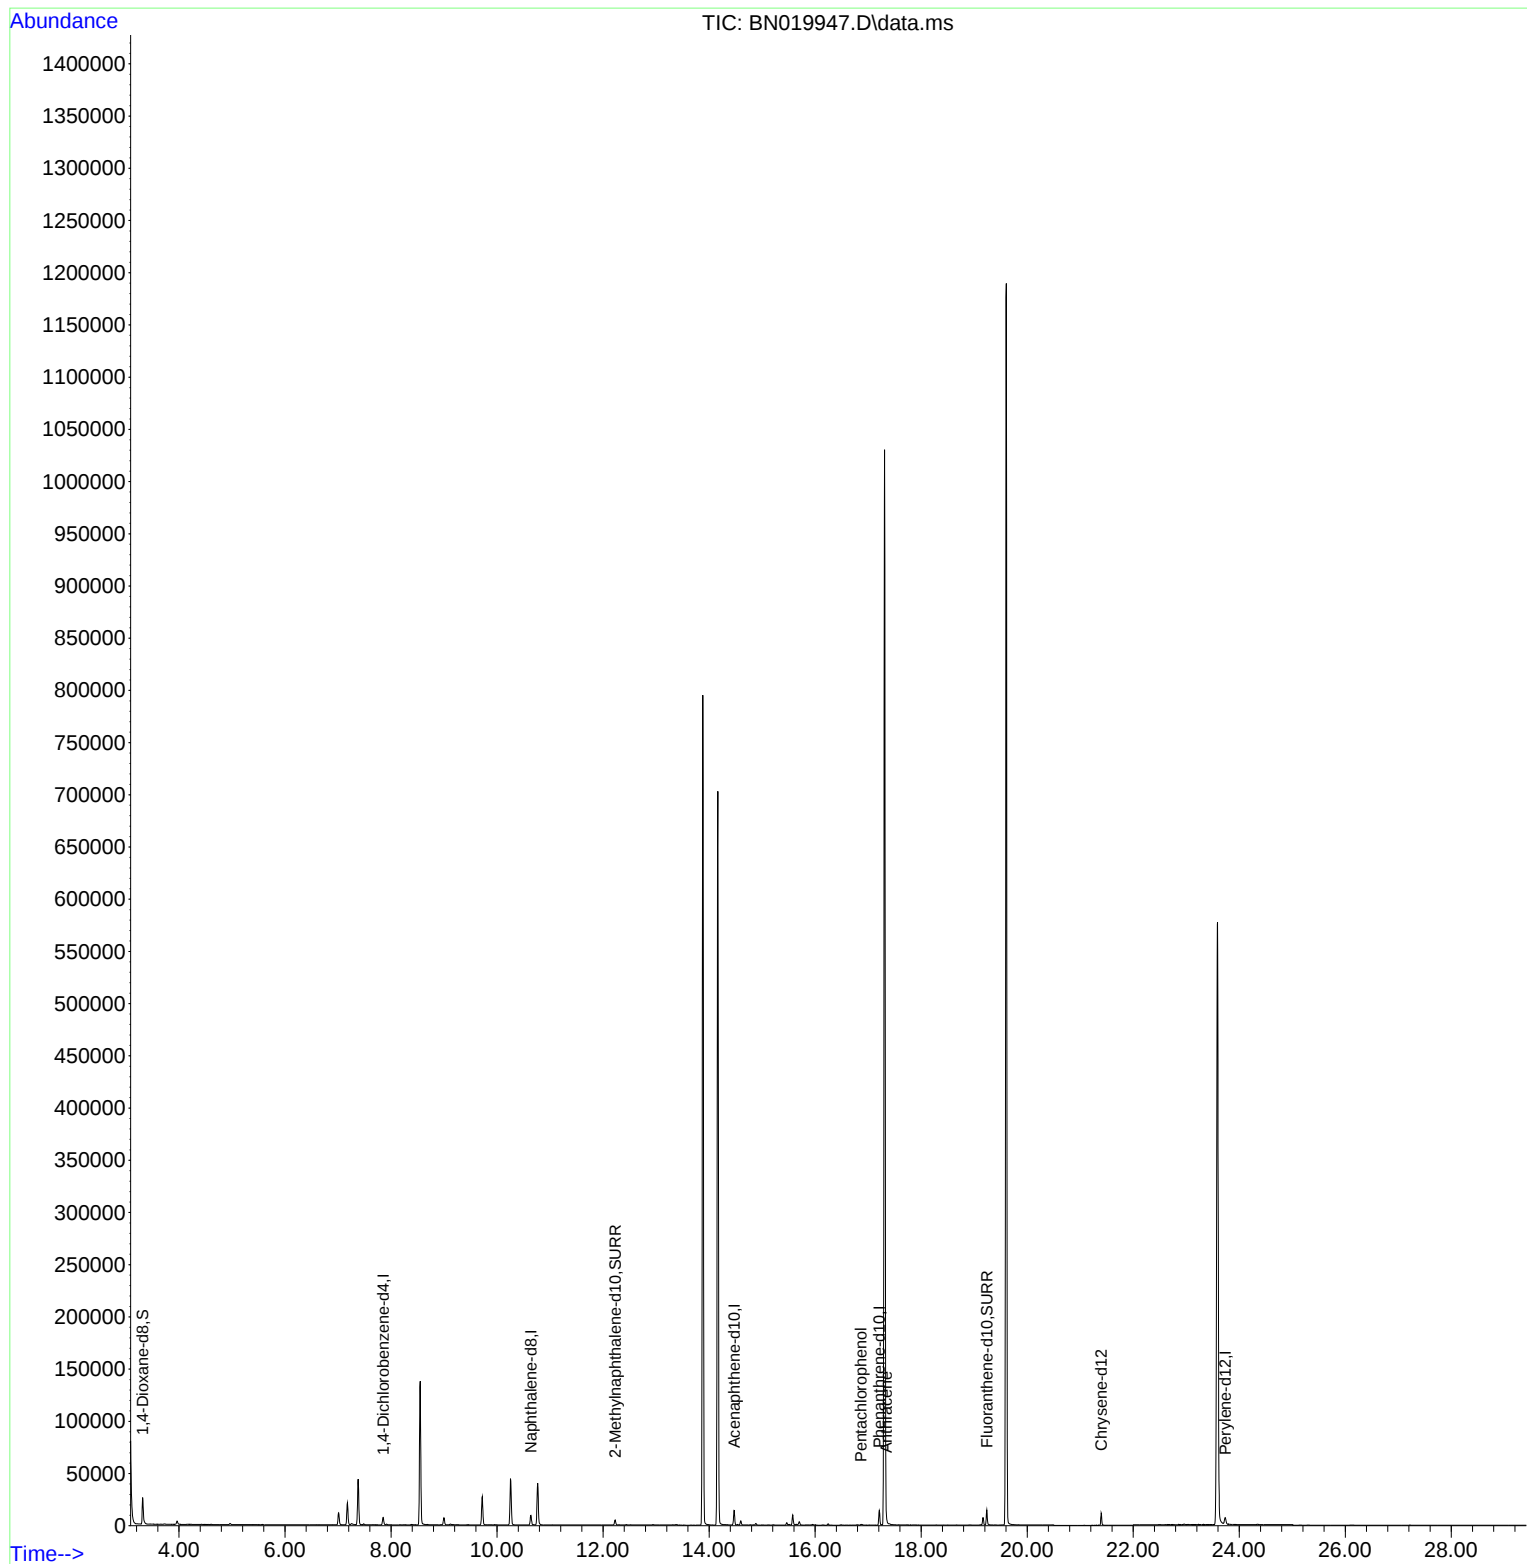




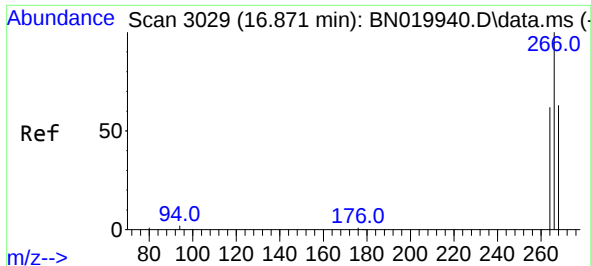


#14
 Pentachlorophenol
 Concen: 0.199 ng/ul
 RT: 16.867 min Scan# 3029
 Delta R.T. -0.007 min
 Lab File: BN019947.D
 Acq: 25 May 2022 12:33

Instrument :
 BNA_N
 ClientSampleId :
 DBTD1

Tgt Ion: 266 Resp: 552

Ion	Ratio	Lower	Upper
266	100		
264	65.4	44.9	67.3
268	64.9	44.6	67.0

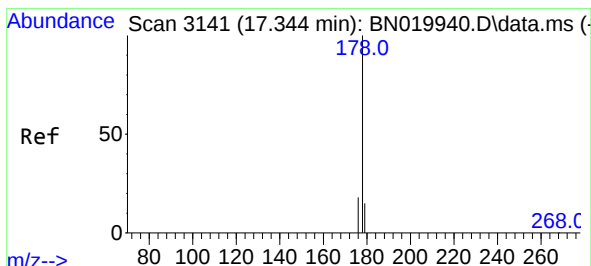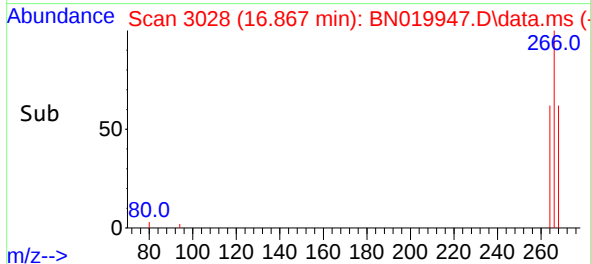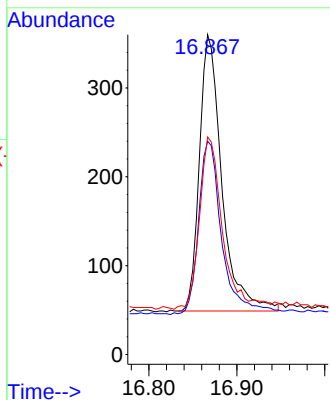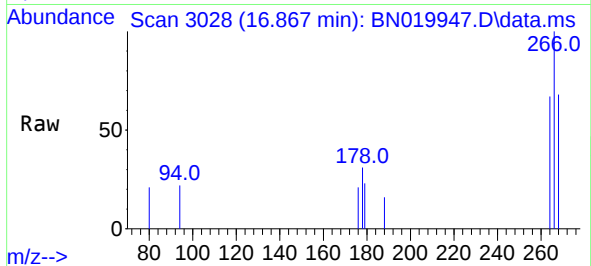

#16
 Anthracene
 Concen: 0.066 ng/ul
 RT: 17.344 min Scan# 3141
 Delta R.T. -0.003 min
 Lab File: BN019947.D
 Acq: 25 May 2022 12:33

Tgt Ion: 178 Resp: 3650

Ion	Ratio	Lower	Upper
178	100		
179	17.5	13.1	19.7
176	20.6	15.3	22.9

