


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052721\
 Data File : BN014784.D
 Acq On : 27 May 2021 09:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN052621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 01:39:07 2021

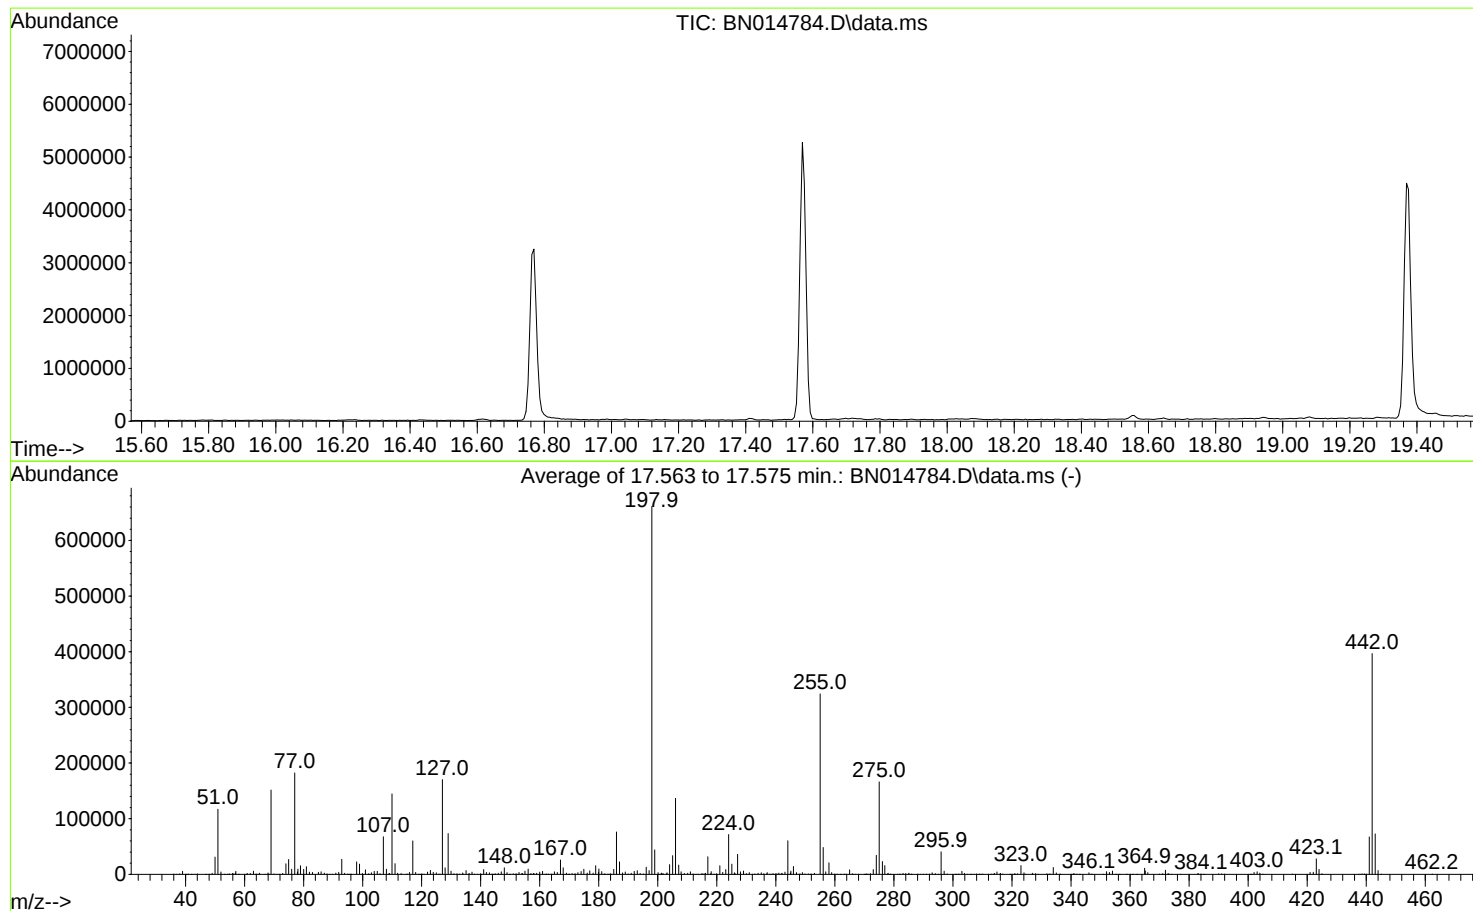

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.7	116939	PASS
68	69	0.00	2	1.7	2650	PASS
69	198	0.00	100	22.9	151532	PASS
70	69	0.00	2	0.5	771	PASS
127	198	10	80	25.7	170112	PASS
197	198	0.00	2	1.1	6967	PASS
198	198	100	100	100.0	660885	PASS
199	198	5	9	6.7	44123	PASS
275	198	10	60	25.2	166251	PASS
365	198	1	100	1.7	11008	PASS
441	198	0.01	100	10.2	67157	PASS
442	442	50	100	100.0	396587	PASS
443	442	15	24	18.3	72760	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/27/2021	BNA_N	<u>BN014784.D</u>
Compound Name	Response	Retention Time
DDT	1575107	20.61
DDD	14853	20.17
DDE	3647	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18500	1593607	1.16

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052721\
 Data File : BN014784.D
 Acq On : 27 May 2021 09:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 27 11:03:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

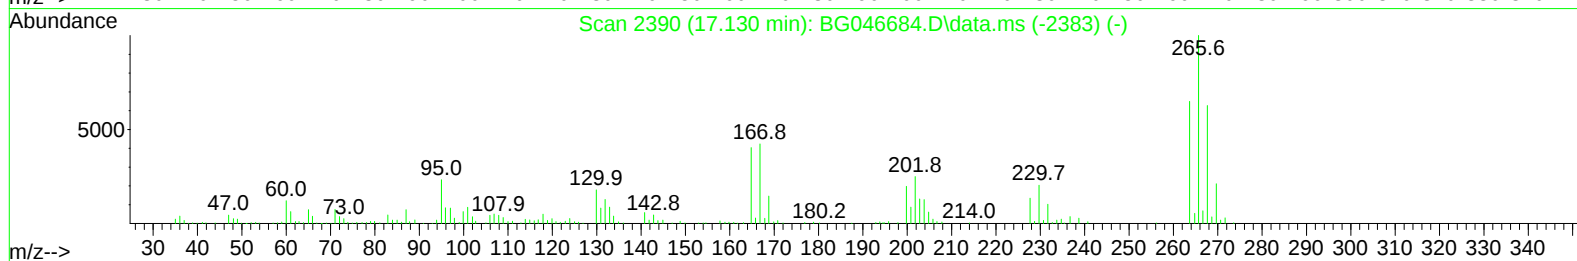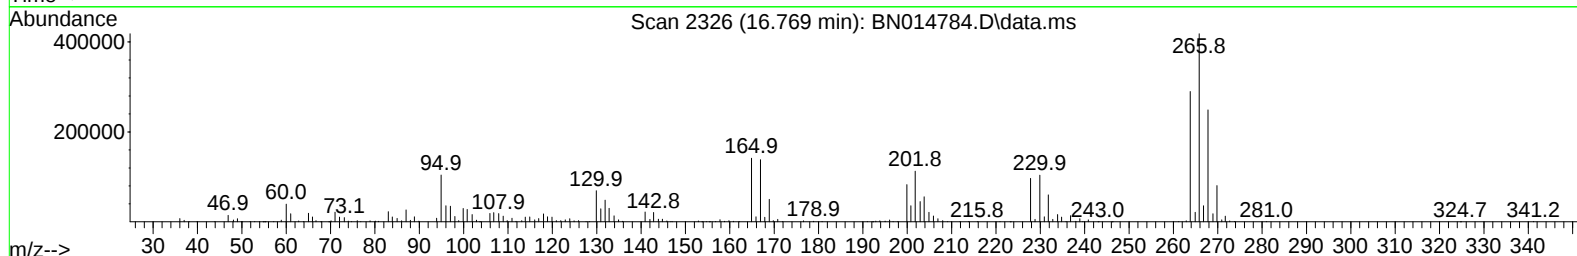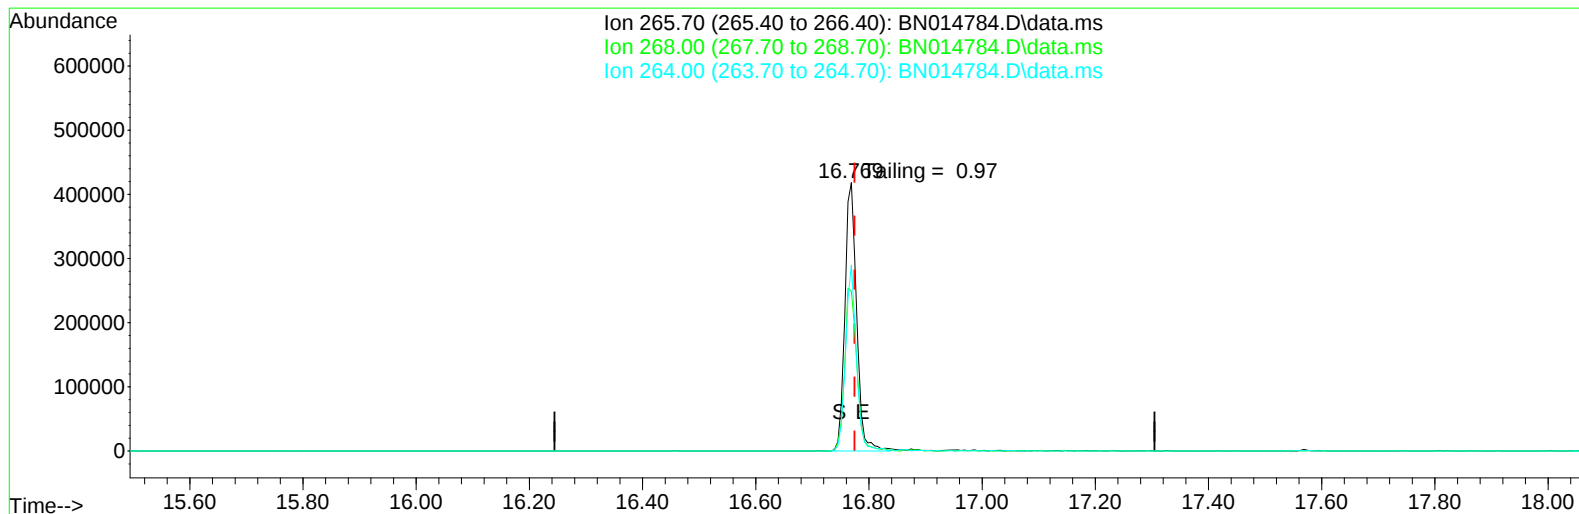

TIC: BN014784.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 17693.16 ng




response 604976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.50
264.00	61.60	69.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052721\
Data File : BN014784.D
Acq On : 27 May 2021 09:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 27 11:03:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

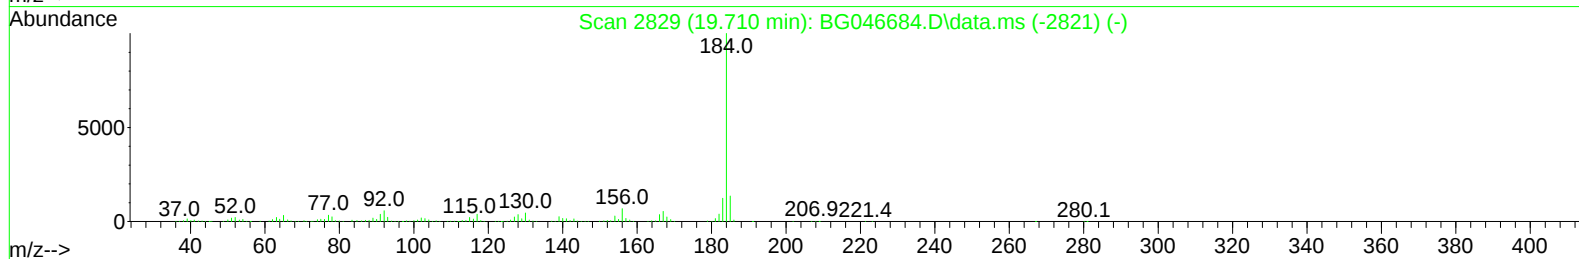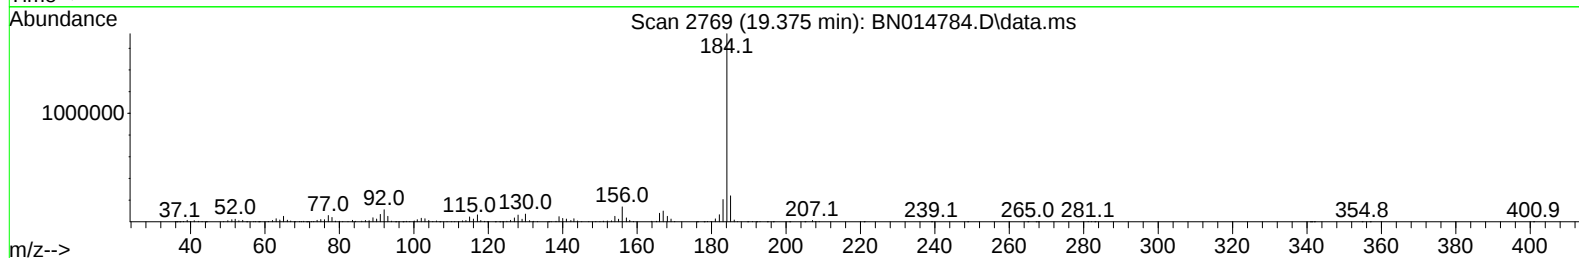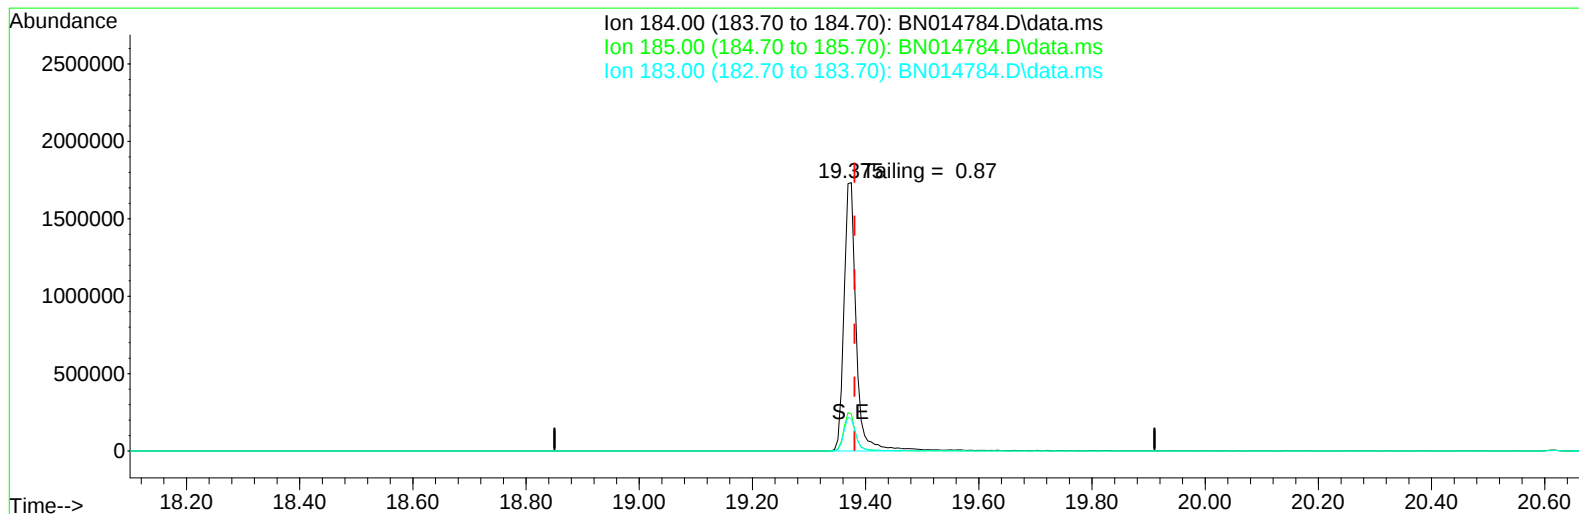

TIC: BN014784.D\data.ms

(77) Benzidine

19.375min (-0.006) 579305.30 ng

response 2607166

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.81
183.00	13.20	11.88
0.00	0.00	0.00