
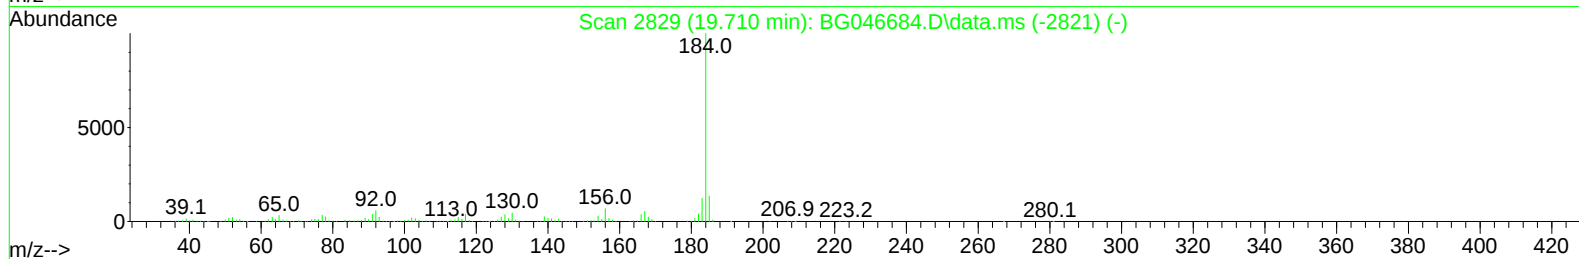
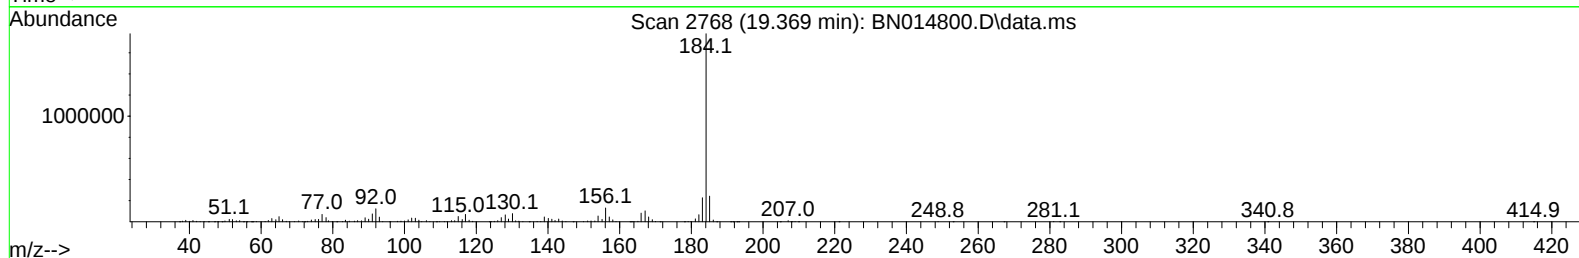


Quant Time: May 28 11:03:27 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

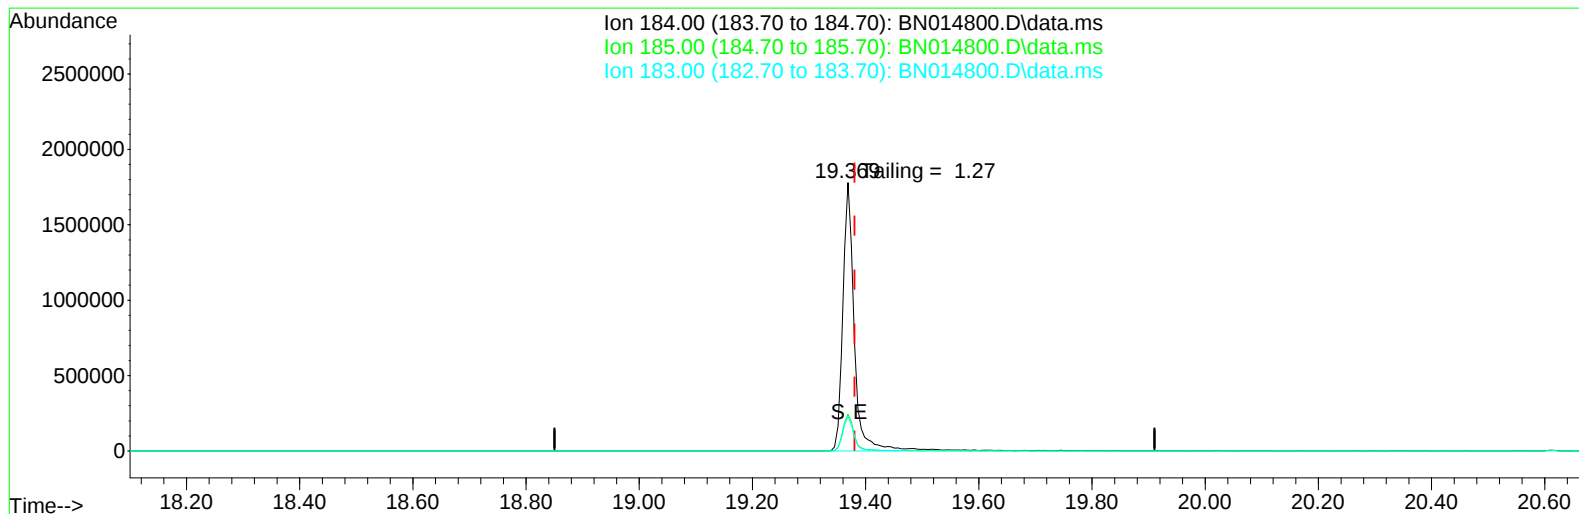

TIC: BN014800.D\data.ms

(77) Benzidine




19.369min (-0.011) 602896.46 ng

response **2453155**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.65
183.00	13.20	12.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052821\
 Data File : BN014800.D
 Acq On : 28 May 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 11:03:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

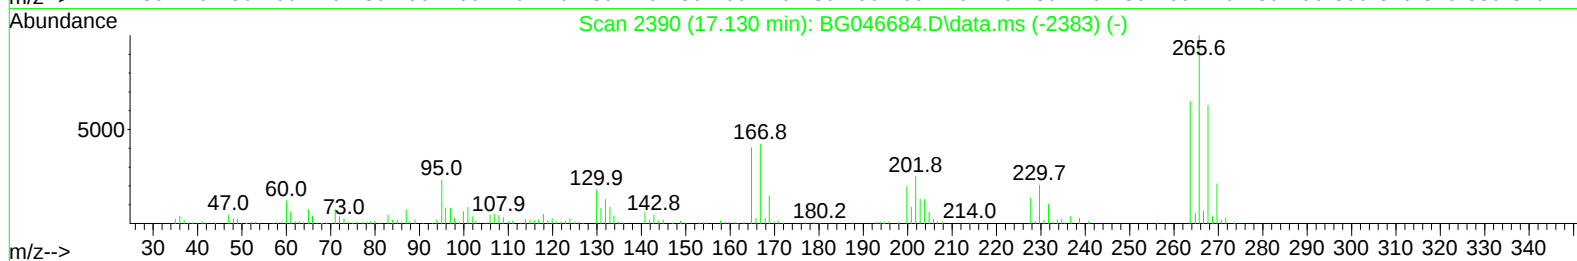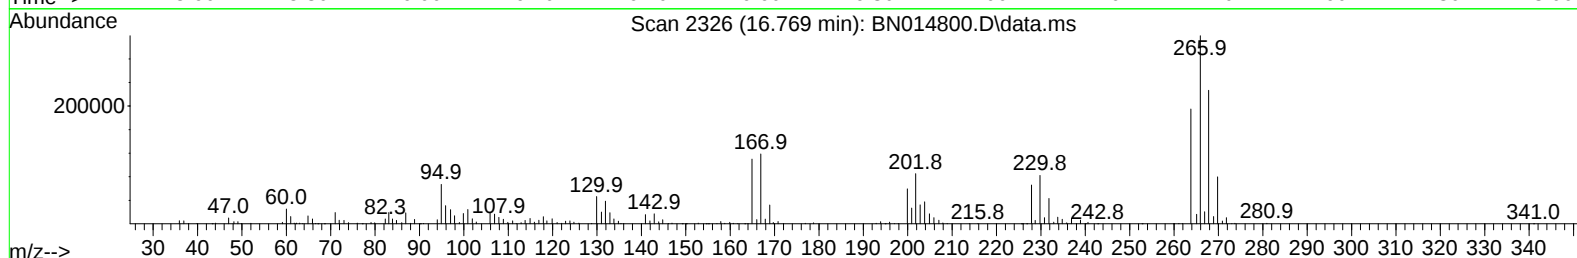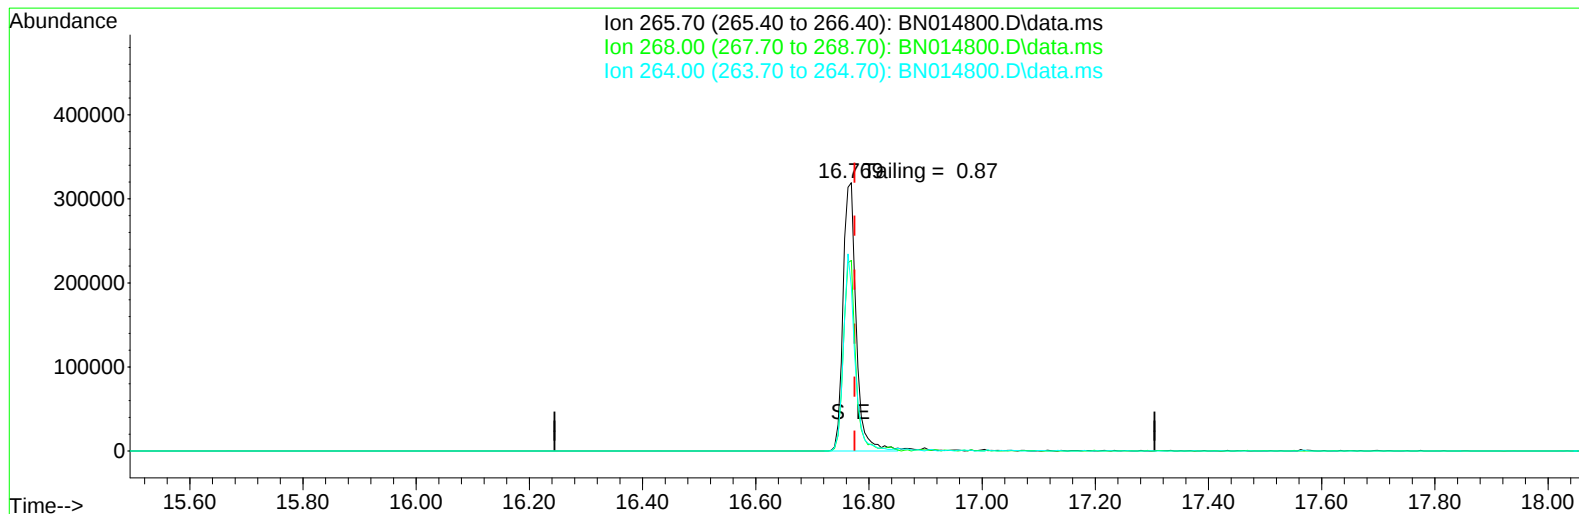

TIC: BN014800.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 16509.36 ng

response 517079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.02
264.00	61.60	61.03
0.00	0.00	0.00