
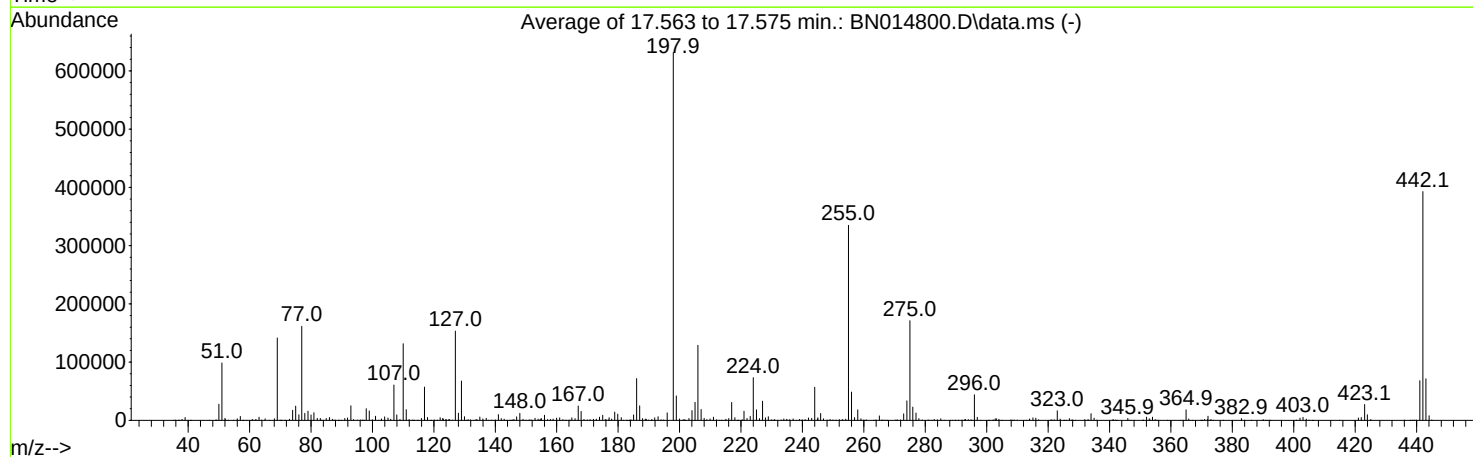


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052821\
 Data File : BN014800.D
 Acq On : 28 May 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN052621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 27 01:39:07 2021

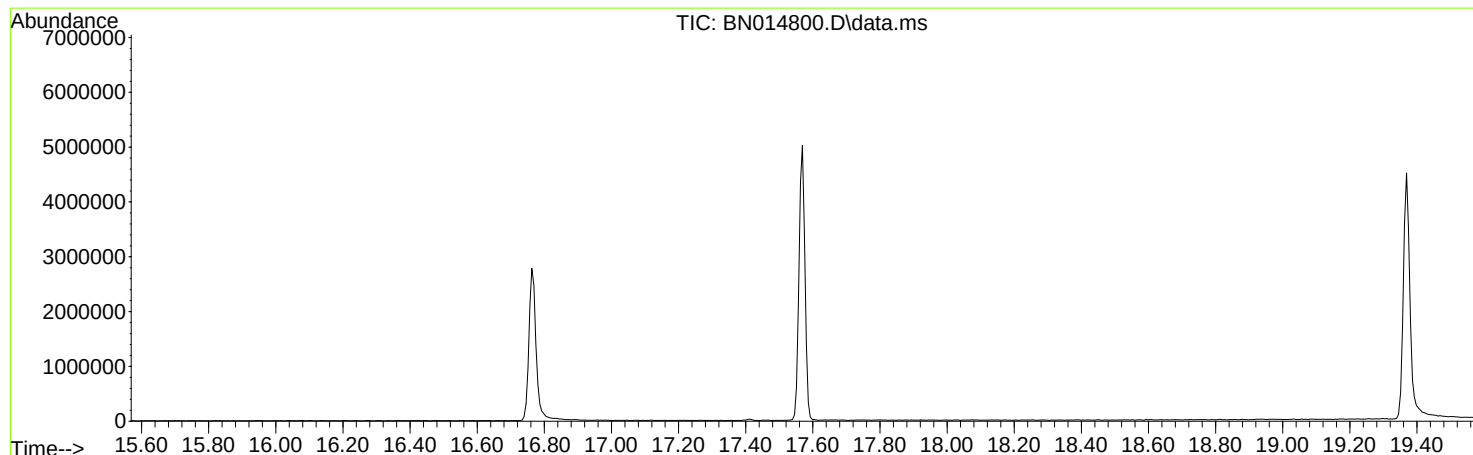

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.6	98617	PASS
68	69	0.00	2	1.9	2745	PASS
69	198	0.00	100	22.4	141544	PASS
70	69	0.00	2	0.5	701	PASS
127	198	10	80	24.3	153320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	631637	PASS
199	198	5	9	6.6	41952	PASS
275	198	10	60	27.1	171307	PASS
365	198	1	100	2.9	18046	PASS
441	198	0.01	100	10.8	68285	PASS
442	442	50	100	100.0	393003	PASS
443	442	15	24	18.2	71573	PASS

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/28/2021	BNA_N	<u>BN014800.D</u>
Compound Name	Response	Retention Time
DDT	1630637	20.61
DDD	20925	20.17
DDE	3248	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24173	1654810	1.46

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052821\
 Data File : BN014800.D
 Acq On : 28 May 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 28 11:03:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

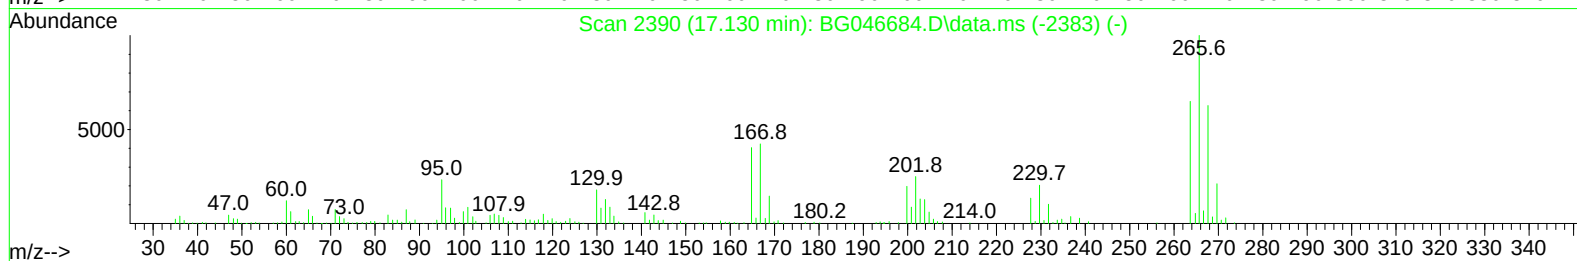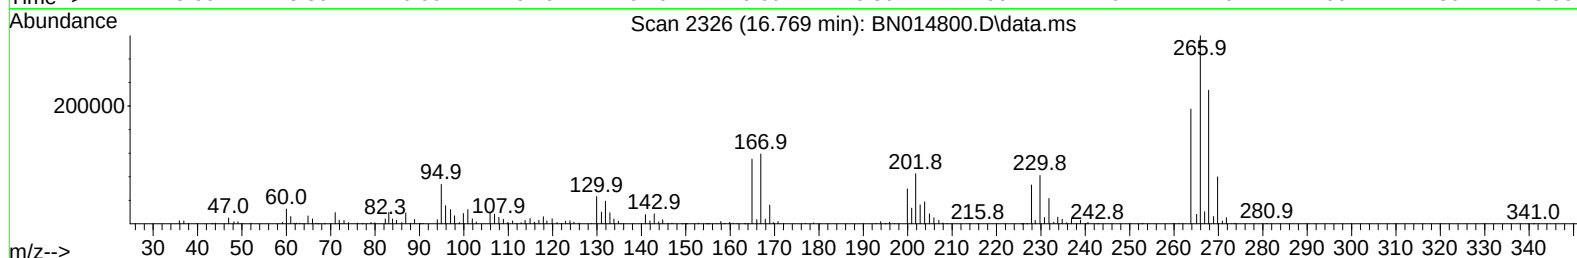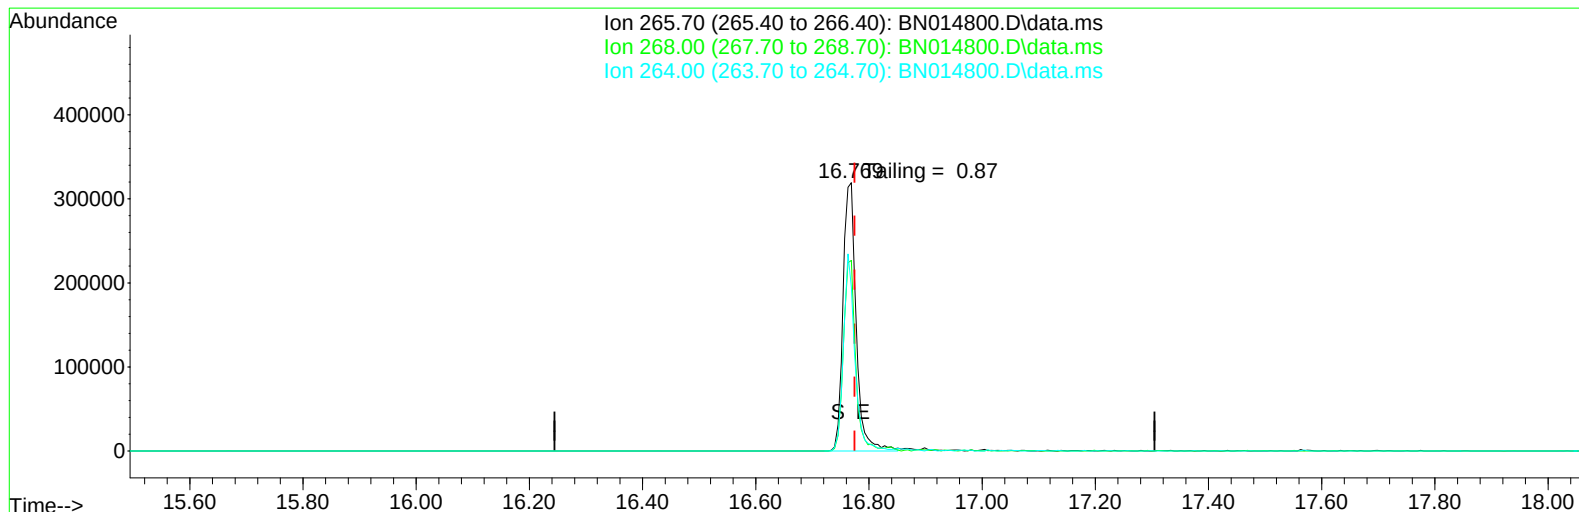

TIC: BN014800.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 16509.36 ng




response 517079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.02
264.00	61.60	61.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052821\
 Data File : BN014800.D
 Acq On : 28 May 2021 09:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 28 11:03:27 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

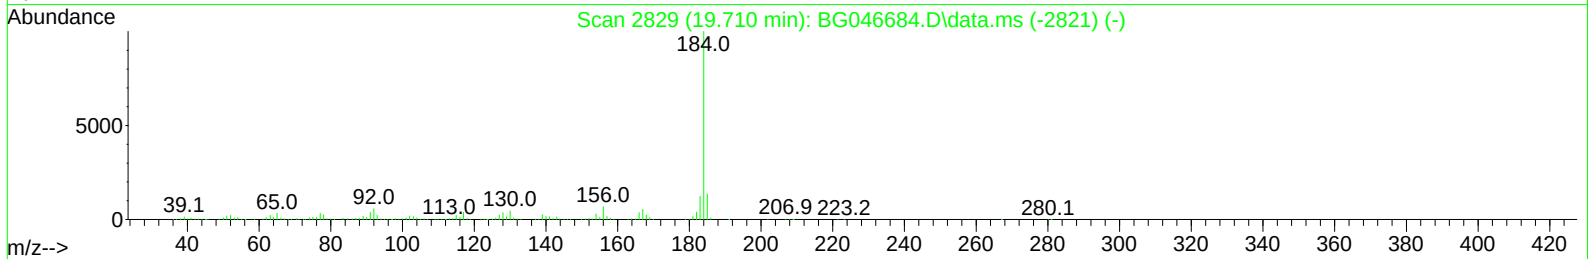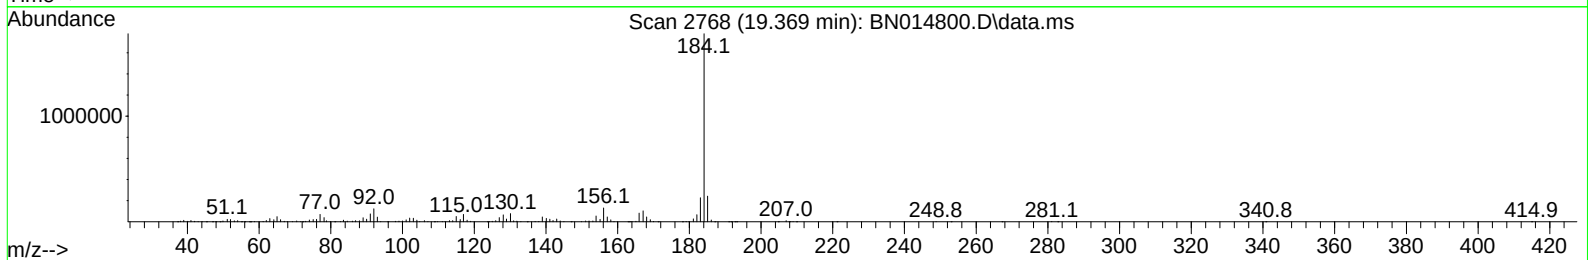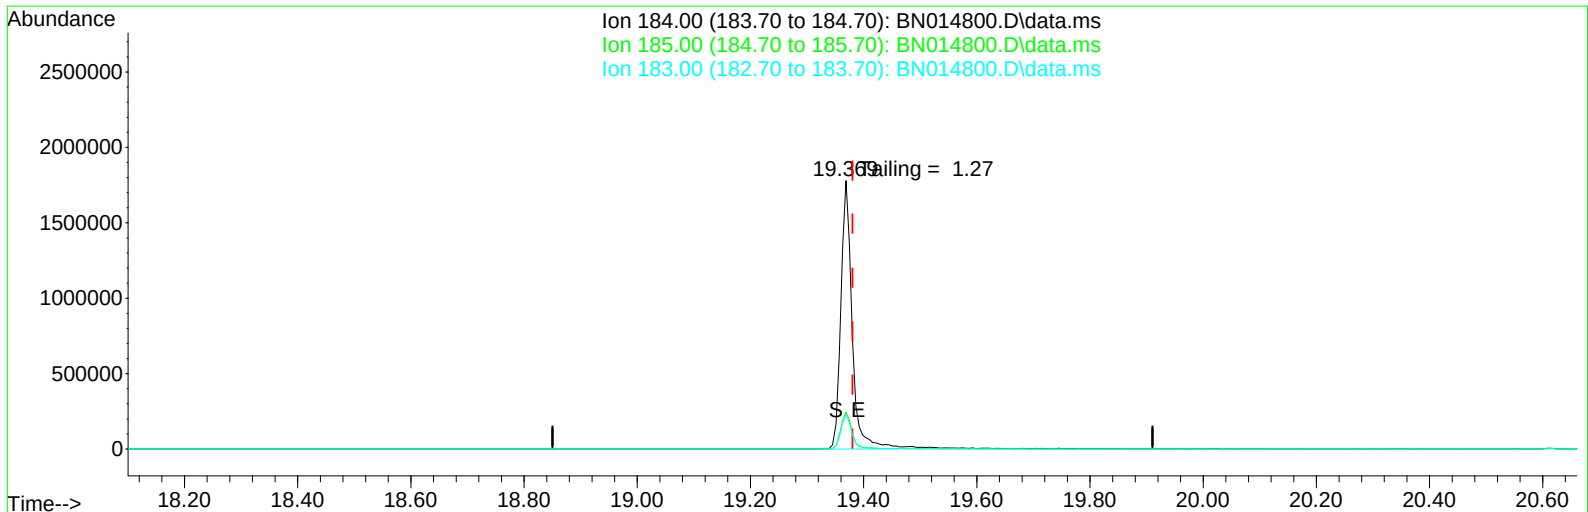

TIC: BN014800.D\data.ms

(77) Benzidine

19.369min (-0.011) 602896.46 ng

response 2453155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.65
183.00	13.20	12.82
0.00	0.00	0.00