
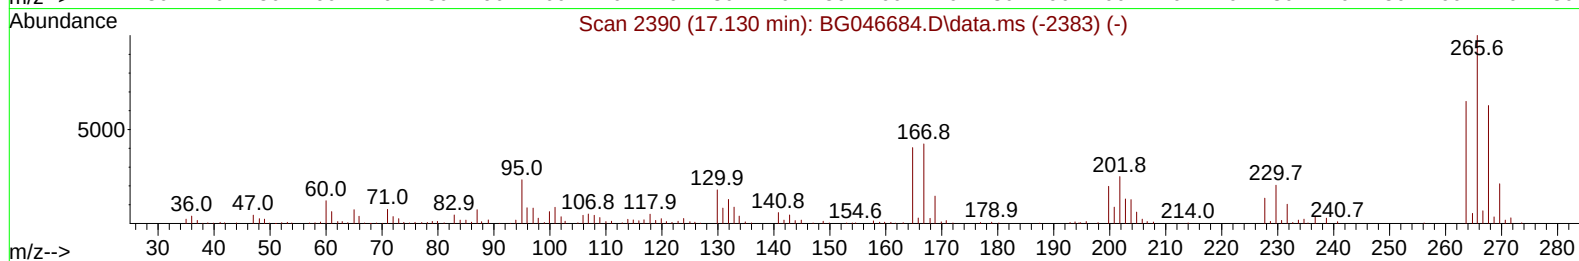
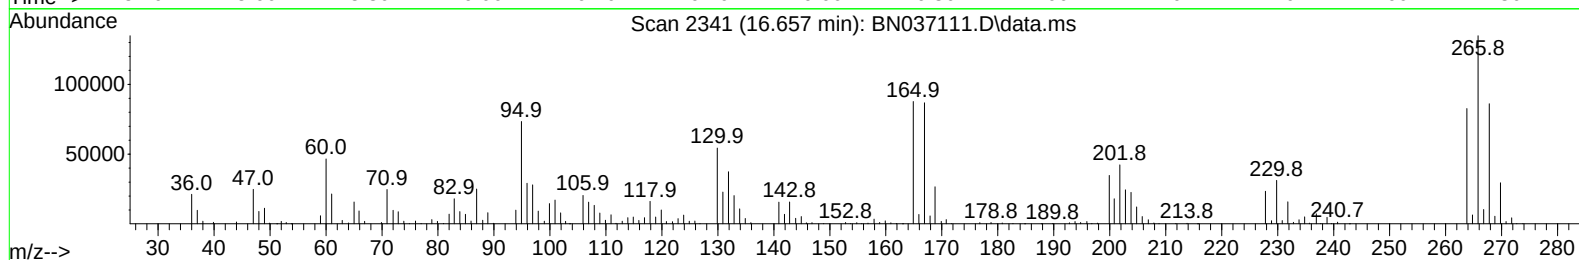


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052825\
Data File : BN037111.D
Acq On : 28 May 2025 16:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 17:56:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

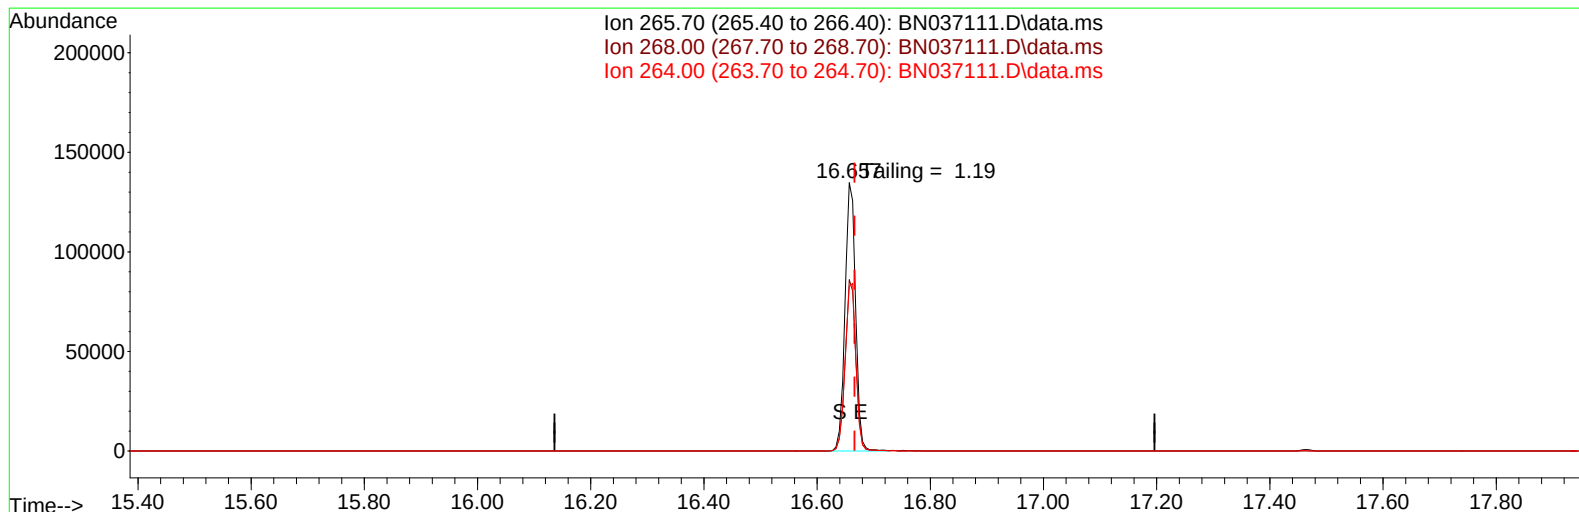

TIC: BN037111.D\data.ms

(70) Pentachlorophenol (C)




16.657min (-0.009) 15873.72 ng

response 175025

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.84
264.00	61.60	61.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052825\
Data File : BN037111.D
Acq On : 28 May 2025 16:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 17:56:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

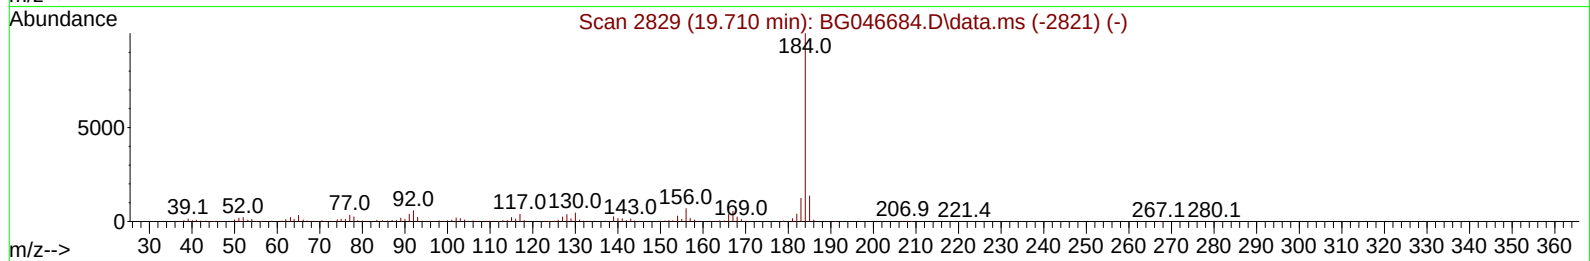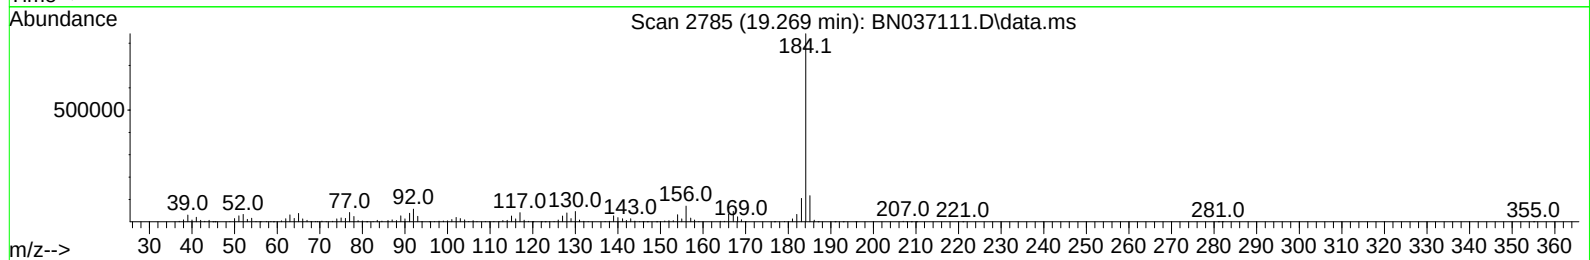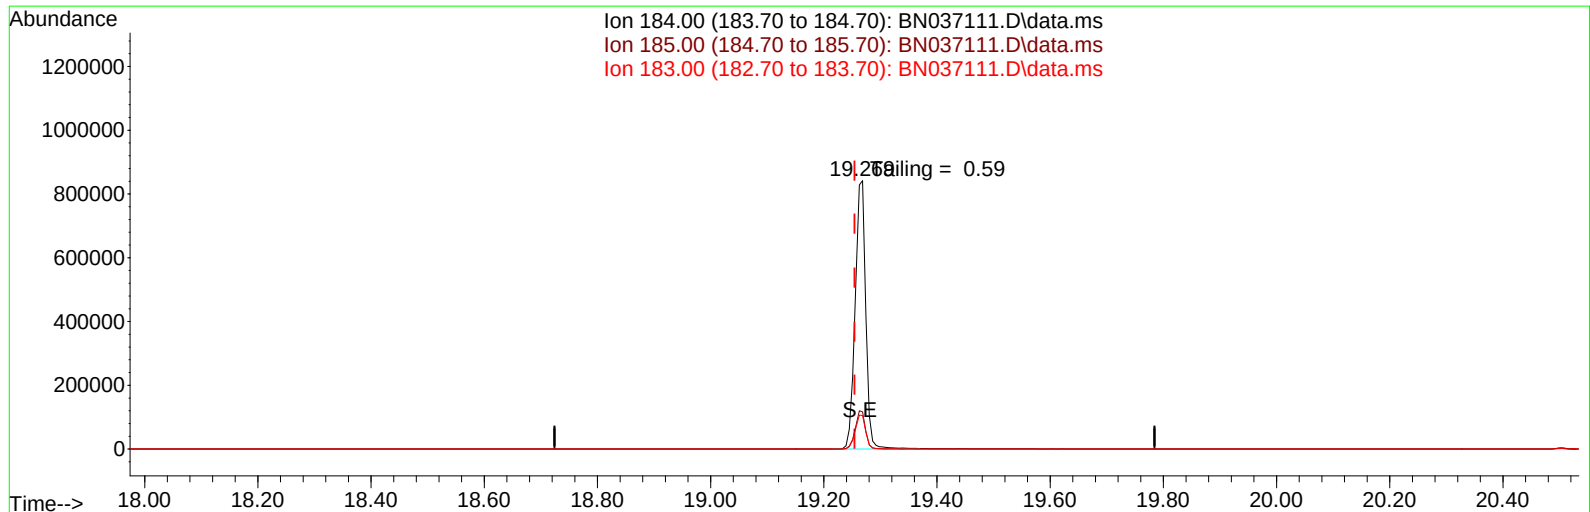

TIC: BN037111.D\data.ms

(77) Benzidine**19.269min (+ 0.014) 0.00 ng****response 1102765**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.87
183.00	13.20	12.47
0.00	0.00	0.00