
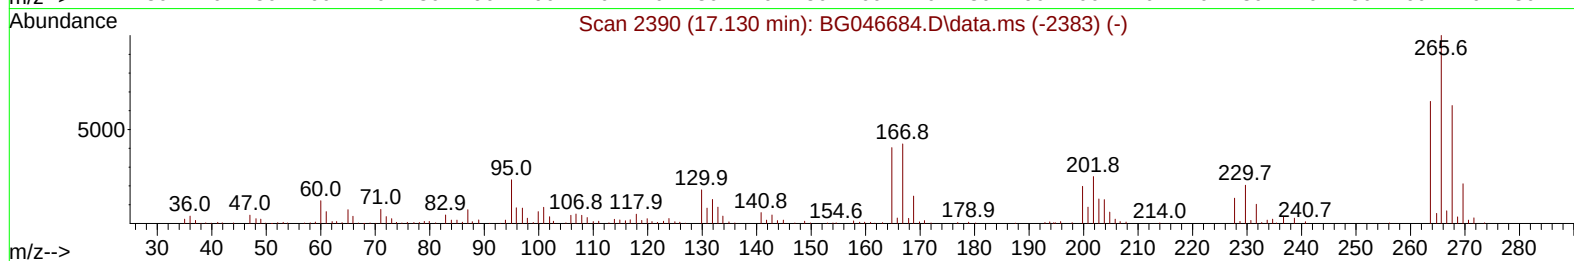
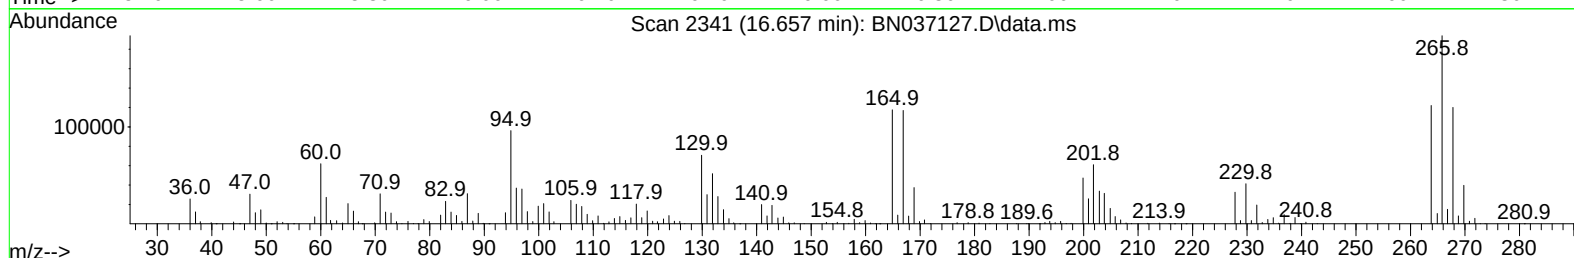


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052925\
Data File : BN037127.D
Acq On : 29 May 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 16:10:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

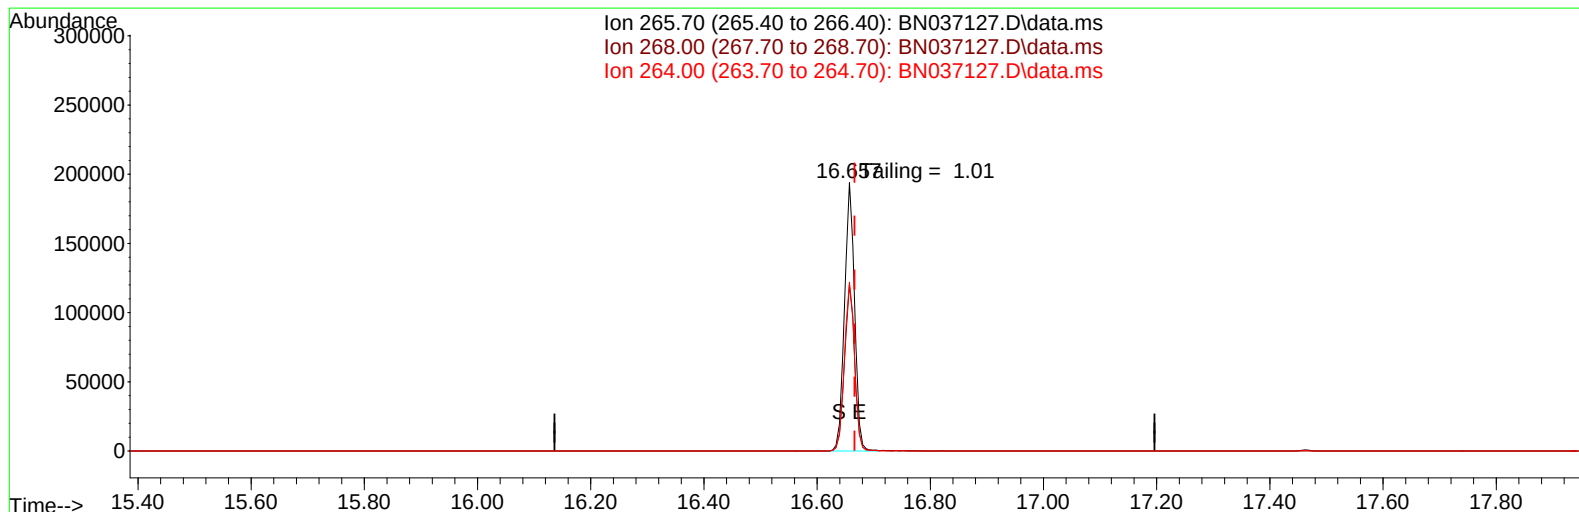

TIC: BN037127.D\data.ms




(70) Pentachlorophenol (C)

16.657min (-0.009) 17413.96 ng

response 239839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.88
264.00	61.60	62.90
0.00	0.00	0.00

Quant Time: May 29 16:10:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

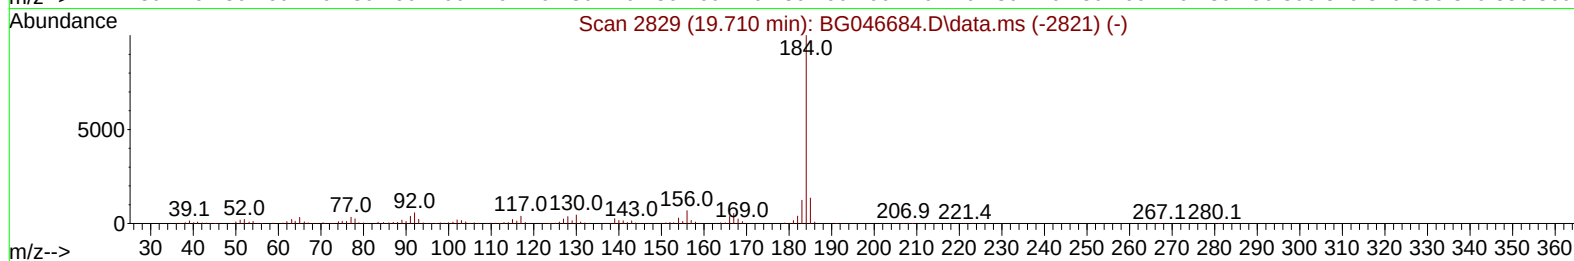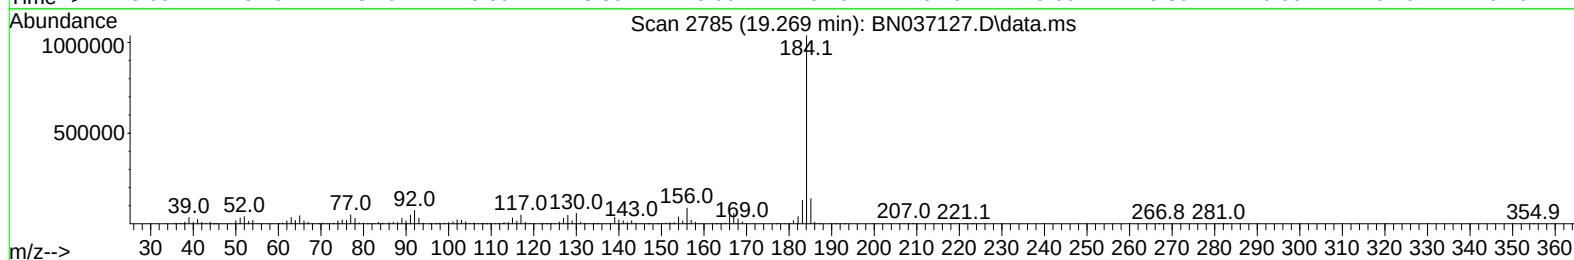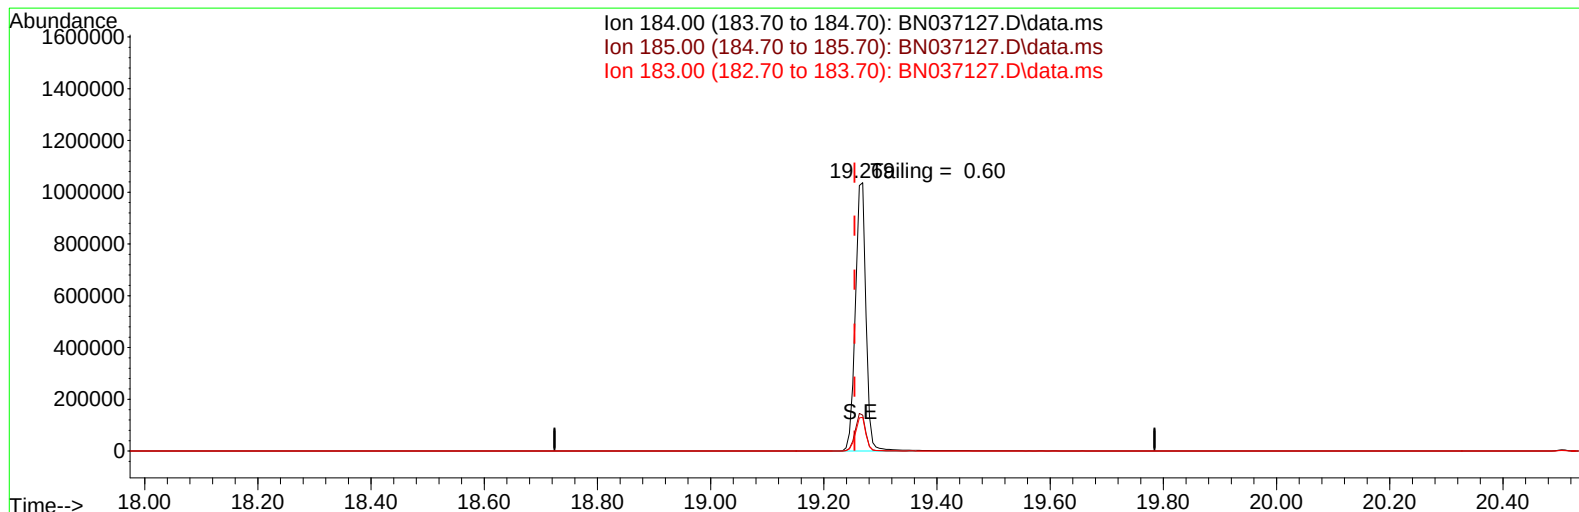

TIC: BN037127.D\data.ms

(77) Benzidine

19.269min (+ 0.015) 0.00 ng m

response **1341629**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.50	13.40
--------	-------	-------

183.00	13.20	12.52
--------	-------	-------

0.00 0.00 0.00