


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052925\
Data File : BN037127.D
Acq On : 29 May 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 14 11:26:32 2025

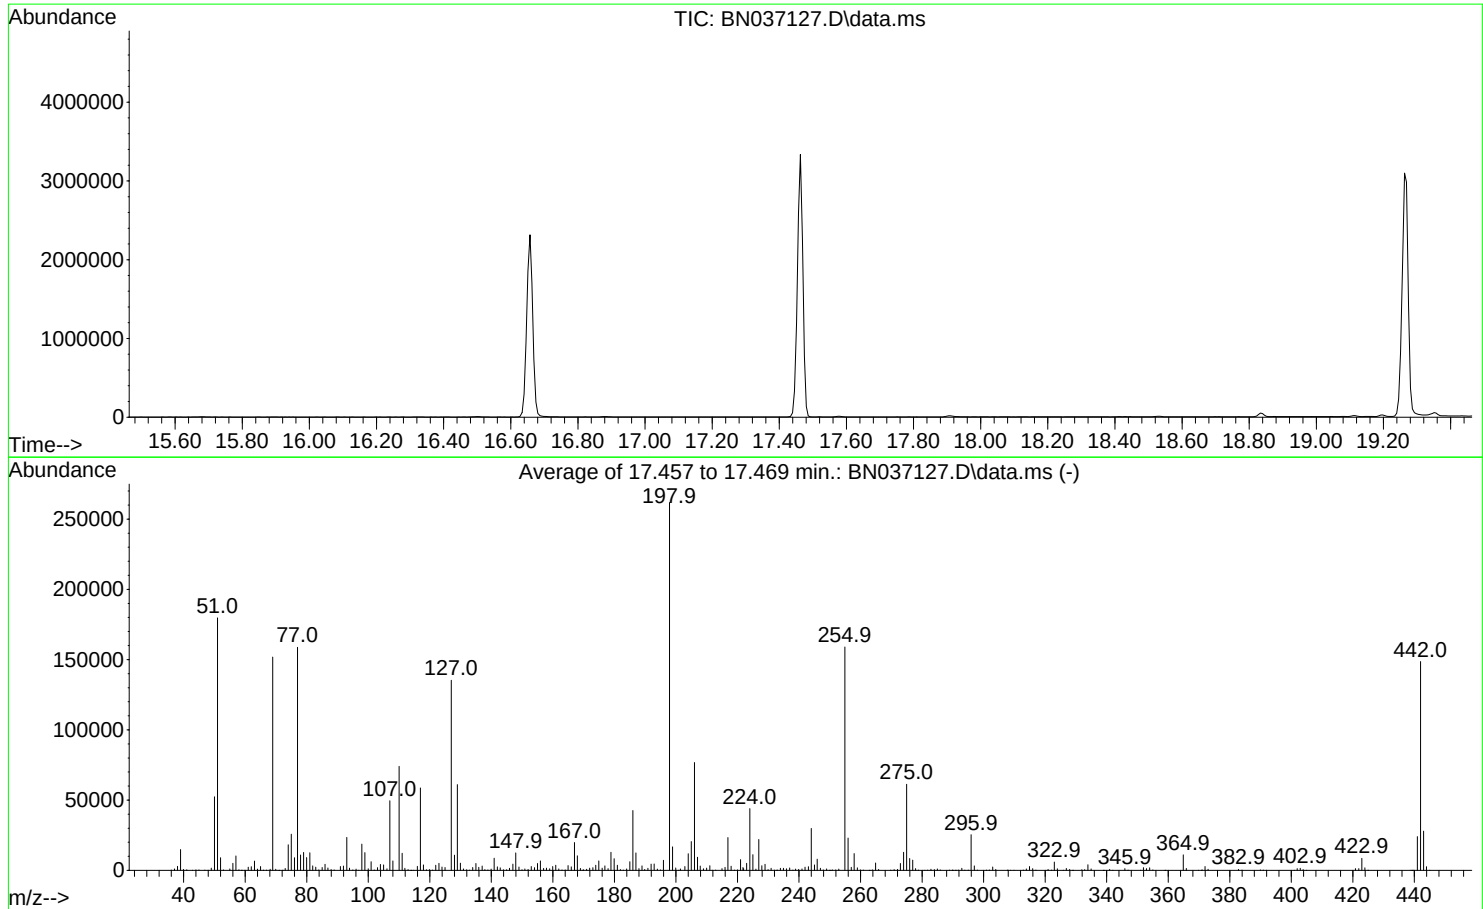




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.7	179763	PASS
68	69	0.00	2	0.5	810	PASS
69	198	0.00	100	58.0	151837	PASS
70	69	0.00	2	0.5	774	PASS
127	198	10	80	51.7	135352	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	261824	PASS
199	198	5	9	6.4	16719	PASS
275	198	10	60	23.4	61272	PASS
365	198	1	100	4.2	11025	PASS
441	198	0.01	100	9.2	23996	PASS
442	442	50	100	100.0	148611	PASS
443	442	15	24	18.8	27931	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052925\
Data File : BN037127.D
Acq On : 29 May 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 29 16:10:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

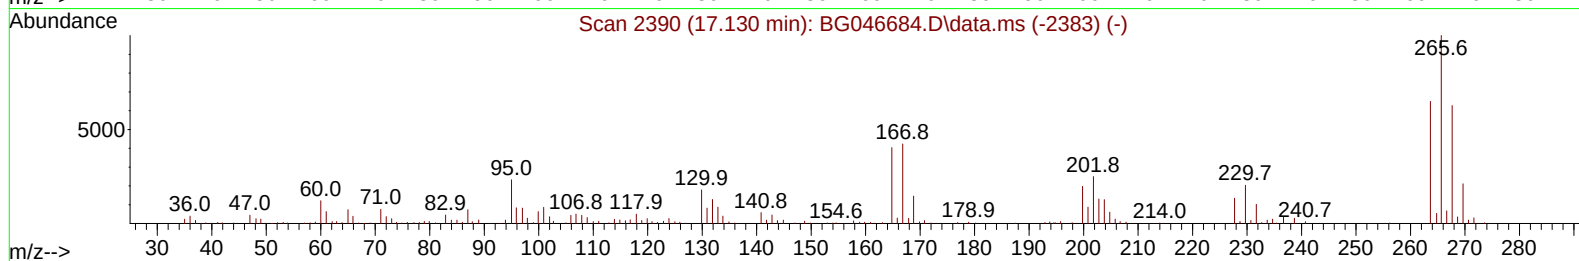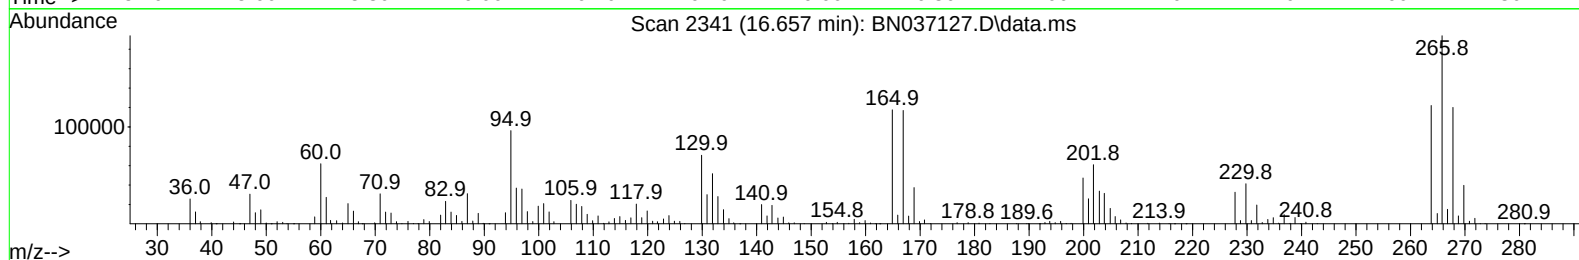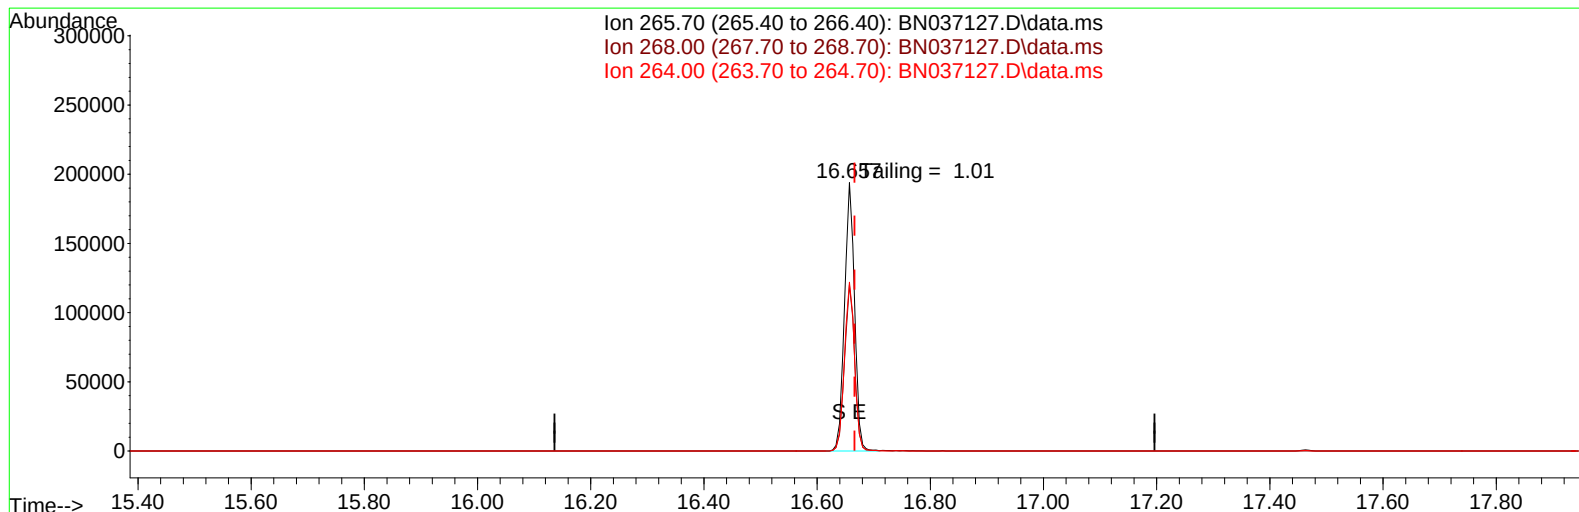

TIC: BN037127.D\data.ms

(70) Pentachlorophenol (C)

16.657min (-0.009) 17413.96 ng




response 239839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.88
264.00	61.60	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052925\
Data File : BN037127.D
Acq On : 29 May 2025 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 29 16:10:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

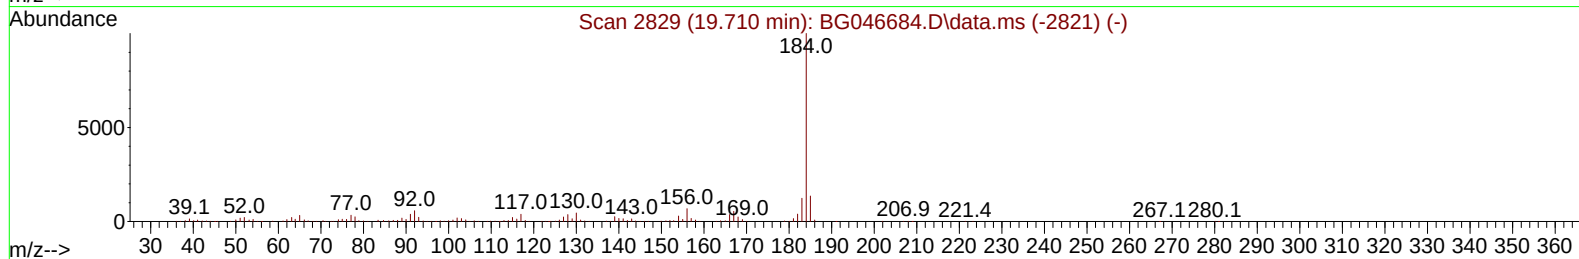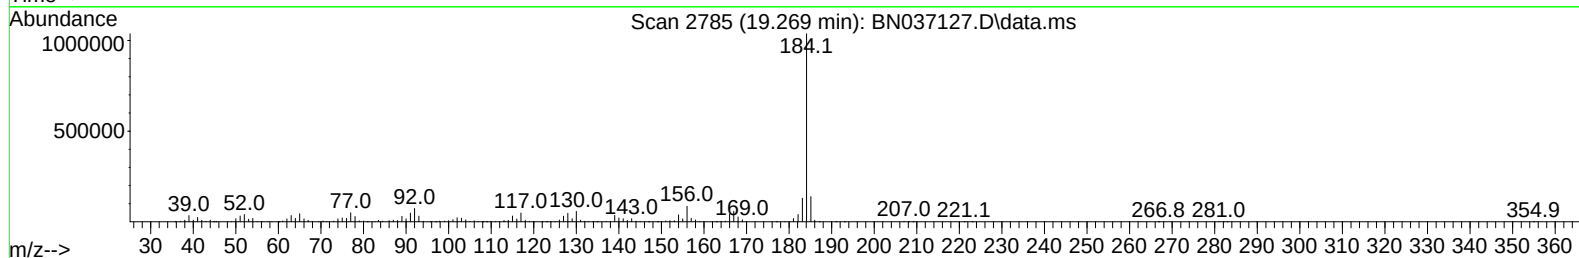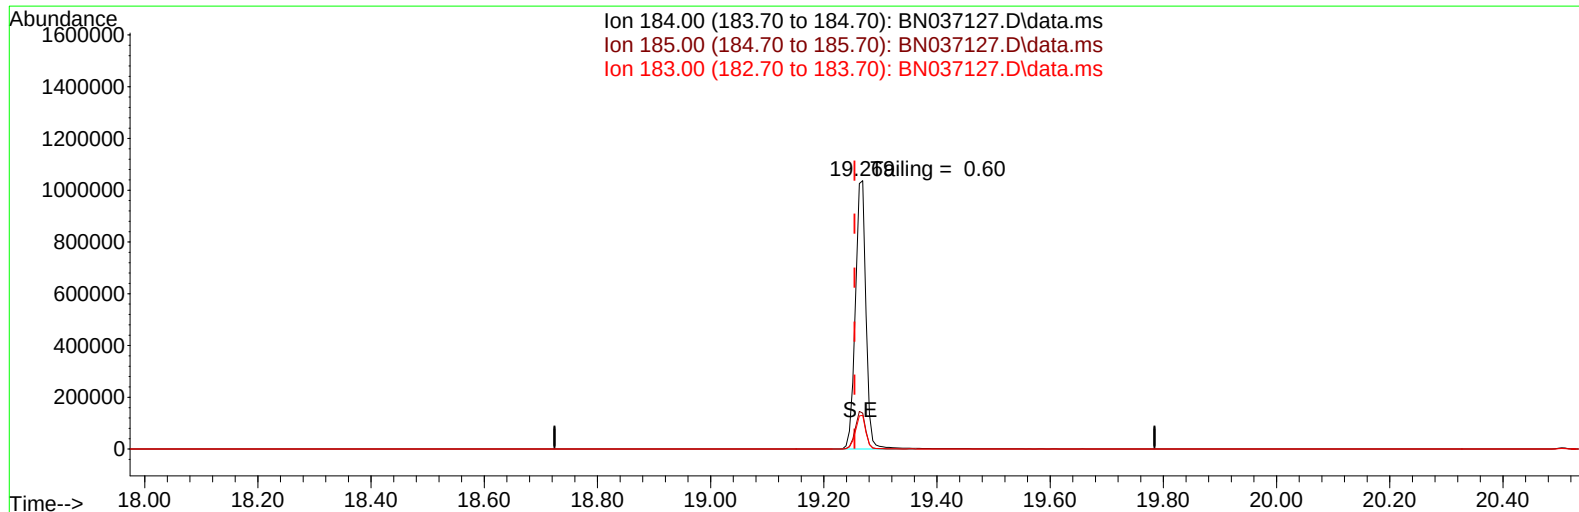

TIC: BN037127.D\data.ms

(77) Benzidine

19.269min (+ 0.015) 0.00 ng m

response 1341629

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.40
183.00	13.20	12.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/29/2025	BNA_N	<u>BN037127.D</u>
Compound Name	Response	Retention Time
DDT	789740	20.504
DDD	15689	20.063
DDE	611	19.557
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16300	806040	2.02

Instrument :
BNA_N
ClientSampleId :
DFTPP