
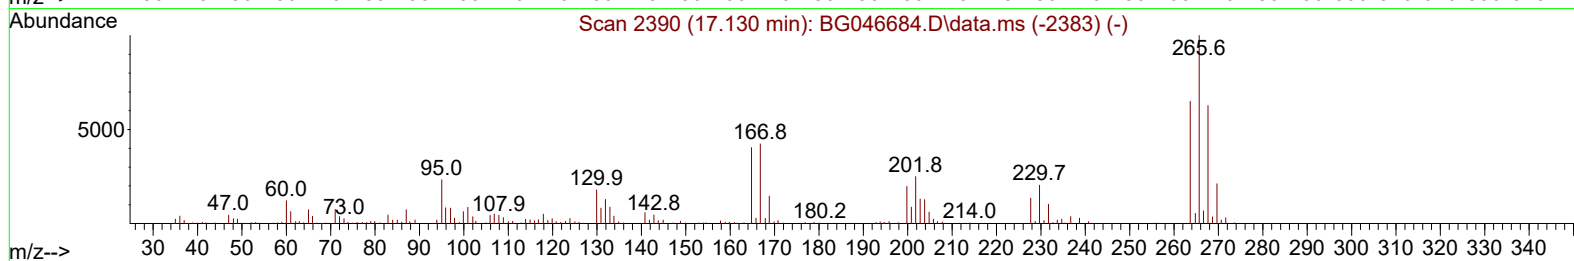
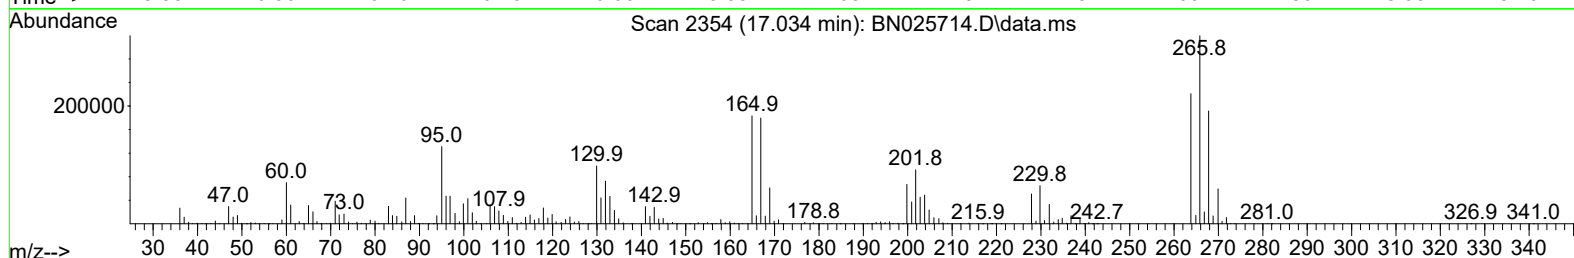


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
Data File : BN025714.D
Acq On : 30 May 2023 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 07:38:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 07:38:46 2023
Response via : Initial Calibration

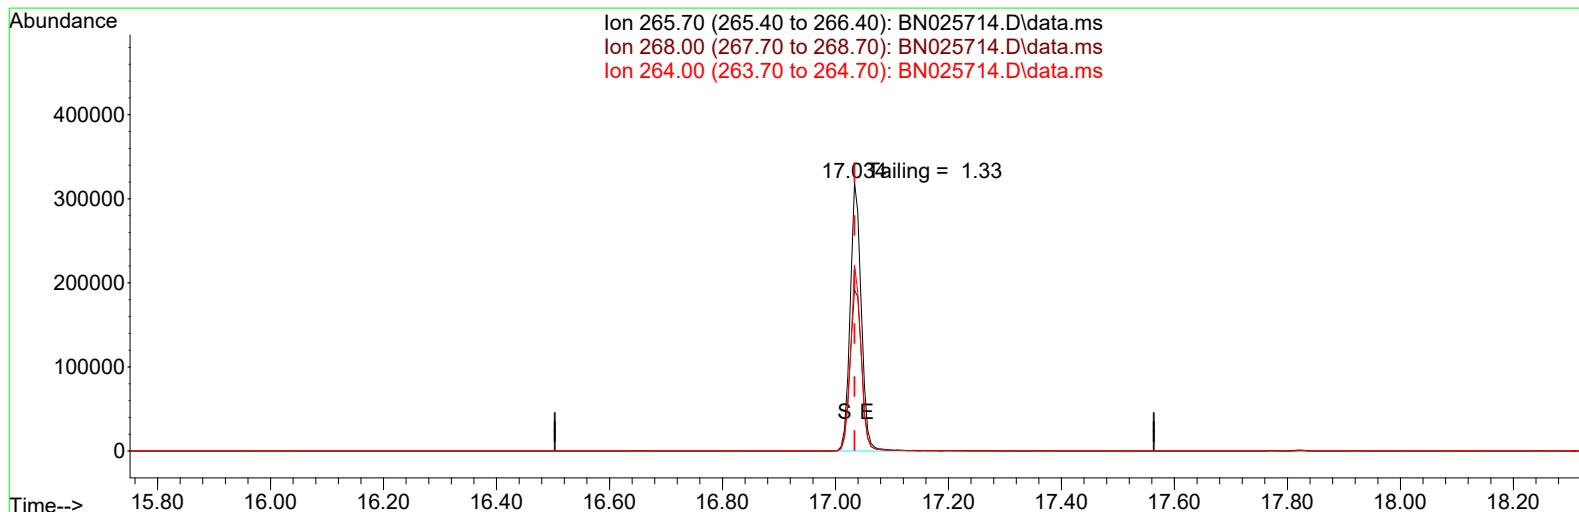

TIC: BN025714.D\data.ms

(70) Pentachlorophenol (C)




17.034min (0.000) 13736.37 ng

response 437774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.06
264.00	61.60	69.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
Data File : BN025714.D
Acq On : 30 May 2023 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 31 07:38:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 07:38:46 2023
Response via : Initial Calibration

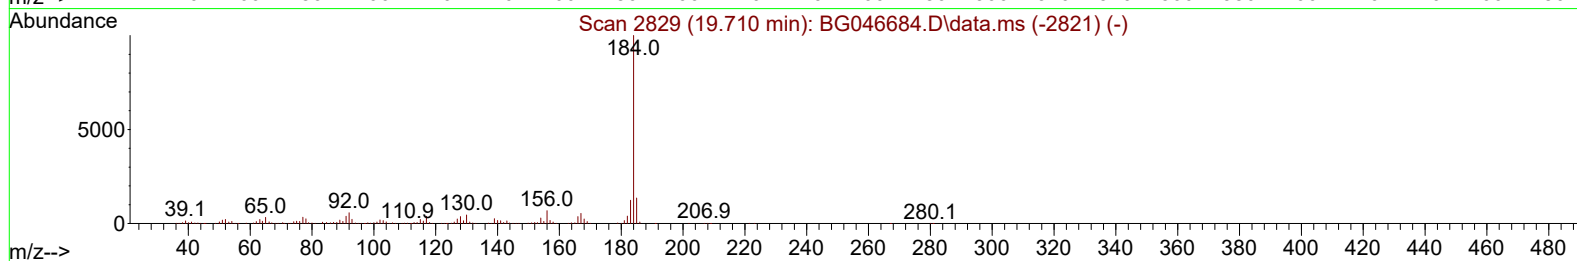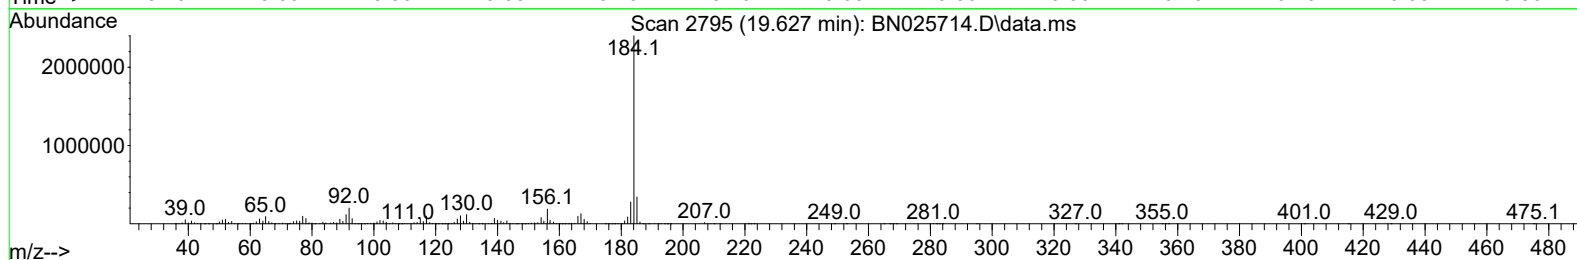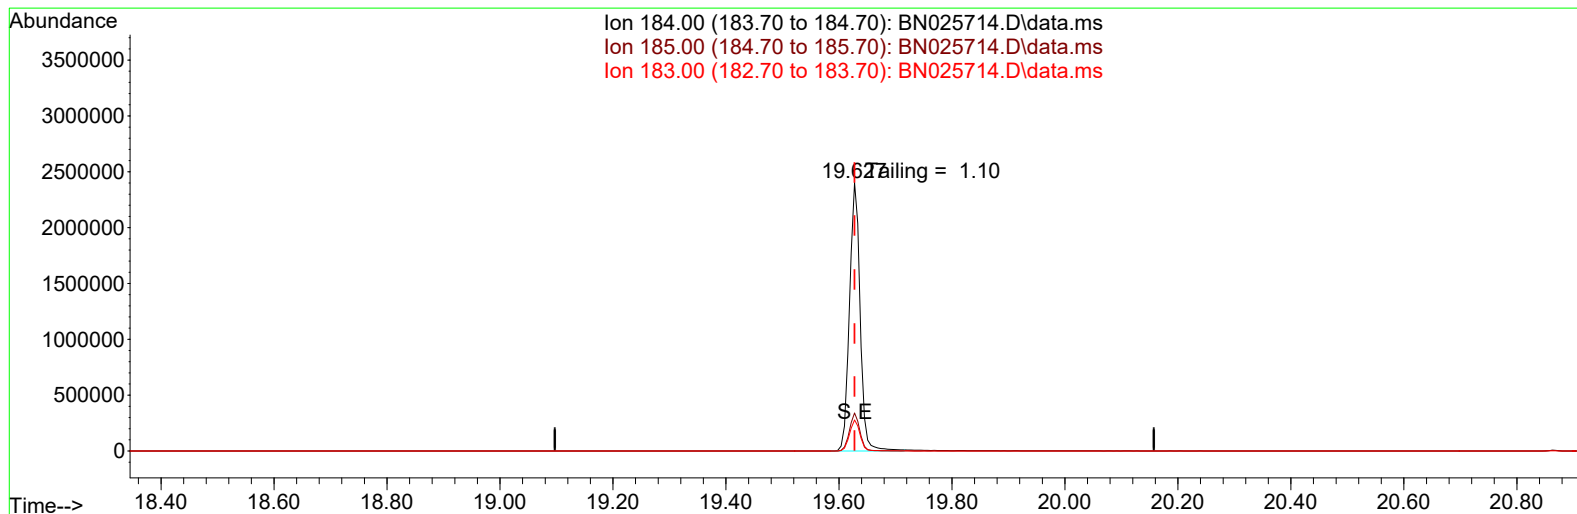

TIC: BN025714.D\data.ms

(77) Benzidine

19.627min (0.000) 268740.43 ng

response 3131361

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.19
183.00	13.20	11.56
0.00	0.00	0.00