


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
 Data File : BN025714.D
 Acq On : 30 May 2023 09:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 29 00:47:45 2023

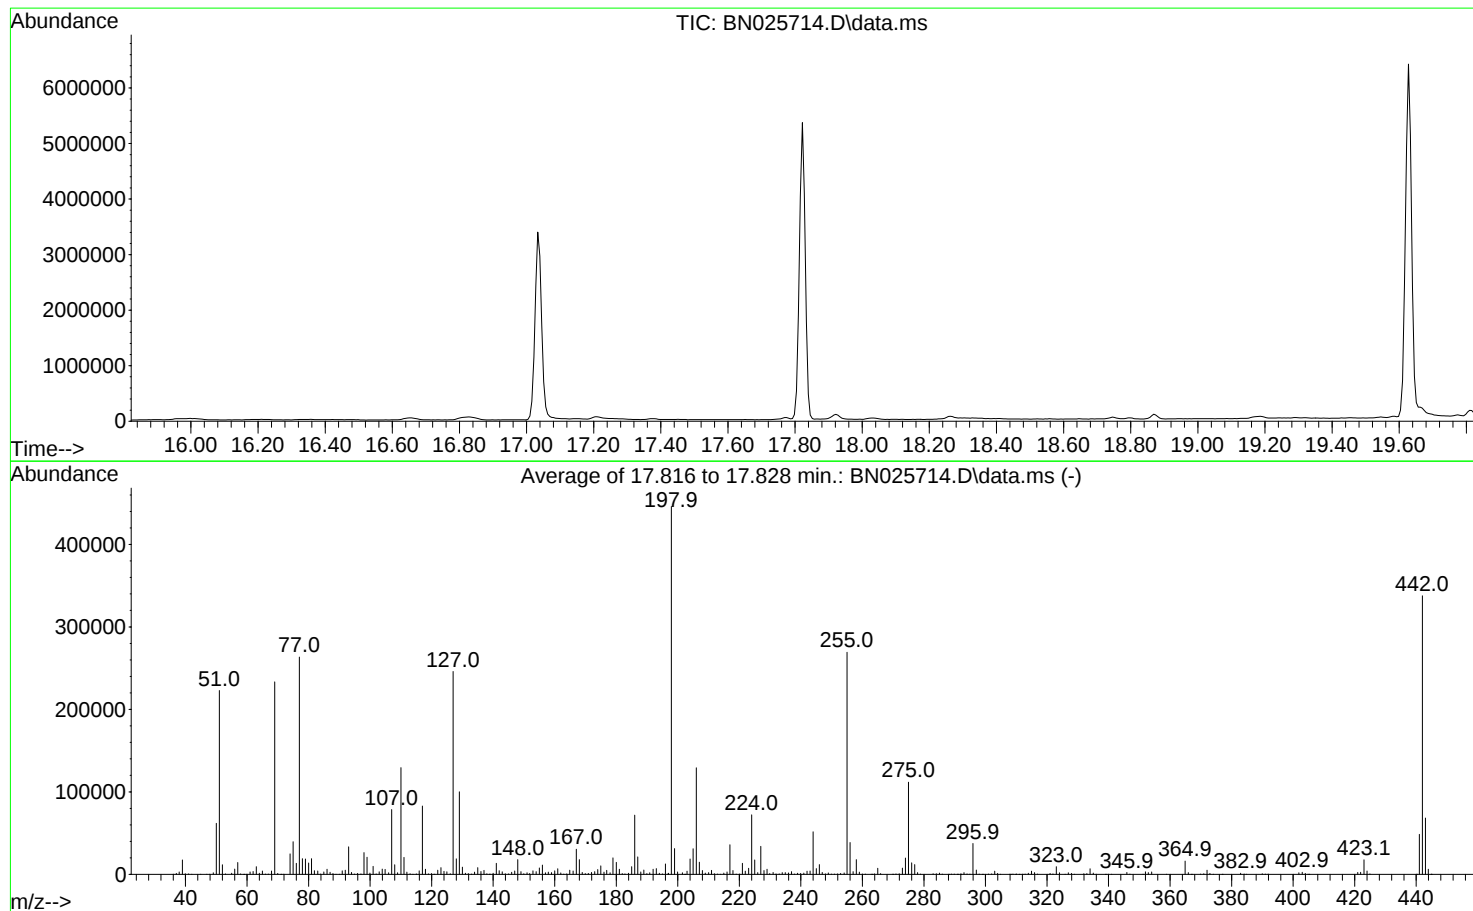




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.0	222885	PASS
68	69	0.00	2	1.8	4112	PASS
69	198	0.00	100	52.3	233413	PASS
70	69	0.00	2	0.5	1172	PASS
127	198	10	80	55.2	246037	PASS
197	198	0.00	2	0.3	1435	PASS
198	198	100	100	100.0	445995	PASS
199	198	5	9	7.0	31176	PASS
275	198	10	60	25.1	111749	PASS
365	198	1	100	3.6	16153	PASS
441	198	0.01	100	10.9	48459	PASS
442	442	50	100	100.0	337728	PASS
443	442	15	24	20.2	68320	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
Data File : BN025714.D
Acq On : 30 May 2023 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 31 07:38:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 07:38:46 2023
Response via : Initial Calibration

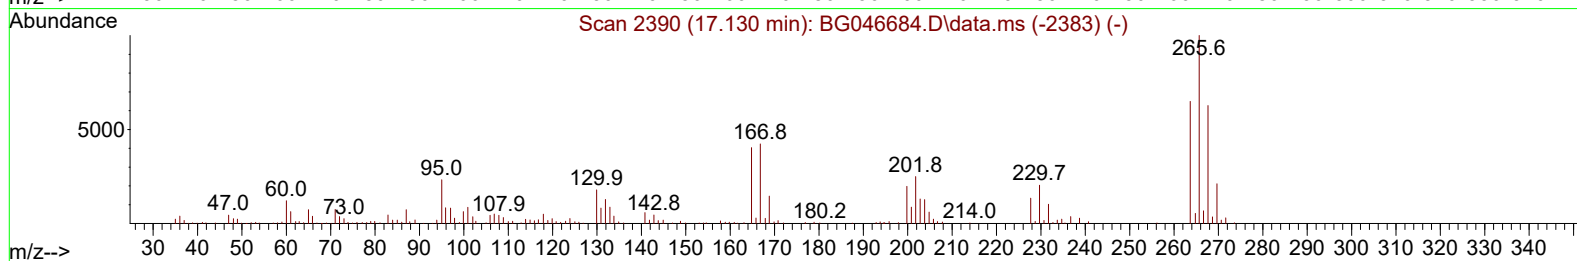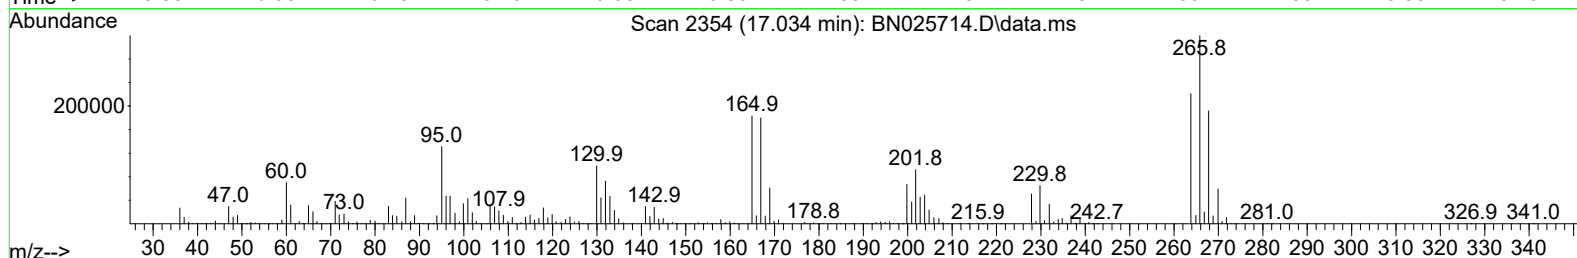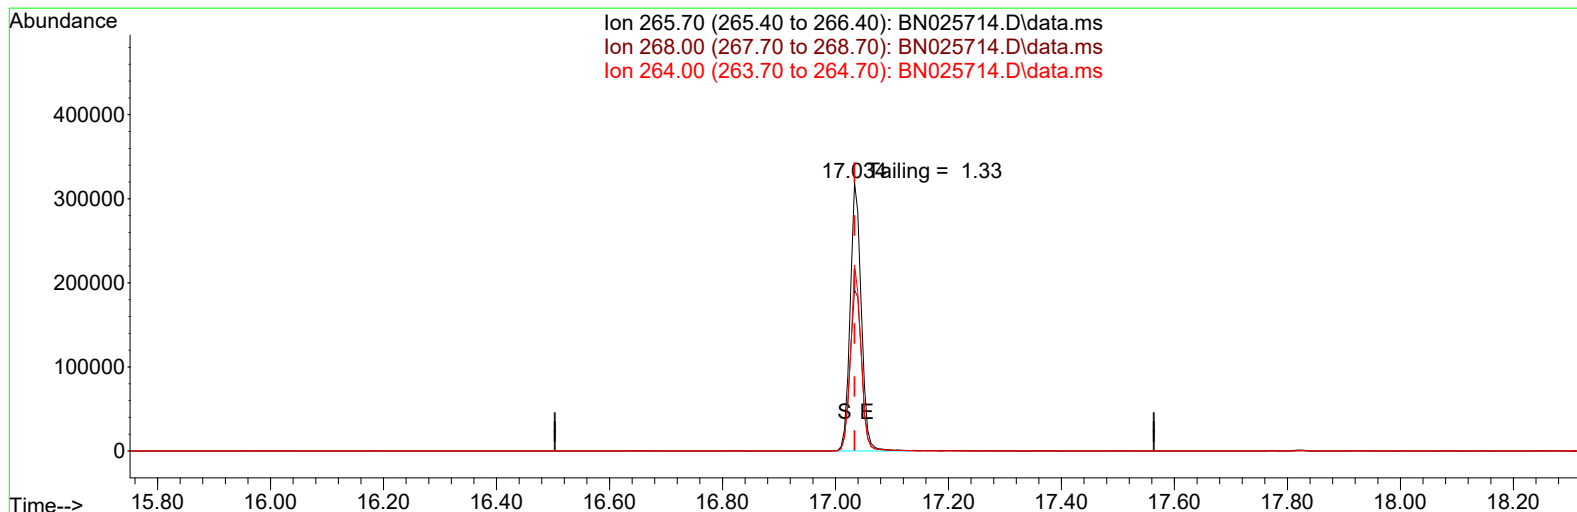

TIC: BN025714.D\data.ms

(70) Pentachlorophenol (C)

17.034min (0.000) 13736.37 ng




response 437774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.06
264.00	61.60	69.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
Data File : BN025714.D
Acq On : 30 May 2023 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 31 07:38:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 07:38:46 2023
Response via : Initial Calibration

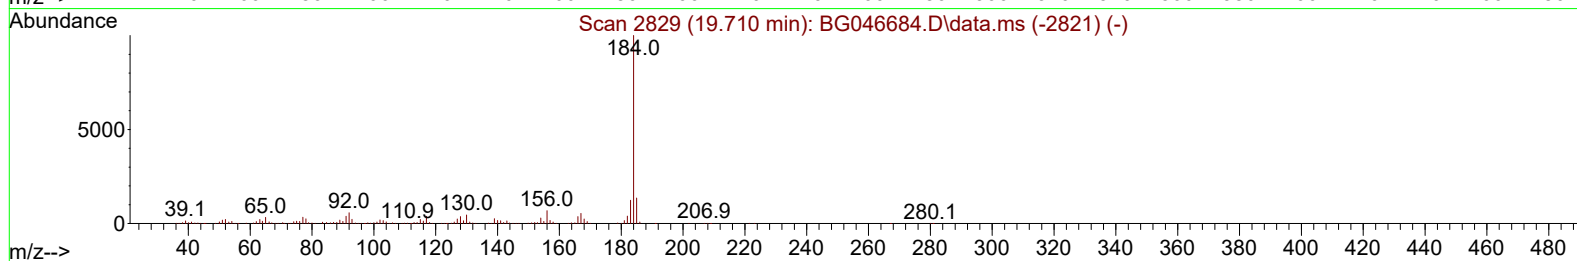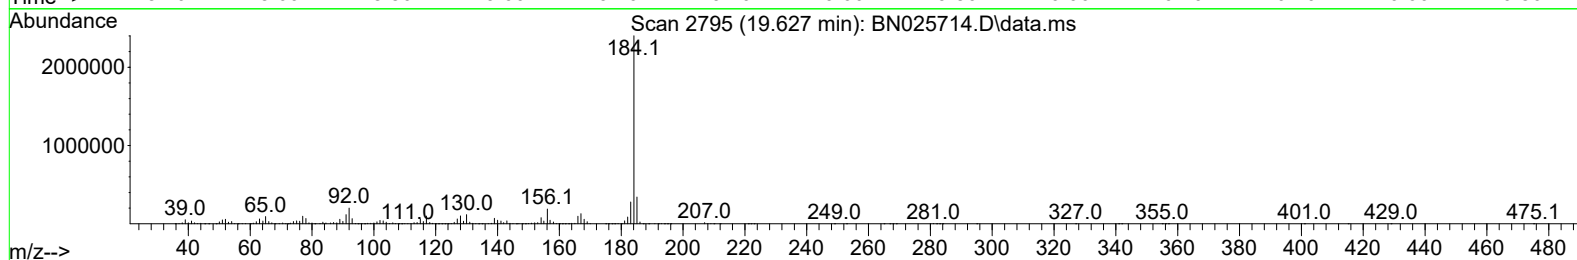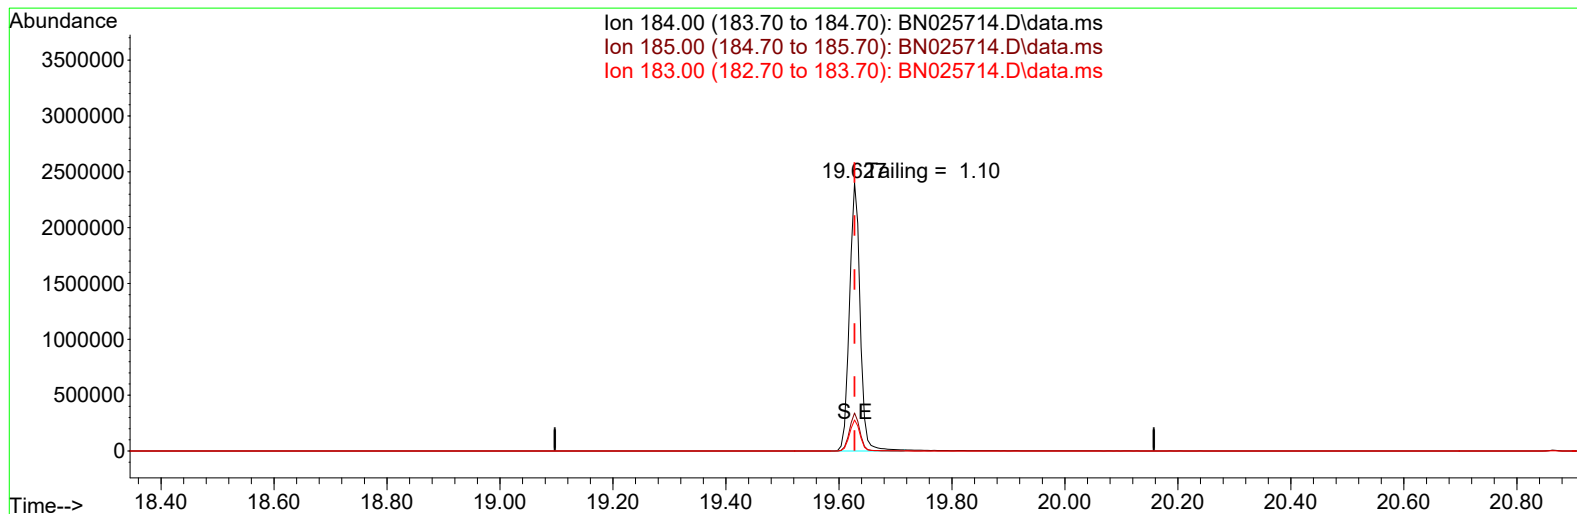

TIC: BN025714.D\data.ms

(77) Benzidine

19.627min (0.000) 268740.43 ng

response 3131361

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.19
183.00	13.20	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/30/2023	BNA_N	<u>BN025714.D</u>
Compound Name	Response	Retention Time
DDT	1318450	20.869
DDD	28394	20.422
DDE	1430	19.6
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29824	1348274	2.21

Instrument :
BNA_N
ClientSampleId :
DFTPP