
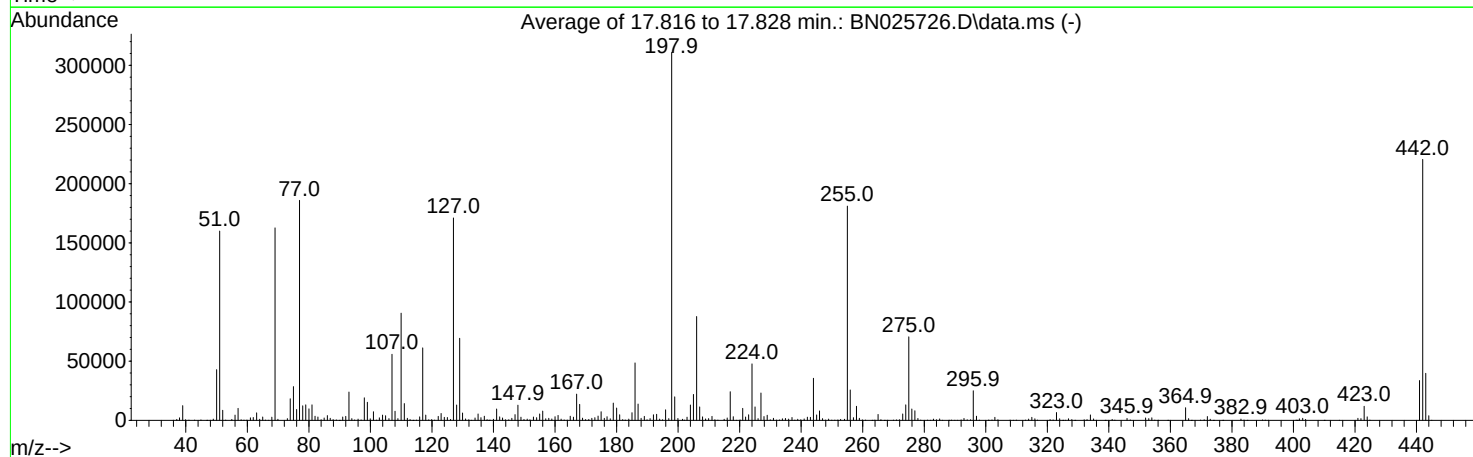


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
 Data File : BN025726.D
 Acq On : 30 May 2023 21:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN052623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 29 00:47:45 2023

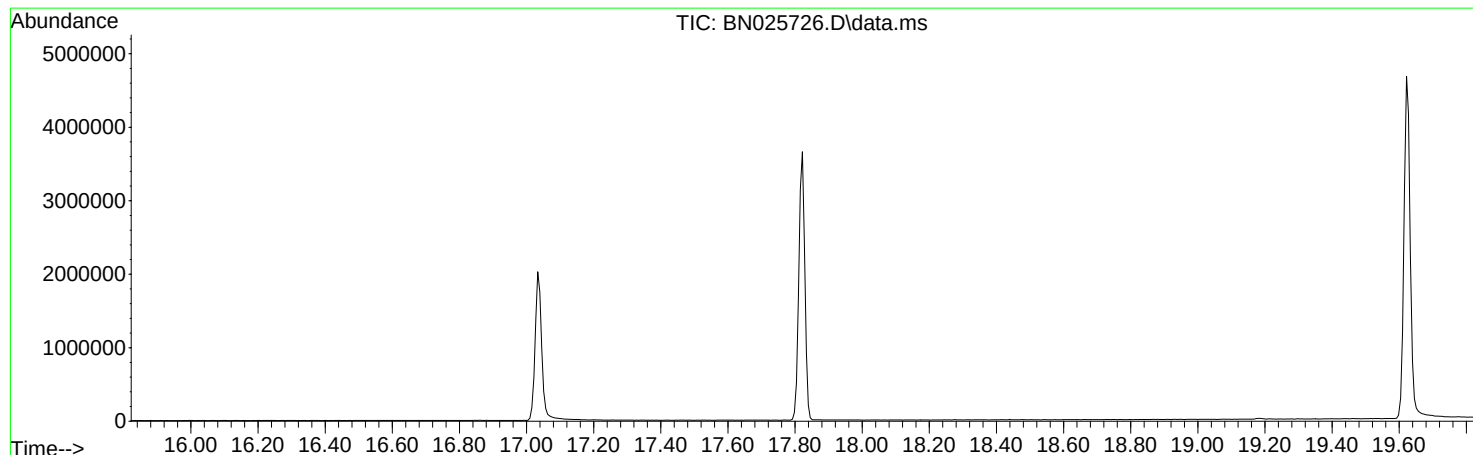

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	160003	PASS
68	69	0.00	2	1.6	2661	PASS
69	198	0.00	100	52.3	162669	PASS
70	69	0.00	2	0.6	974	PASS
127	198	10	80	55.0	171059	PASS
197	198	0.00	2	0.5	1487	PASS
198	198	100	100	100.0	310848	PASS
199	198	5	9	6.4	19885	PASS
275	198	10	60	22.7	70541	PASS
365	198	1	100	3.5	10750	PASS
441	198	0.01	100	10.8	33725	PASS
442	442	50	100	100.0	220523	PASS
443	442	15	24	18.0	39699	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/30/2023	BNA_N	<u>BN025726.D</u>
Compound Name	Response	Retention Time
DDT	952277	20.857
DDD	19886	20.416
DDE	589	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20475	972752	2.10

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
Data File : BN025726.D
Acq On : 30 May 2023 21:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 31 07:40:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 07:38:46 2023
Response via : Initial Calibration

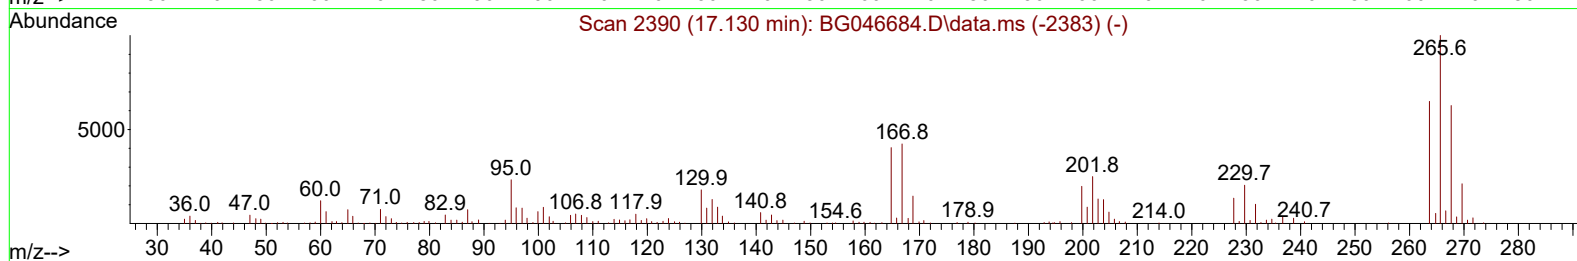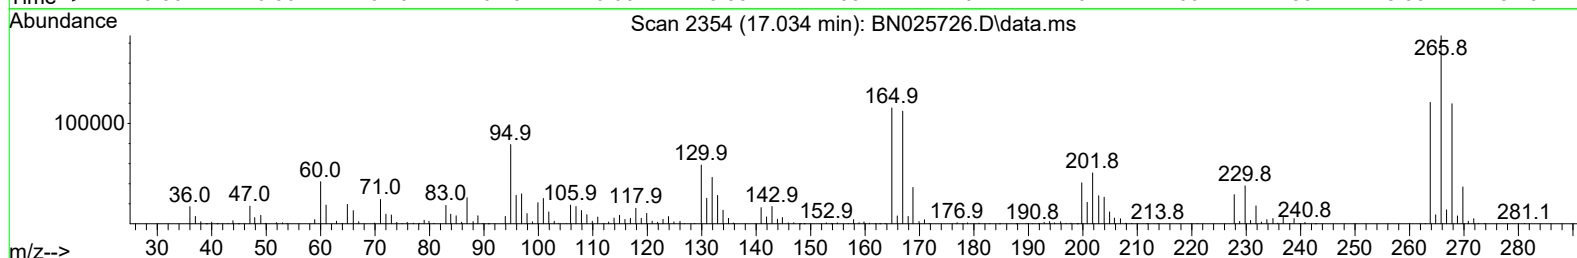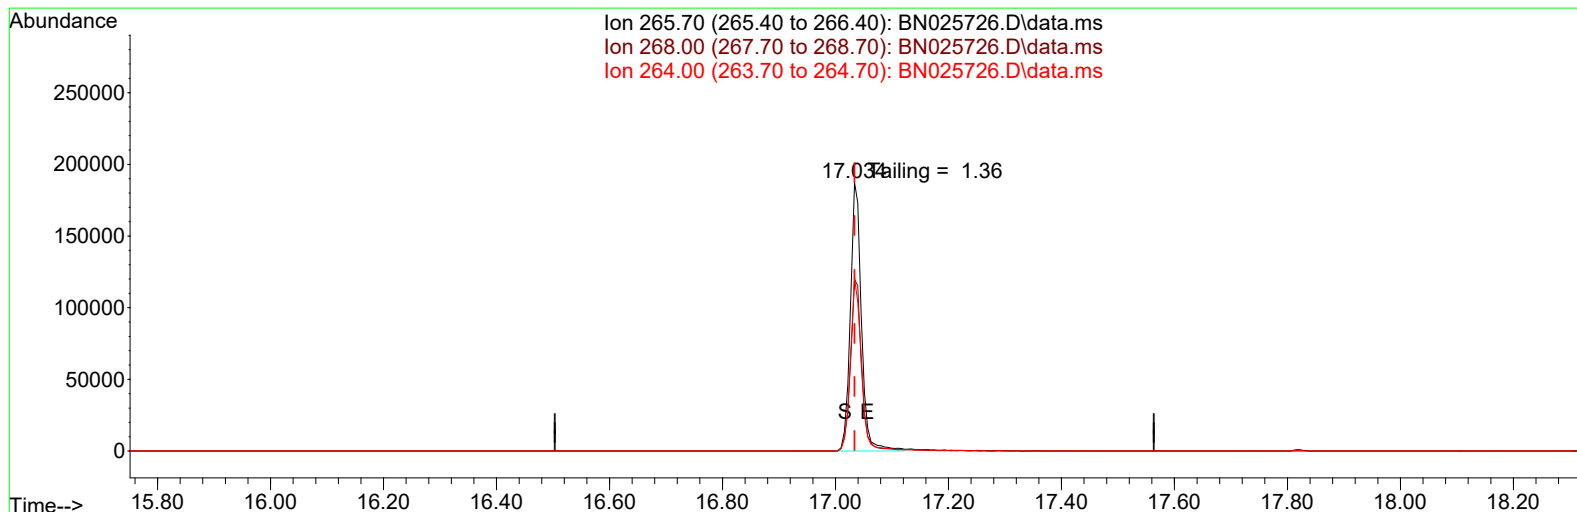

TIC: BN025726.D\data.ms

(70) Pentachlorophenol (C)

17.034min (+ 0.000) 13510.83 ng




response 257652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.89
264.00	61.60	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053023\
Data File : BN025726.D
Acq On : 30 May 2023 21:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 31 07:40:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 31 07:38:46 2023
Response via : Initial Calibration

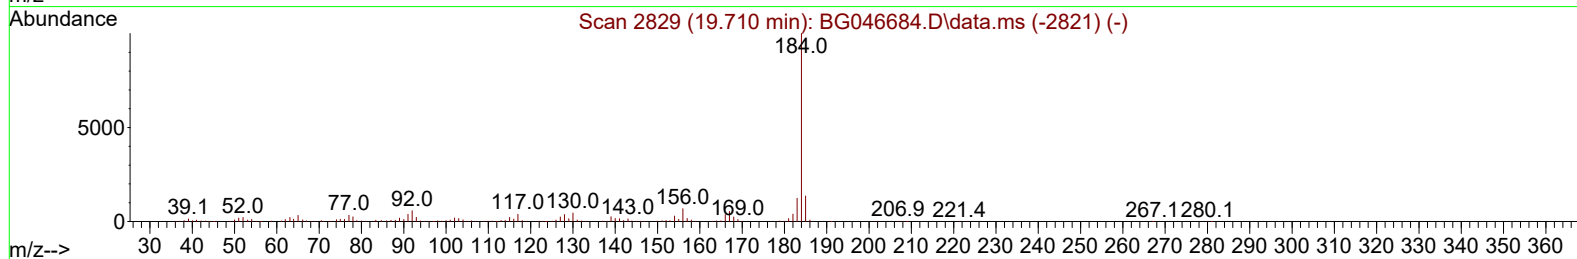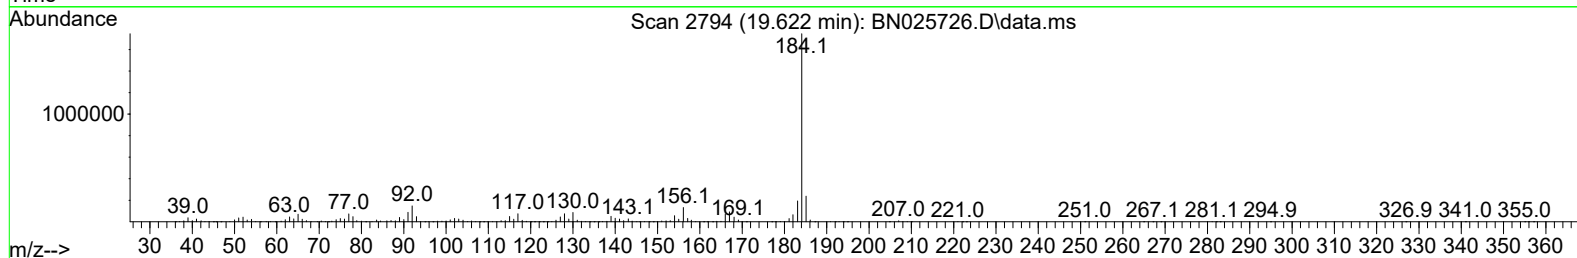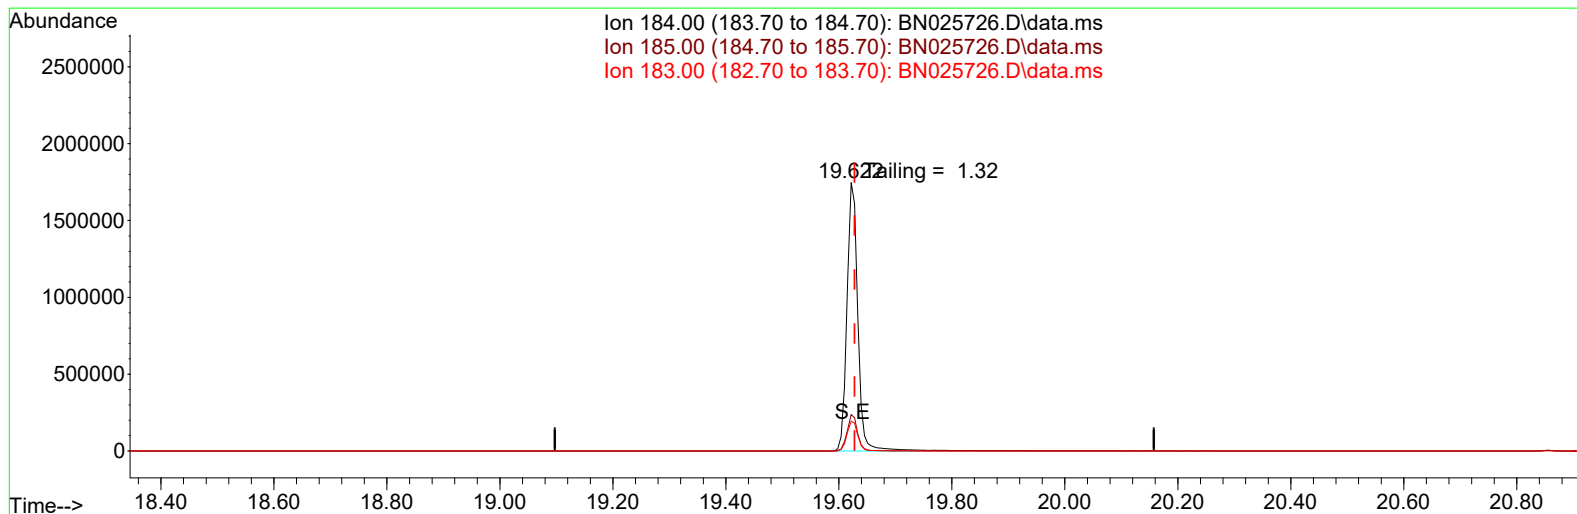

TIC: BN025726.D\data.ms

(77) Benzidine

19.622min (-0.006) 0.00 ng

response 2329028

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.10
0.00	0.00	0.00