

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
 Data File : BN020033.D
 Acq On : 07 Jun 2022 18:04
 Operator : CG/JU
 Sample : PB145287BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK287

Quant Time: Jun 07 22:34:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	129312	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	587488	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	390598	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	827769	20.000	ng/ul	0.00
79) Chrysene-d12	21.375	240	844007	20.000	ng/ul	0.00
88) Perylene-d12	23.704	264	859194	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	20715	6.938	ng/uL	0.00
4) Pyridine-d5	3.687	84	283894	34.790	ng/ul	0.00
7) Phenol-d5	6.987	99	354598	33.139	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	233743	34.964	ng/ul	0.00
11) 2-Chlorophenol-d4	7.358	132	304020	34.968	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	313389	33.852	ng/ul	0.00
21) Nitrobenzene-d5	8.975	128	156589	35.035	ng/ul	0.00
24) 2-Nitrophenol-d4	9.699	143	174087	36.701	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	274803	33.186	ng/ul	0.00
31) 4-Chloroaniline-d4	10.746	131	591912	44.141	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	1056257	37.165	ng/ul	0.00
49) Acenaphthylene-d8	14.140	160	1177019	35.712	ng/ul	0.00
54) 4-Nitrophenol-d4	14.640	143	195497	34.327	ng/ul	0.00
60) Fluorene-d10	15.440	176	869165	36.957	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	169301	35.308	ng/ul	0.00
73) Anthracene-d10	17.292	188	1423532	39.405	ng/ul	0.00
81) Pyrene-d10	19.586	212	1631468	35.656	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.563	264	1636779	38.935	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.528	70	8008	1.113 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020033.D
Acq On : 07 Jun 2022 18:04
Operator : CG/JU
Sample : PB145287BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK287


Quant Time: Jun 07 22:34:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

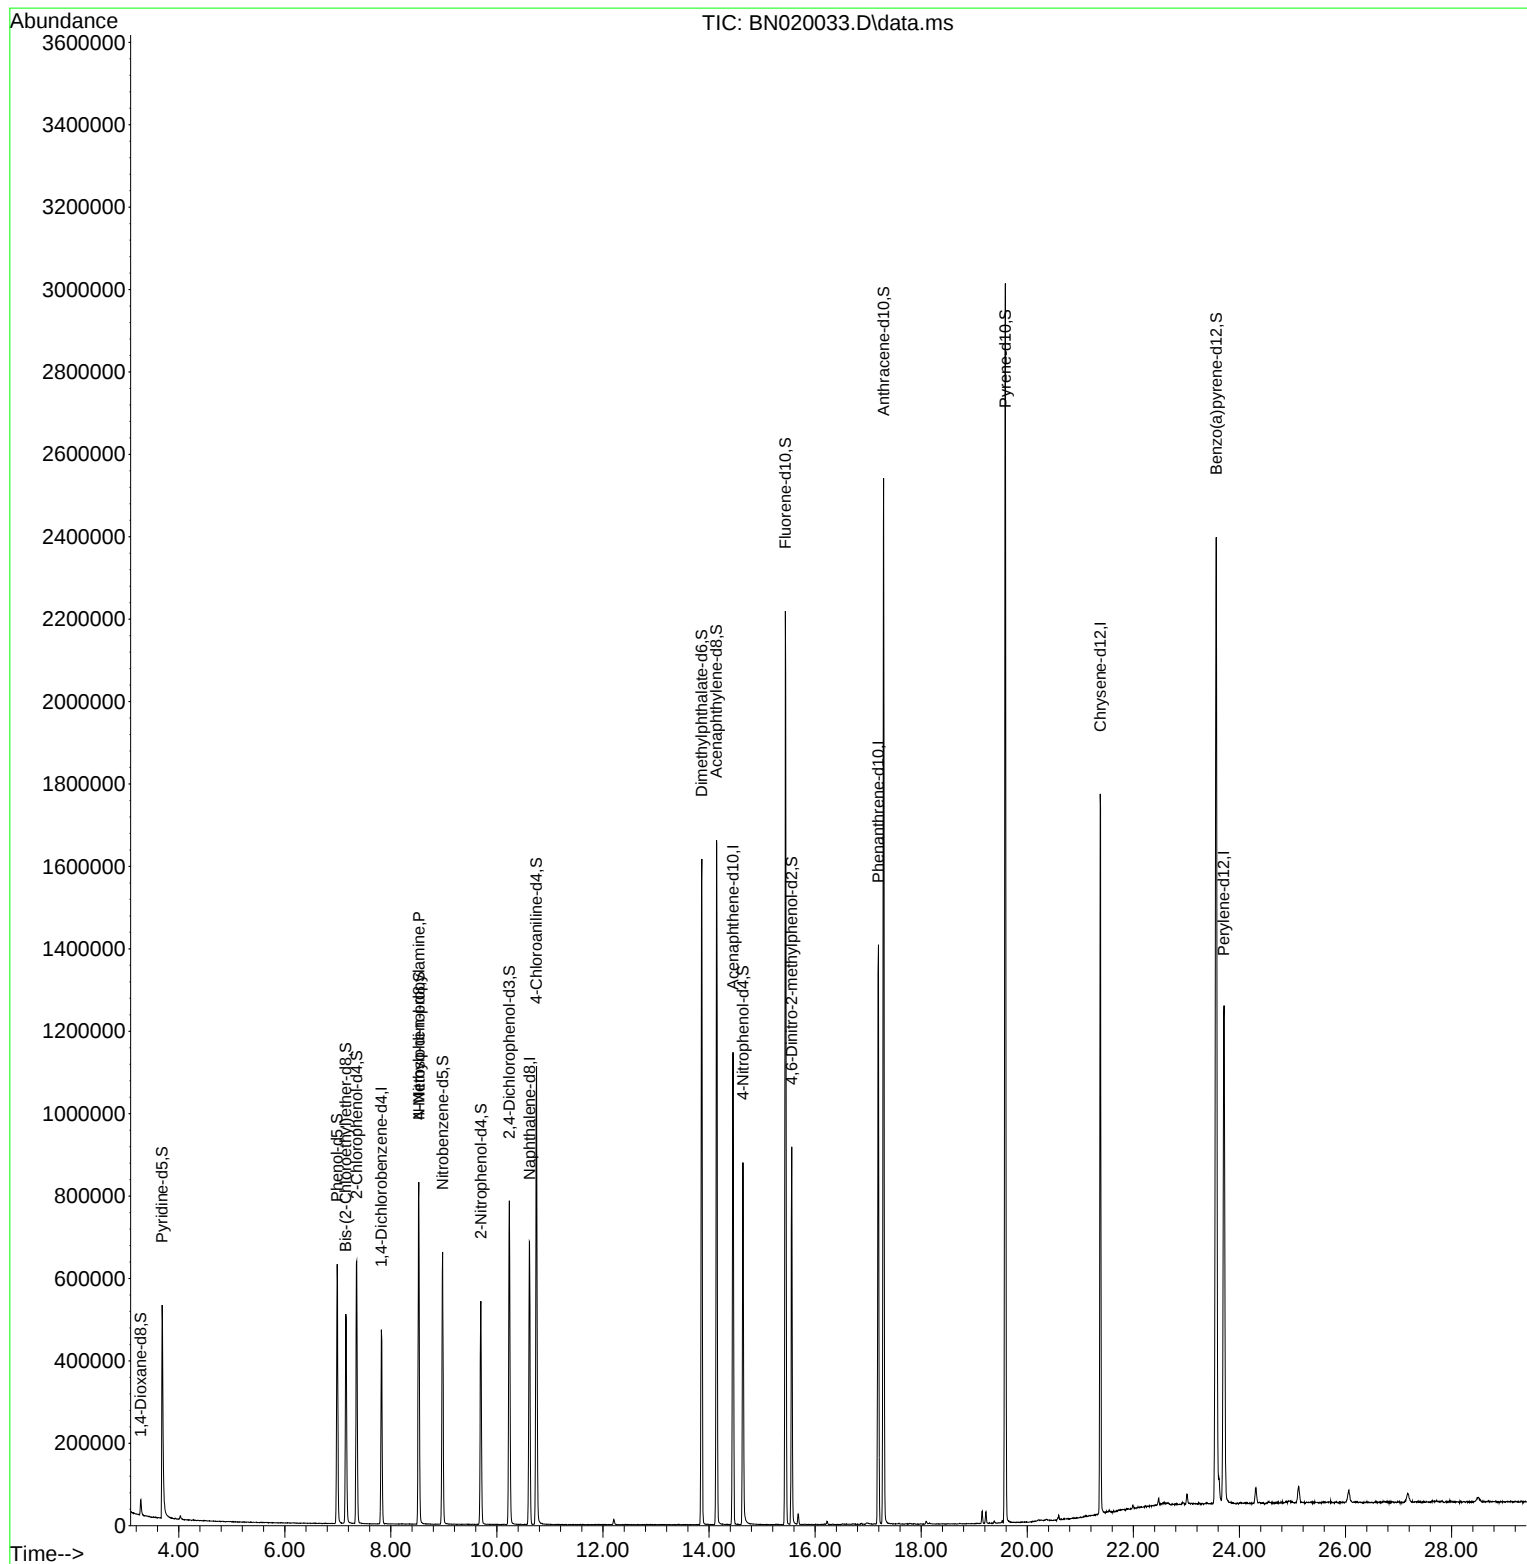

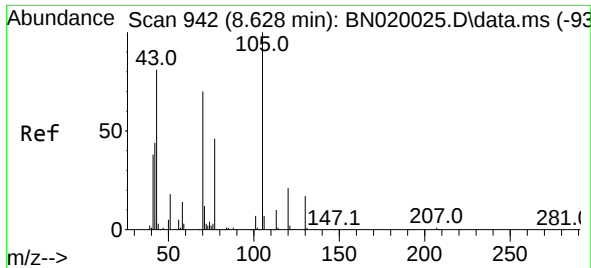

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.113 ng/ul
 RT: 8.528 min Scan# 91
 Delta R.T. -0.100 min
 Lab File: BN020033.D
 Acq: 07 Jun 2022 18:04

Instrument :
 BNA_N
 ClientSampleId :
 SBLK287

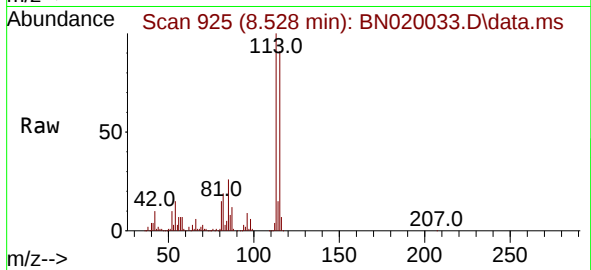

Tgt Ion: 70 Resp: 8008

Ion	Ratio	Lower	Upper
70	100		
42	408.4	47.8	71.6#
101	0.0	7.8	11.6#
130	0.0	15.8	23.8#

