

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
 Data File : BN020035.D
 Acq On : 07 Jun 2022 19:16
 Operator : CG/JU
 Sample : N3171-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBTZ6

Quant Time: Jun 07 22:34:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	125815	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	575068	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	374749	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	798376	20.000	ng/ul	0.00
79) Chrysene-d12	21.375	240	792321	20.000	ng/ul	0.00
88) Perylene-d12	23.710	264	802877	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	10788	3.714	ng/uL	0.00
4) Pyridine-d5	3.699	84	21892	2.757	ng/ul	0.01
7) Phenol-d5	6.987	99	50355	4.837	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	181400	27.888	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	172546	20.398	ng/ul	0.00
15) 4-Methylphenol-d8	8.528	113	88537	9.830	ng/ul	0.00
21) Nitrobenzene-d5	8.975	128	123685	28.271	ng/ul	0.00
24) 2-Nitrophenol-d4	9.693	143	124763	26.871	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	199634	24.629	ng/ul	0.00
31) 4-Chloroaniline-d4	10.746	131	54335	4.139	ng/ul	0.00
46) Dimethylphthalate-d6	13.863	166	852061	31.248	ng/ul	0.00
49) Acenaphthylene-d8	14.146	160	953015	30.138	ng/ul	0.00
54) 4-Nitrophenol-d4	14.640	143	27879	5.102	ng/ul	0.00
60) Fluorene-d10	15.440	176	730855	32.391	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	124469	26.914	ng/ul	0.00
73) Anthracene-d10	17.292	188	1158020	33.235	ng/ul	0.00
81) Pyrene-d10	19.586	212	1426613	33.213	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.563	264	1381001	35.155	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	13.863	165	6353	1.184	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020035.D
Acq On : 07 Jun 2022 19:16
Operator : CG/JU
Sample : N3171-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBTZ6


Quant Time: Jun 07 22:34:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

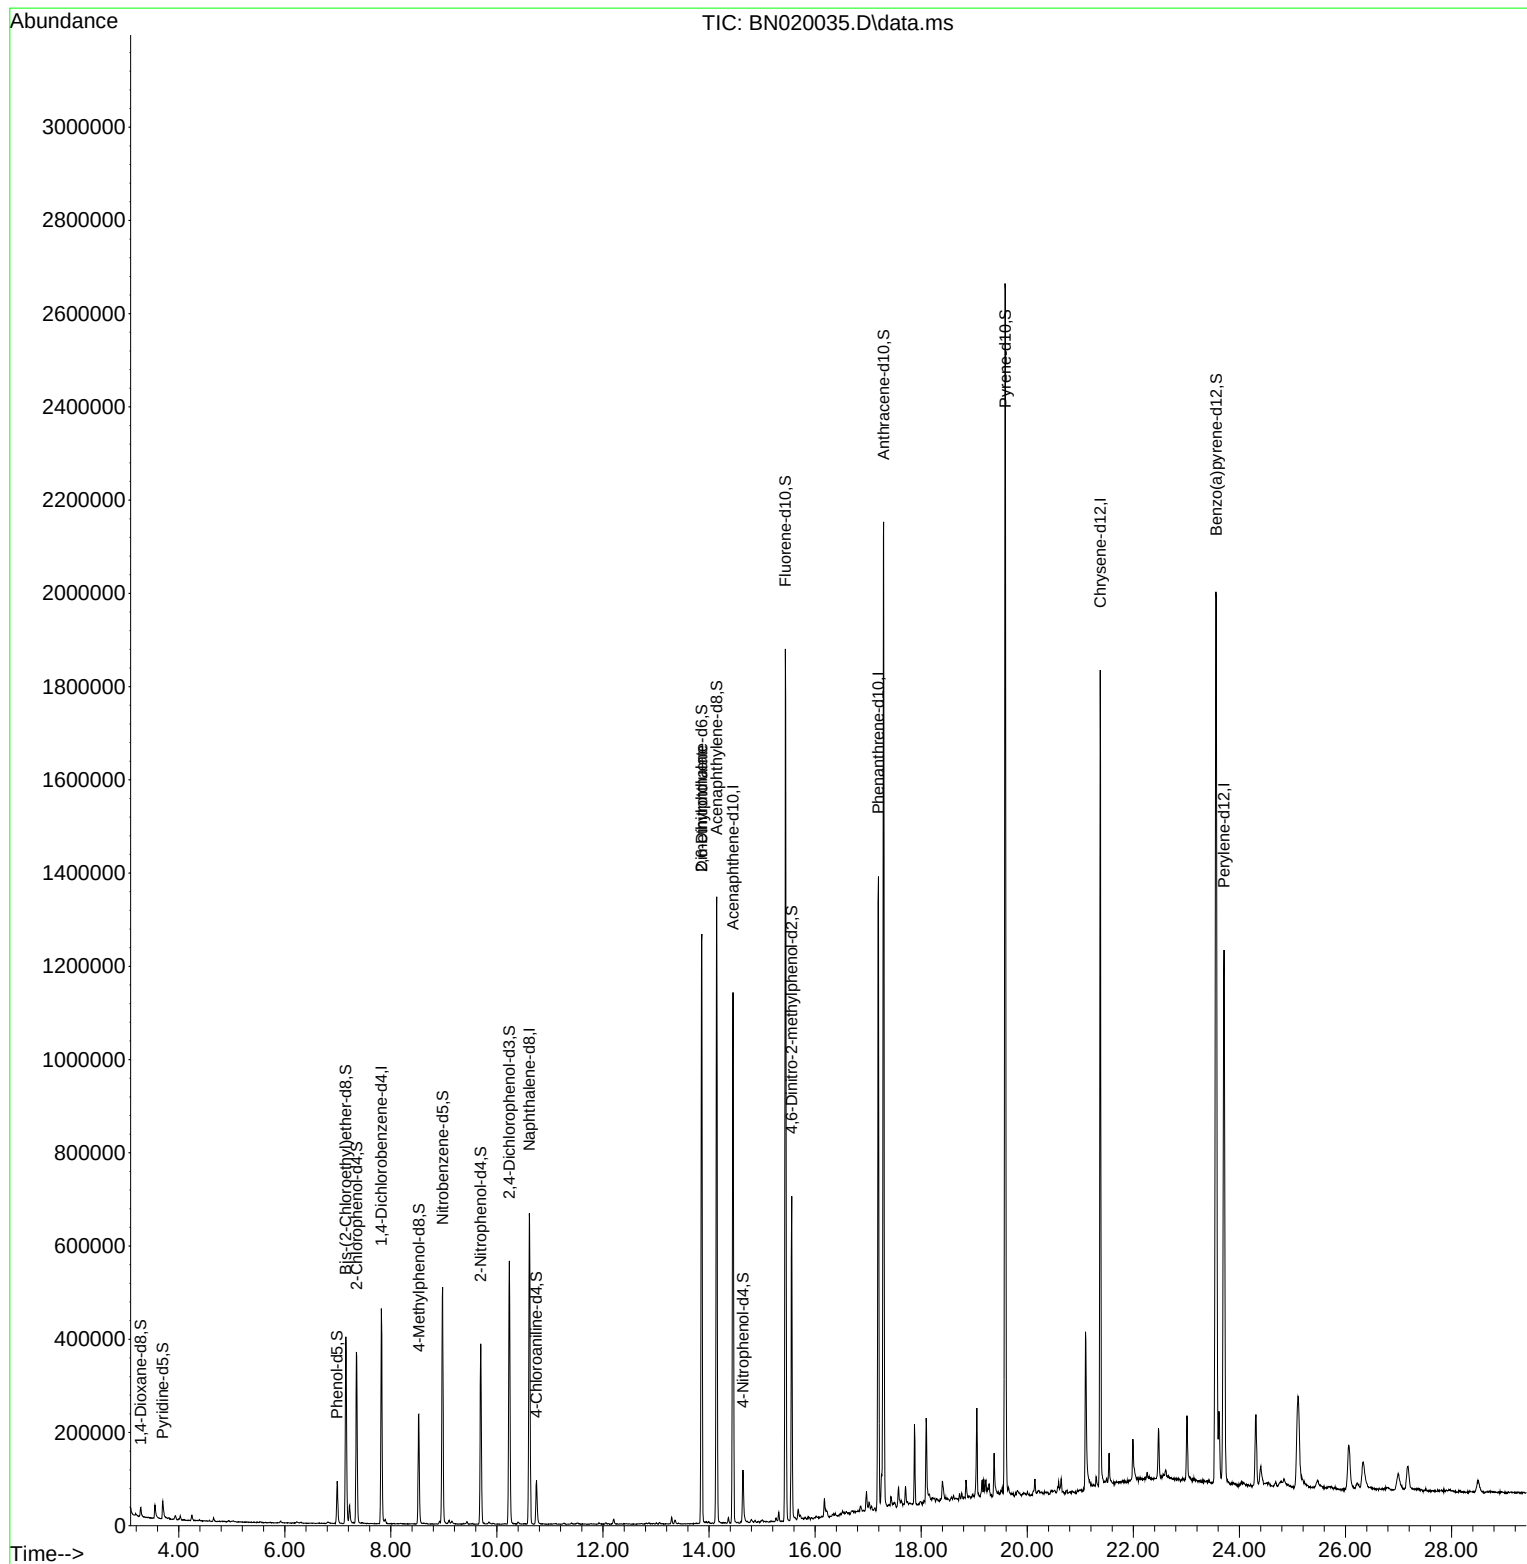

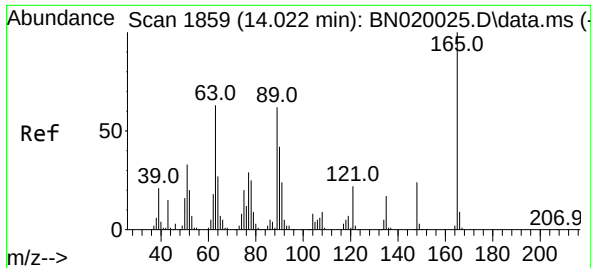

#48
 2,6-Dinitrotoluene
 Concen: 1.184 ng/ul
 RT: 13.863 min Scan# 11
 Delta R.T. -0.164 min
 Lab File: BN020035.D
 Acq: 07 Jun 2022 19:16

Instrument :
 BNA_N
 ClientSampleId :
 DBTZ6

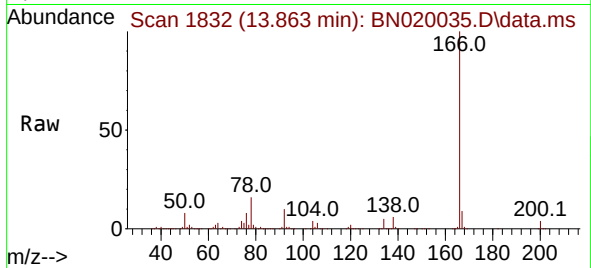

Tgt Ion:165 Resp: 6353
 Ion Ratio Lower Upper
 165 100
 89 0.0 50.6 75.8#
 121 28.2 17.9 26.9#

