

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
 Data File : BN020053.D
 Acq On : 08 Jun 2022 06:44
 Operator : CG/JU
 Sample : N3212-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A52

Quant Time: Jun 08 07:14:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	120007	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	561137	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	371142	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	781494	20.000	ng/u1	0.00
79) Chrysene-d12	21.374	240	761622	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	737279	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	14837	5.355	ng/uL	0.00
4) Pyridine-d5	3.687	84	104777	13.835	ng/u1	0.00
7) Phenol-d5	6.987	99	68323	6.880	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	234086	37.730	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	231322	28.670	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	156274	18.190	ng/u1	0.00
21) Nitrobenzene-d5	8.975	128	166435	38.987	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	172718	38.123	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	279140	35.293	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	471151	36.785	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1157385	42.858	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1274777	40.705	ng/u1	0.00
54) 4-Nitrophenol-d4	14.645	143	37723	6.971	ng/u1	0.00
60) Fluorene-d10	15.439	176	959417	42.934	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	187736	41.471	ng/u1	0.00
73) Anthracene-d10	17.286	188	1535495	45.021	ng/u1	0.00
81) Pyrene-d10	19.580	212	1826668	44.241	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.557	264	1708672	47.367	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.317	88	55698	19.042	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020053.D
Acq On : 08 Jun 2022 06:44
Operator : CG/JU
Sample : N3212-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A52


Quant Time: Jun 08 07:14:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

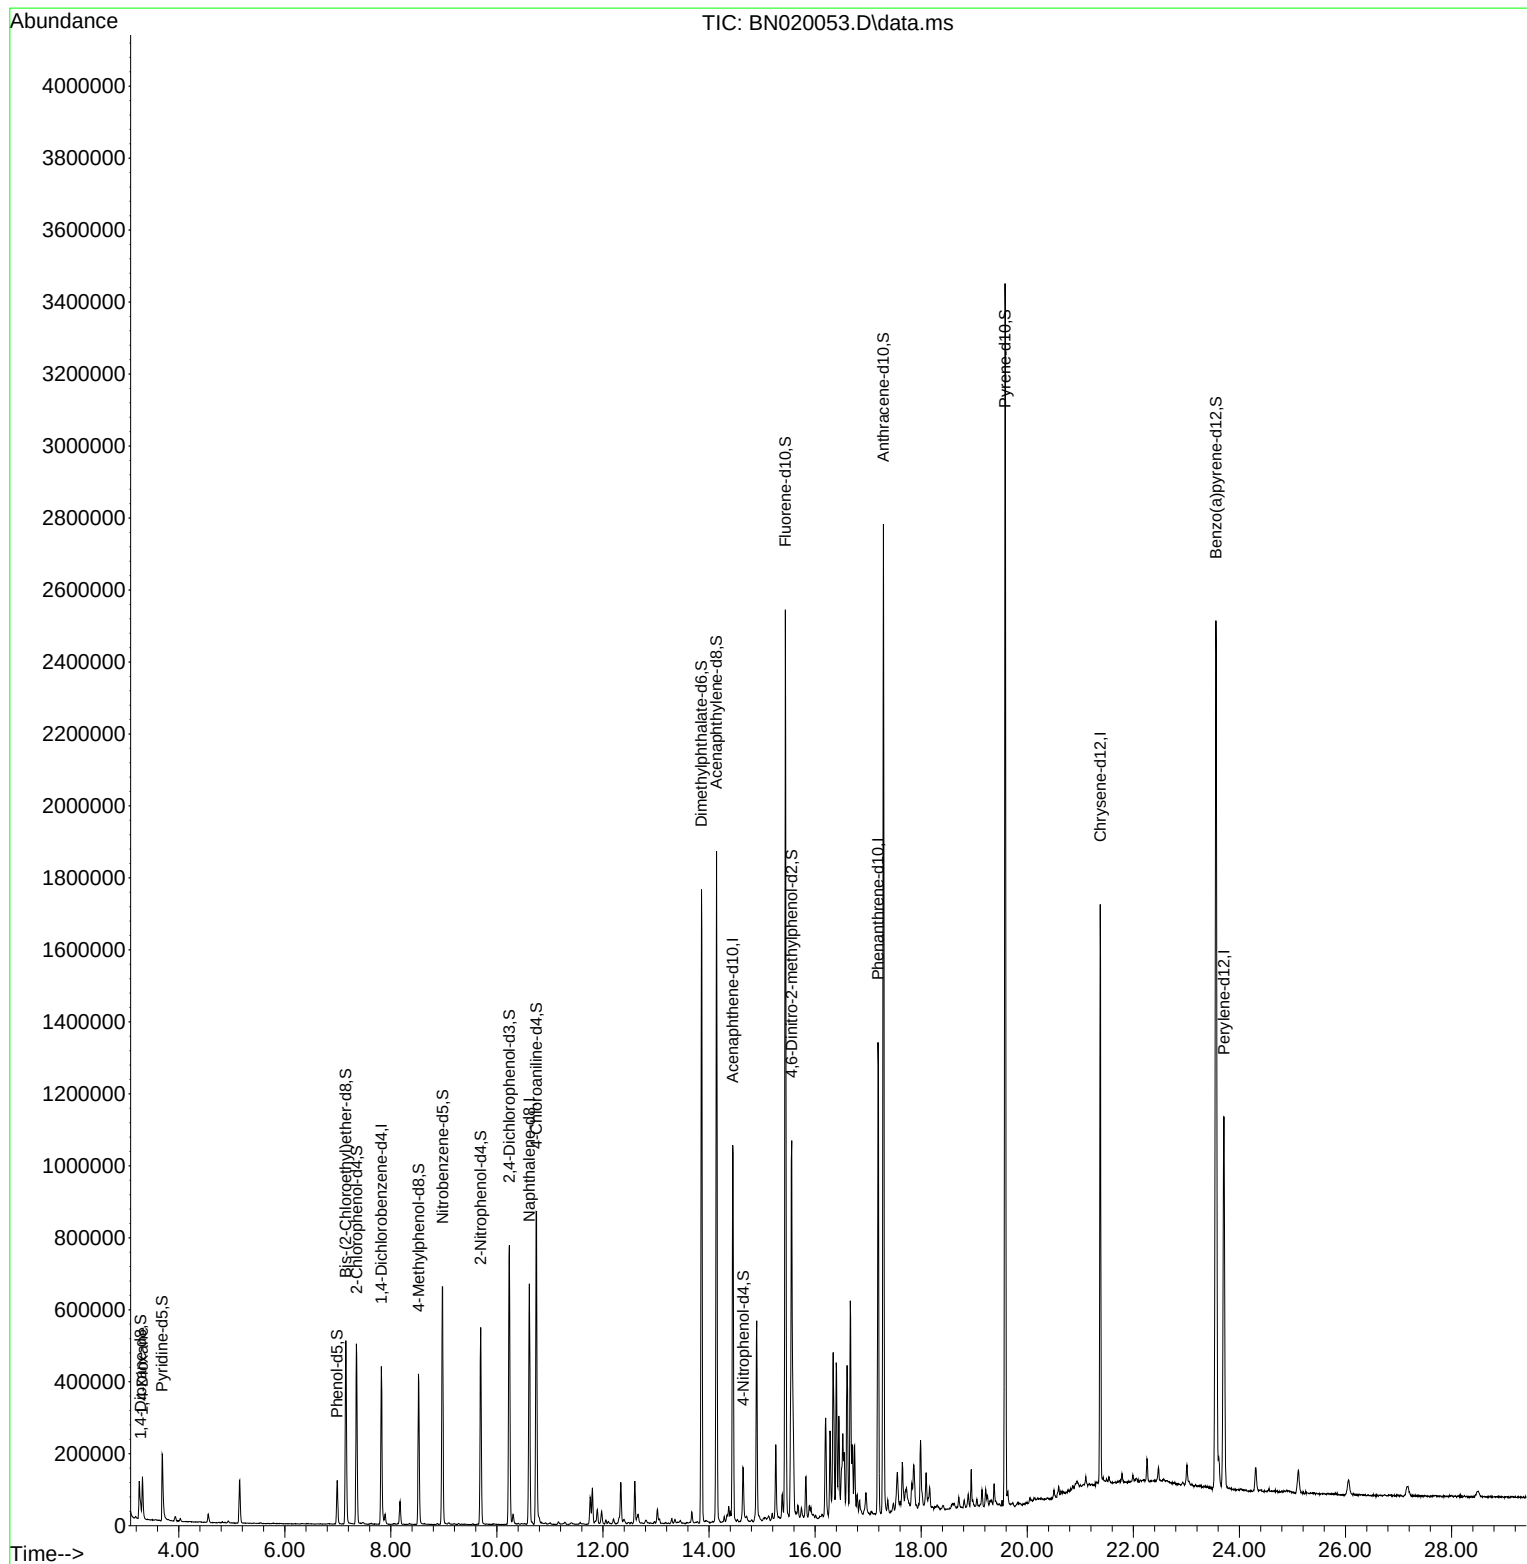

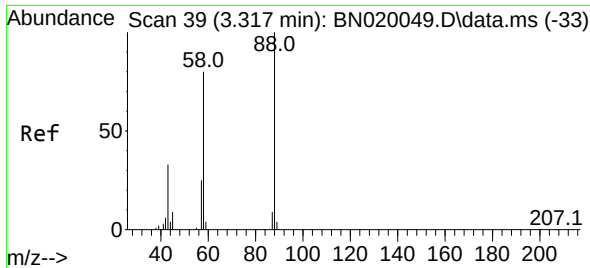

#2
 1,4-Dioxane
 Concen: 19.042 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020053.D
 Acq: 08 Jun 2022 06:44

Instrument :
 BNA_N
 ClientSampleId :
 F5A52

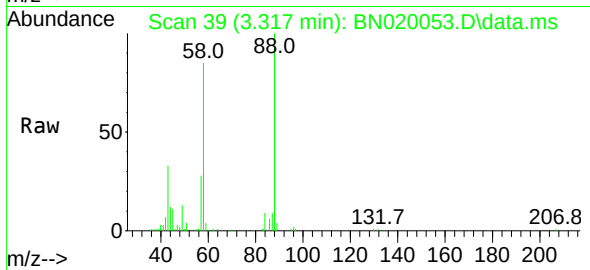

Tgt Ion:	88	Resp:	55698
Ion	Ratio	Lower	Upper
88	100		
43	32.6	22.4	33.6
58	85.0	61.0	91.4

