

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
 Data File : BN020026.D
 Acq On : 07 Jun 2022 09:14
 Operator : CG/JU
 Sample : PB145310BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK310

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	43	rVB	40470	59817	1.08%	0.113%
2	3.687	99	102	122	rBV	524114	977953	17.63%	1.852%
3	4.028	157	160	166	rVB2	10037	12970	0.23%	0.025%
4	6.987	656	663	674	rBV	707569	1178117	21.24%	2.231%
5	7.152	685	691	706	rVB	581953	964904	17.40%	1.827%
6	7.352	718	725	742	rVB	731681	1239468	22.35%	2.347%
7	7.822	798	805	815	rBV	530159	901368	16.25%	1.707%
8	8.522	917	924	936	rBV	943274	1570226	28.31%	2.974%
9	8.969	992	1000	1018	rBV	742930	1277450	23.03%	2.419%
10	9.693	1116	1123	1136	rBV	644112	1080442	19.48%	2.046%
11	10.228	1207	1214	1227	rBV	884549	1538166	27.73%	2.913%
12	10.610	1270	1279	1287	rBV	828079	1430574	25.79%	2.709%
13	10.740	1294	1301	1316	rBV	1078722	1955035	35.25%	3.703%
14	12.199	1543	1549	1558	rBV	13975	25097	0.45%	0.048%
15	13.857	1824	1831	1842	rBV	1855476	2722420	49.08%	5.156%
16	14.140	1872	1879	1893	rBV	1943891	2997012	54.03%	5.676%
17	14.451	1925	1932	1939	rBV	1294758	2005554	36.16%	3.798%
18	14.640	1957	1964	1983	rBV	1010131	1479470	26.67%	2.802%
19	15.440	2093	2100	2108	rBV	2581679	3799503	68.50%	7.196%
20	15.557	2113	2120	2136	rVV	1078569	1476383	26.62%	2.796%
21	15.681	2136	2141	2146	rVB	30224	44794	0.81%	0.085%
22	16.228	2229	2234	2239	rVB4	9456	15320	0.28%	0.029%
23	16.969	2353	2360	2365	rBV4	5961	12099	0.22%	0.023%
24	17.187	2390	2397	2407	rBV	1615979	2491441	44.92%	4.719%
25	17.287	2407	2414	2429	rBV2	2799378	4299283	77.51%	8.143%
26	18.092	2546	2551	2555	rBV5	9816	14625	0.26%	0.028%
27	19.145	2725	2730	2735	rBV2	34479	50431	0.91%	0.096%
28	19.216	2738	2742	2749	rVV	32327	44809	0.81%	0.085%
29	19.375	2765	2769	2775	rBV7	7762	12599	0.23%	0.024%
30	19.586	2798	2805	2817	rBV	3424440	4913327	88.58%	9.306%
31	20.598	2971	2977	2981	rBV3	10213	14946	0.27%	0.028%
32	21.380	3104	3110	3123	rBV	2171533	2839354	51.19%	5.378%
33	21.998	3212	3215	3219	rVB4	16860	19102	0.34%	0.036%
34	22.480	3293	3297	3301	rBV	34956	45330	0.82%	0.086%
35	23.016	3383	3388	3398	rVB2	65732	115665	2.09%	0.219%
36	23.563	3472	3481	3488	rBV2	2758846	5546486	100.00%	10.505%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020026.D
Acq On : 07 Jun 2022 09:14
Operator : CG/JU
Sample : PB145310BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK310

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.710	3498	3506	3528	rVB2	1514148	3038266	54.78%	5.754%
38	24.310	3602	3608	3615	rBV2	89680	186086	3.36%	0.352%
39	25.116	3740	3745	3758	rVB3	90150	216050	3.90%	0.409%
40	26.057	3899	3905	3918	rVB3	62190	187617	3.38%	0.355%




Sum of corrected areas: 52799559

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020026.D
Acq On : 07 Jun 2022 09:14
Operator : CG/JU
Sample : PB145310BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK310

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

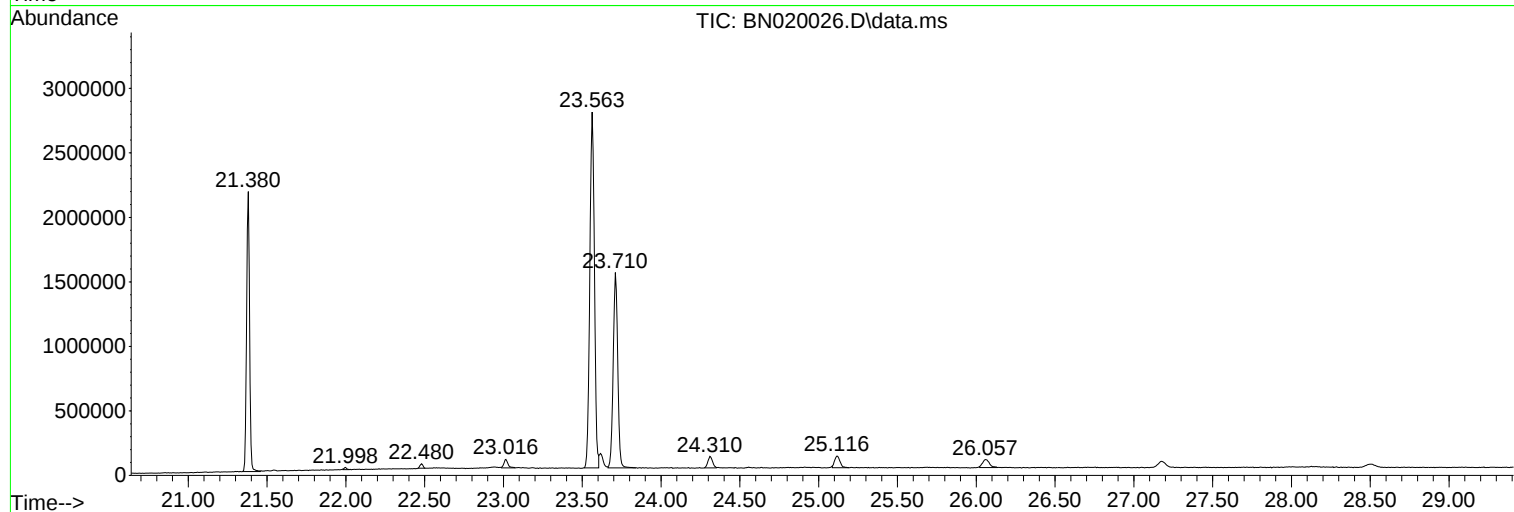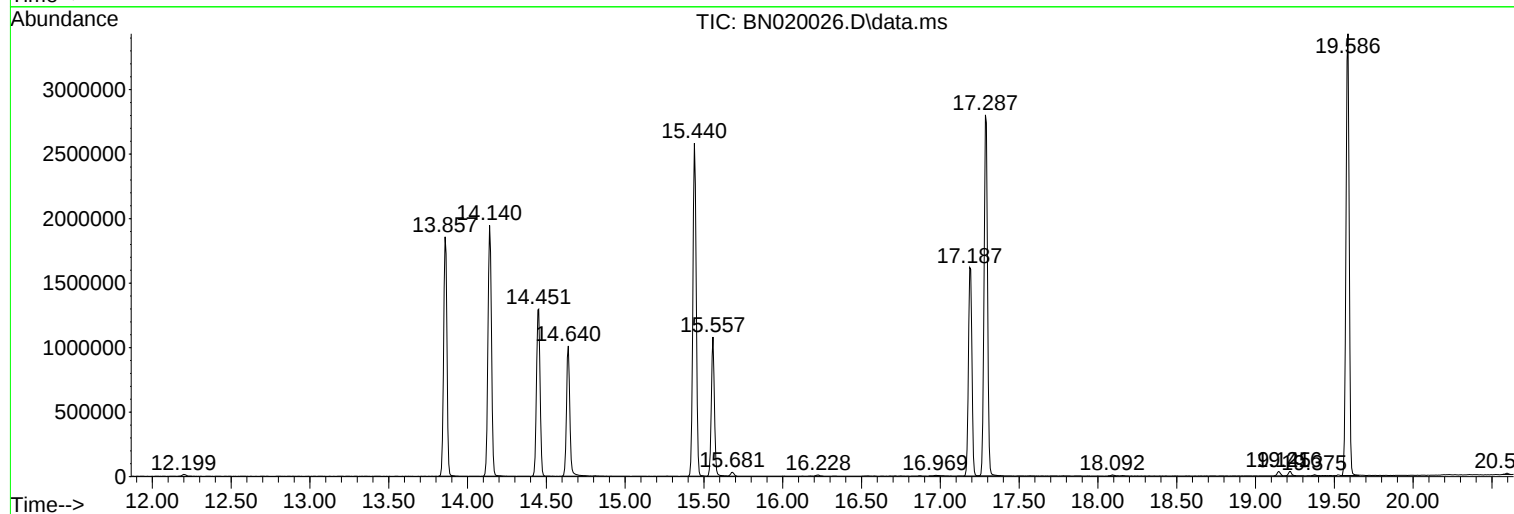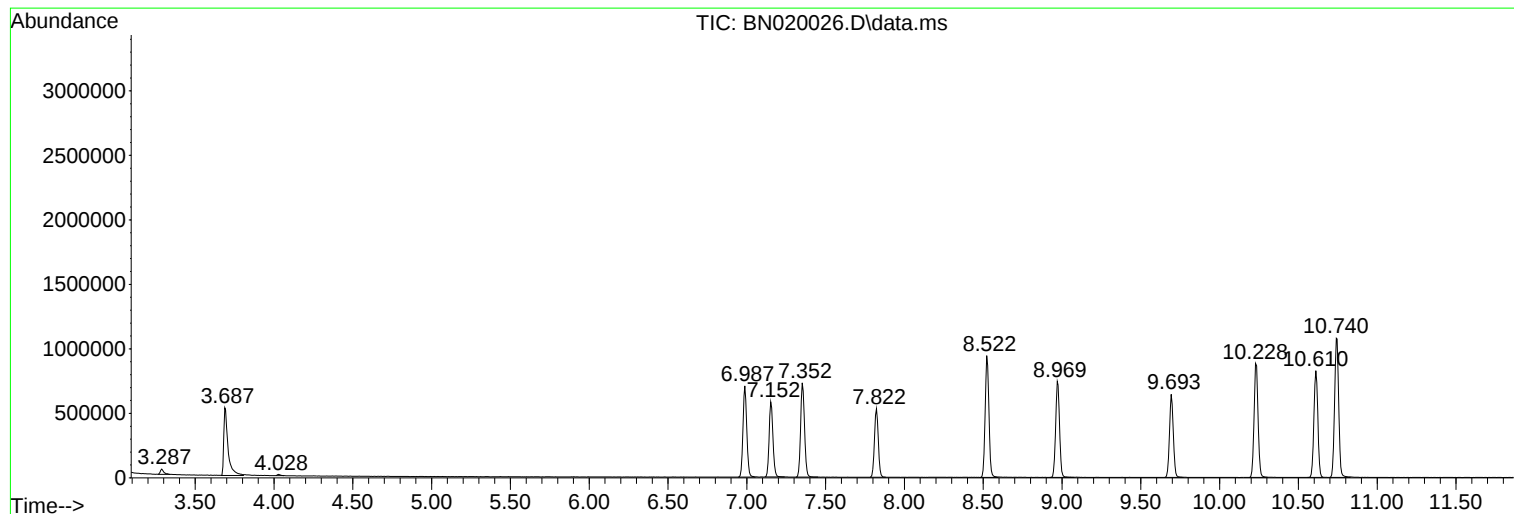

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020026.D
Acq On : 07 Jun 2022 09:14
Operator : CG/JU
Sample : PB145310BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK310

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020026.D
Acq On : 07 Jun 2022 09:14
Operator : CG/JU
Sample : PB145310BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK310

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------