

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
 Data File : BN020029.D
 Acq On : 07 Jun 2022 15:01
 Operator : CG/JU
 Sample : N3195-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.022	155	159	165	rVB2	7531	12598	0.53%	0.128%
2	7.816	796	804	815	rBV	393844	667422	28.10%	6.775%
3	10.610	1271	1279	1290	rBV	584283	1020375	42.95%	10.358%
4	14.451	1925	1932	1943	rBV	962964	1458049	61.38%	14.801%
5	15.463	2098	2104	2110	rVB5	3483	5894	0.25%	0.060%
6	16.169	2218	2224	2227	rBV4	2745	4815	0.20%	0.049%
7	16.328	2247	2251	2255	rVB3	2299	2715	0.11%	0.028%
8	16.516	2278	2283	2286	rBV3	3275	5716	0.24%	0.058%
9	16.633	2298	2303	2307	rBV5	1544	2879	0.12%	0.029%
10	16.716	2314	2317	2320	rVV4	3101	4157	0.17%	0.042%
11	16.969	2354	2360	2362	rBV4	6482	10285	0.43%	0.104%
12	17.022	2366	2369	2372	rVB5	1972	3040	0.13%	0.031%
13	17.128	2383	2387	2391	rVB7	1797	2815	0.12%	0.029%
14	17.192	2391	2398	2408	rBV	1224546	1833491	77.18%	18.613%
15	17.280	2408	2413	2419	rVB6	3458	8223	0.35%	0.083%
16	17.398	2429	2433	2437	rVB3	2172	3384	0.14%	0.034%
17	17.439	2437	2440	2445	rBV6	2663	3757	0.16%	0.038%
18	17.786	2495	2499	2503	rBV4	1733	2676	0.11%	0.027%
19	17.875	2511	2514	2519	rVB5	2491	3537	0.15%	0.036%
20	18.092	2547	2551	2559	rBV5	6646	12284	0.52%	0.125%
21	18.163	2561	2563	2568	rVB4	2703	4288	0.18%	0.044%
22	18.727	2655	2659	2665	rBV6	2952	4560	0.19%	0.046%
23	19.527	2792	2795	2800	rVB6	4507	7108	0.30%	0.072%
24	20.598	2974	2977	2981	rVB2	17430	20787	0.88%	0.211%
25	21.380	3104	3110	3122	rBV	1702870	2277727	95.88%	23.122%
26	23.621	3488	3491	3497	rVB3	25321	39087	1.65%	0.397%
27	23.715	3499	3507	3516	rVV2	1152762	2375530	100.00%	24.115%
28	25.121	3741	3746	3751	rBV4	24223	53583	2.26%	0.544%




Sum of corrected areas: 9850782

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020029.D
Acq On : 07 Jun 2022 15:01
Operator : CG/JU
Sample : N3195-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

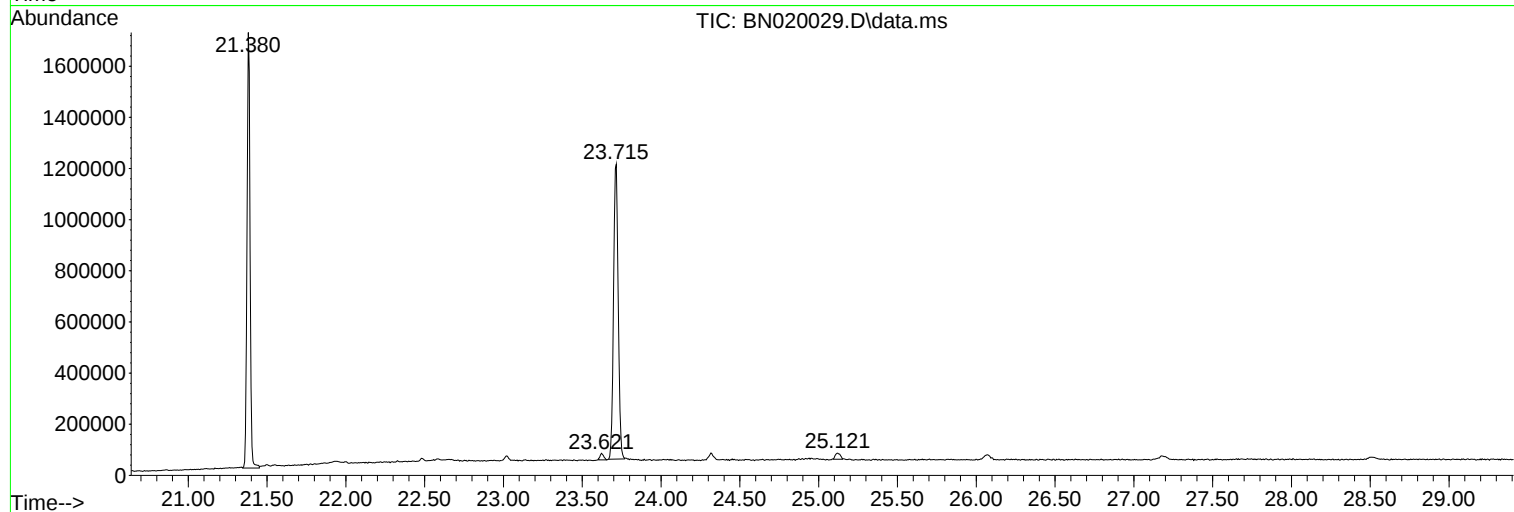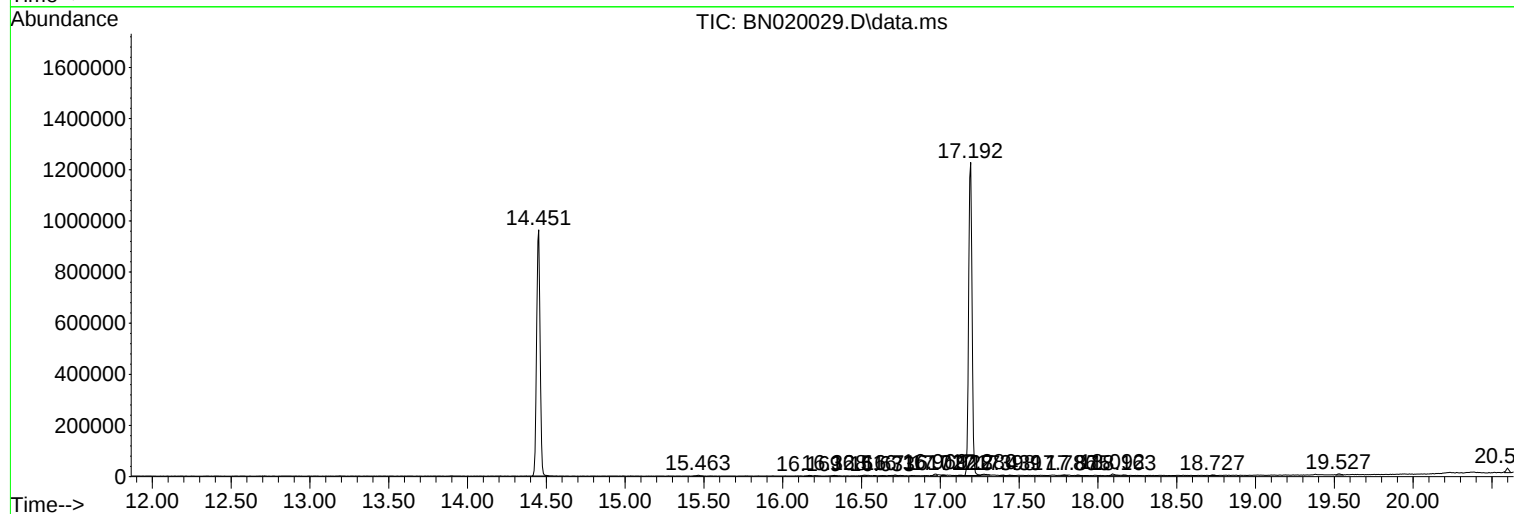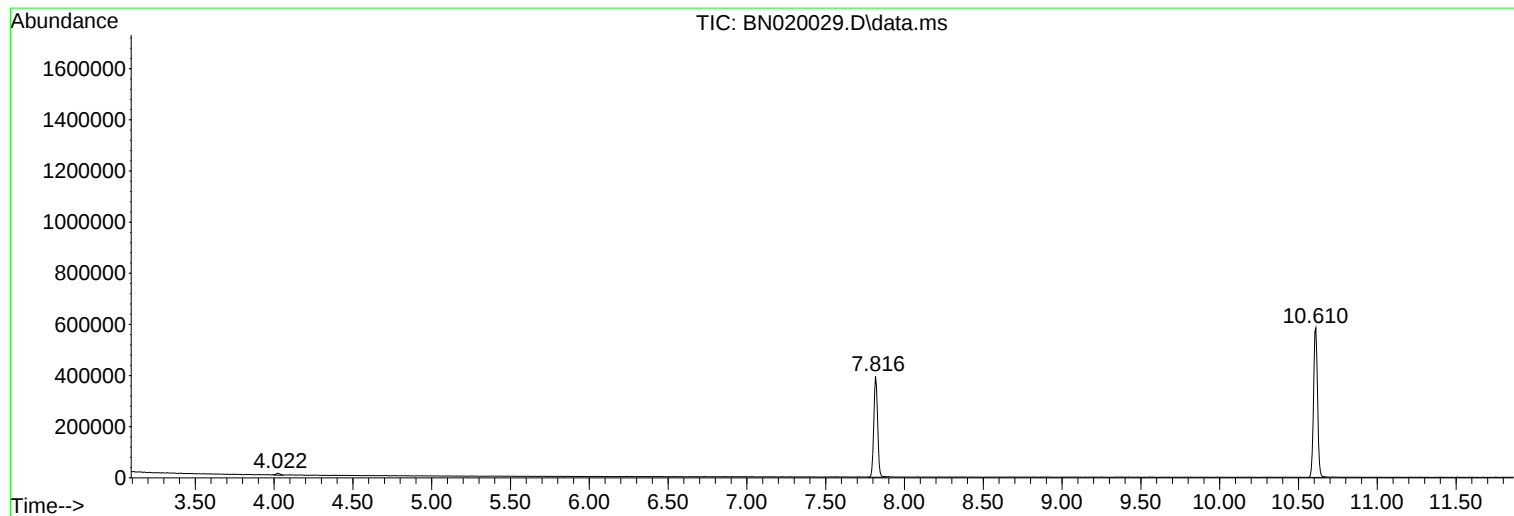

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020029.D
Acq On : 07 Jun 2022 15:01
Operator : CG/JU
Sample : N3195-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020029.D
Acq On : 07 Jun 2022 15:01
Operator : CG/JU
Sample : N3195-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc