

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
 Data File : BN020032.D
 Acq On : 07 Jun 2022 17:27
 Operator : CG/JU
 Sample : PB145285BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK285

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	41	rVB	33762	47700	1.20%	0.116%
2	3.687	99	102	119	rBV	432818	710512	17.95%	1.733%
3	4.028	157	160	164	rVB2	7548	10795	0.27%	0.026%
4	6.987	657	663	677	rBV	536859	868914	21.95%	2.119%
5	7.151	682	691	706	rBV	429248	716994	18.11%	1.748%
6	7.351	719	725	736	rBV	548057	921199	23.27%	2.246%
7	7.822	798	805	815	rBV	489556	811502	20.50%	1.979%
8	8.528	915	925	938	rBV	677104	1158171	29.26%	2.824%
9	8.975	993	1001	1014	rBV	553426	927058	23.42%	2.261%
10	9.692	1117	1123	1140	rBV	445025	775644	19.59%	1.891%
11	10.234	1208	1215	1230	rBV	654089	1121511	28.33%	2.735%
12	10.616	1272	1280	1293	rVB	716825	1269584	32.07%	3.096%
13	10.745	1294	1302	1319	rBV	1097870	1912948	48.32%	4.665%
14	12.204	1545	1550	1557	rBV2	10395	17480	0.44%	0.043%
15	13.863	1825	1832	1845	rBV	1342238	1970447	49.77%	4.805%
16	14.145	1871	1880	1888	rBV	1416369	2186879	55.24%	5.333%
17	14.451	1925	1932	1939	rBV	1207002	1770282	44.72%	4.317%
18	14.639	1957	1964	1982	rBV	698805	1033698	26.11%	2.521%
19	15.439	2093	2100	2110	rBV	1850086	2794726	70.60%	6.815%
20	15.557	2114	2120	2134	rVV	755442	1051827	26.57%	2.565%
21	15.680	2136	2141	2146	rVB2	23103	31847	0.80%	0.078%
22	16.222	2229	2233	2238	rVV4	6054	8520	0.22%	0.021%
23	17.192	2391	2398	2406	rBV	1451706	2140176	54.06%	5.219%
24	17.286	2408	2414	2428	rBV2	2131729	3207679	81.03%	7.822%
25	18.092	2547	2551	2555	rBV3	6448	10073	0.25%	0.025%
26	18.157	2559	2562	2567	rVB5	2589	4079	0.10%	0.010%
27	19.151	2725	2731	2737	rBV2	25058	34366	0.87%	0.084%
28	19.216	2738	2742	2749	rVV	22707	31254	0.79%	0.076%
29	19.374	2766	2769	2775	rBV3	3608	5259	0.13%	0.013%
30	19.527	2791	2795	2798	rBV5	5010	6254	0.16%	0.015%
31	19.580	2798	2804	2815	rVV	2516370	3665299	92.59%	8.938%
32	20.192	2904	2908	2909	rBV3	4171	4820	0.12%	0.012%
33	20.598	2971	2977	2980	rBV3	10234	14010	0.35%	0.034%
34	21.380	3104	3110	3120	rBV	1797532	2421291	61.16%	5.905%
35	22.480	3293	3297	3303	rVB3	30544	43262	1.09%	0.105%
36	23.015	3384	3388	3394	rVB	56491	86489	2.18%	0.211%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020032.D
Acq On : 07 Jun 2022 17:27
Operator : CG/JU
Sample : PB145285BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.562	3472	3481	3488	rBV	1983636	3958768	100.00%	9.654%
38	23.615	3488	3490	3497	rVV	98107	159730	4.03%	0.390%
39	23.709	3498	3506	3525	rVB	1249543	2573406	65.01%	6.276%
40	24.315	3603	3609	3617	rVB2	81835	169584	4.28%	0.414%
41	25.115	3739	3745	3753	rVB2	85338	193238	4.88%	0.471%
42	26.062	3900	3906	3916	rVB3	62114	159708	4.03%	0.389%




Sum of corrected areas: 41006983

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020032.D
Acq On : 07 Jun 2022 17:27
Operator : CG/JU
Sample : PB145285BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

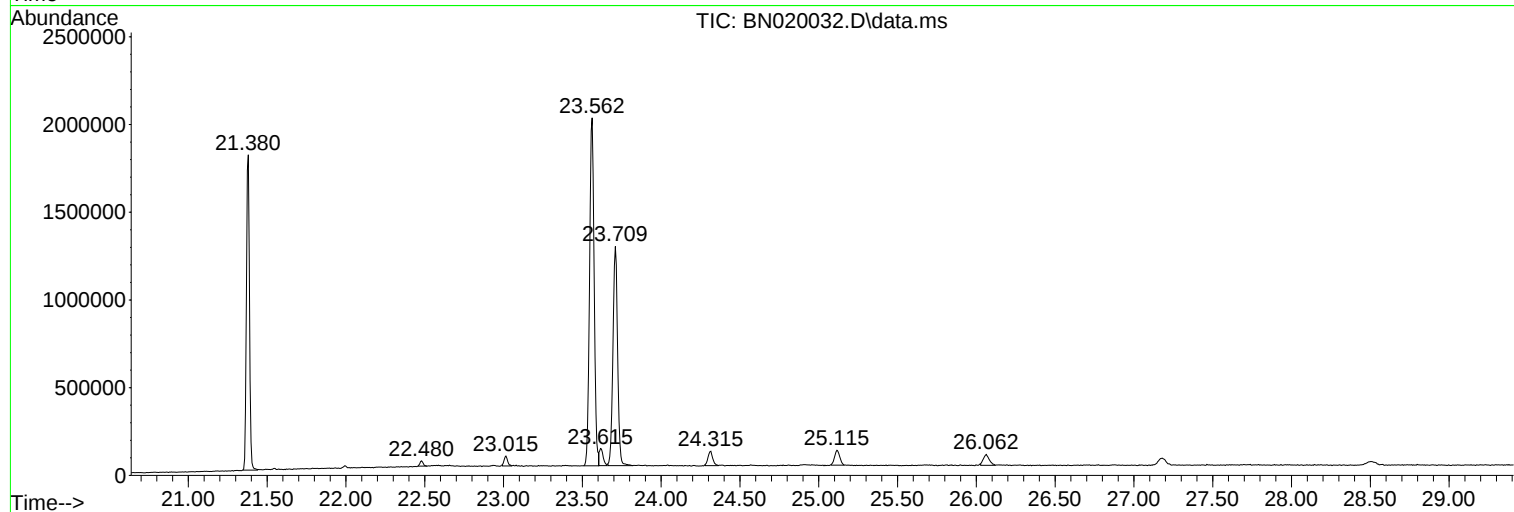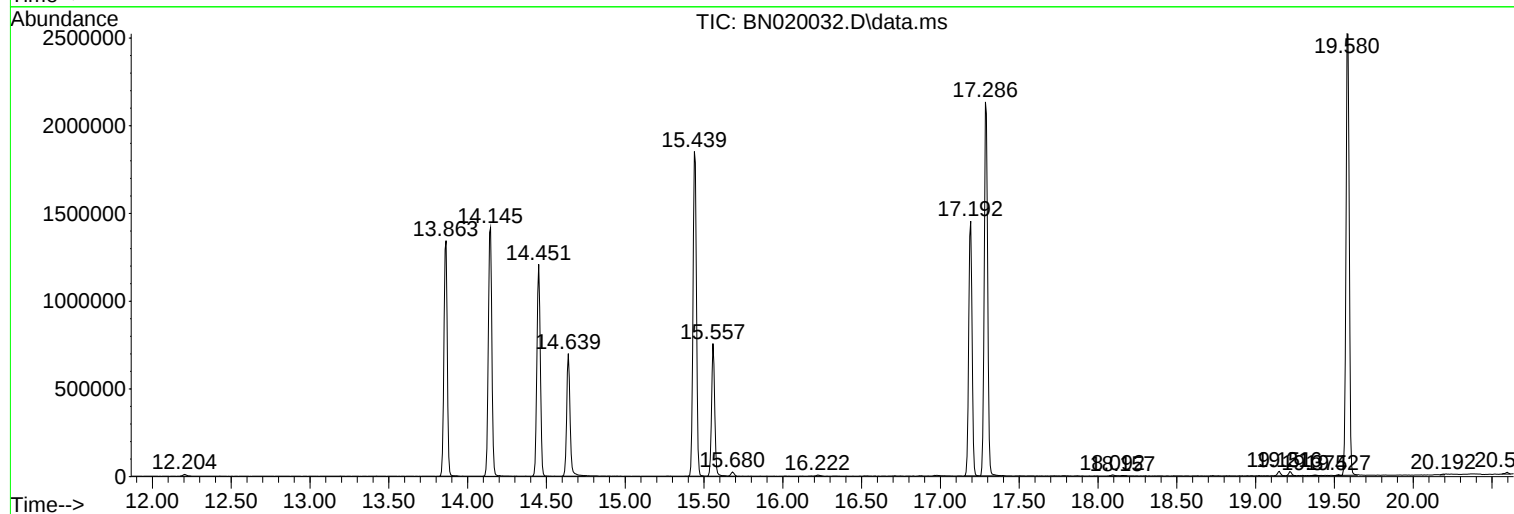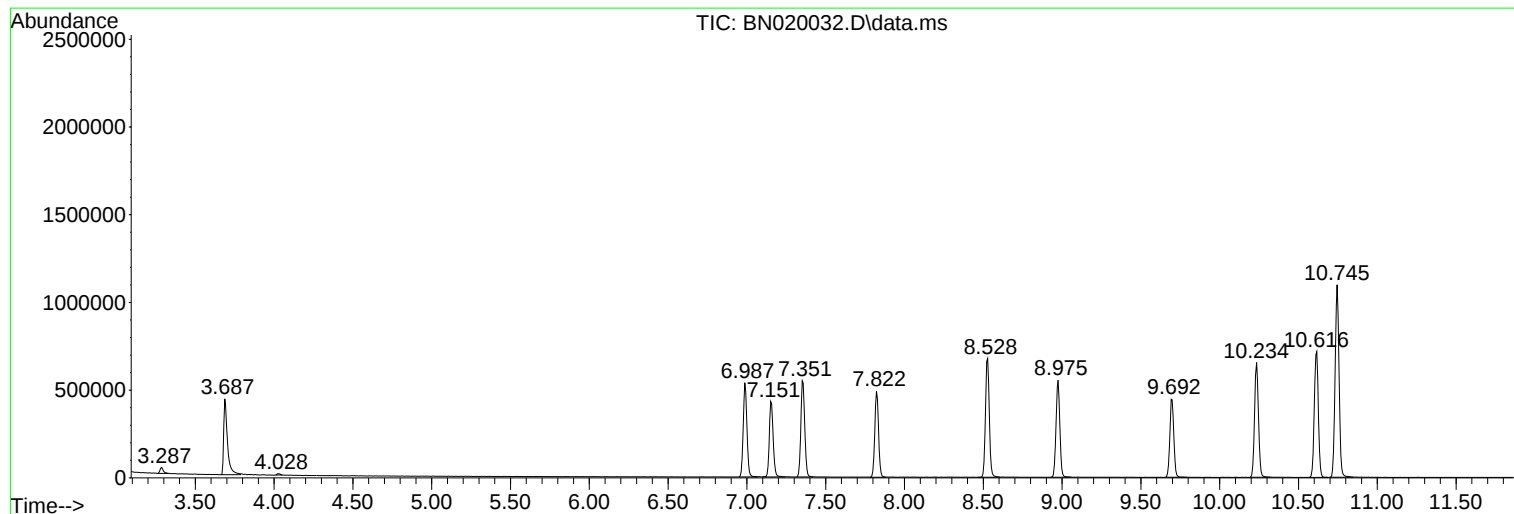

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020032.D
Acq On : 07 Jun 2022 17:27
Operator : CG/JU
Sample : PB145285BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020032.D
Acq On : 07 Jun 2022 17:27
Operator : CG/JU
Sample : PB145285BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK285

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------