

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
 Data File : BN020033.D
 Acq On : 07 Jun 2022 18:04
 Operator : CG/JU
 Sample : PB145287BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK287

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020033.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	44	rVB	40169	65665	1.36%	0.144%
2	3.687	99	102	119	rBV	517022	851082	17.66%	1.871%
3	4.028	157	160	167	rVB3	8462	12053	0.25%	0.026%
4	6.987	655	663	676	rBV	629255	1032259	21.42%	2.269%
5	7.152	682	691	704	rBV	507420	848357	17.60%	1.865%
6	7.358	719	726	734	rBV	636349	1080000	22.41%	2.374%
7	7.822	798	805	815	rVB	471318	779878	16.18%	1.714%
8	8.528	918	925	939	rBV	830235	1385083	28.73%	3.044%
9	8.975	994	1001	1012	rBV	660403	1108495	23.00%	2.436%
10	9.699	1115	1124	1137	rBV	541753	935615	19.41%	2.056%
11	10.234	1205	1215	1232	rBV	785681	1341934	27.84%	2.950%
12	10.610	1272	1279	1288	rBV	686537	1222751	25.37%	2.688%
13	10.746	1294	1302	1315	rBV	1111242	1934629	40.14%	4.252%
14	12.204	1543	1550	1556	rBV2	12413	20141	0.42%	0.044%
15	13.863	1825	1832	1843	rBV	1615059	2319794	48.13%	5.099%
16	14.140	1872	1879	1894	rBV	1660779	2598964	53.92%	5.712%
17	14.451	1925	1932	1939	rBV	1145973	1710245	35.48%	3.759%
18	14.640	1957	1964	1983	rBV	878273	1263081	26.20%	2.776%
19	15.440	2093	2100	2114	rBV	2217067	3316729	68.81%	7.290%
20	15.557	2114	2120	2136	rVV	916559	1291868	26.80%	2.839%
21	15.681	2136	2141	2146	rVB	25530	39124	0.81%	0.086%
22	16.222	2227	2233	2238	rVB3	8048	11651	0.24%	0.026%
23	16.981	2356	2362	2366	rBV3	3495	8206	0.17%	0.018%
24	17.192	2391	2398	2407	rVB	1404989	2068994	42.92%	4.548%
25	17.292	2408	2415	2427	rBV	2537243	3795477	78.74%	8.342%
26	18.092	2545	2551	2557	rBV6	7496	13526	0.28%	0.030%
27	19.151	2726	2731	2737	rVB	30710	42190	0.88%	0.093%
28	19.222	2737	2743	2750	rBV	29277	41556	0.86%	0.091%
29	19.381	2765	2770	2774	rBV6	6285	10178	0.21%	0.022%
30	19.528	2792	2795	2798	rVB3	5382	5750	0.12%	0.013%
31	19.586	2798	2805	2818	rBV	3007556	4378137	90.83%	9.623%
32	20.592	2969	2976	2981	rBV4	14158	27905	0.58%	0.061%
33	21.375	3104	3109	3123	rBV	1745619	2397412	49.74%	5.269%
34	23.010	3383	3387	3393	rBV3	24398	41619	0.86%	0.091%
35	23.563	3472	3481	3489	rBV	2343962	4820241	100.00%	10.595%
36	23.710	3498	3506	3519	rVB2	1202980	2508626	52.04%	5.514%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020033.D
Acq On : 07 Jun 2022 18:04
Operator : CG/JU
Sample : PB145287BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK287

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	24.310	3603	3608	3615	rVB3	37152	76569	1.59%	0.168%
38	25.116	3740	3745	3752	rVB4	39360	91007	1.89%	0.200%




Sum of corrected areas: 45496791

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020033.D
Acq On : 07 Jun 2022 18:04
Operator : CG/JU
Sample : PB145287BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

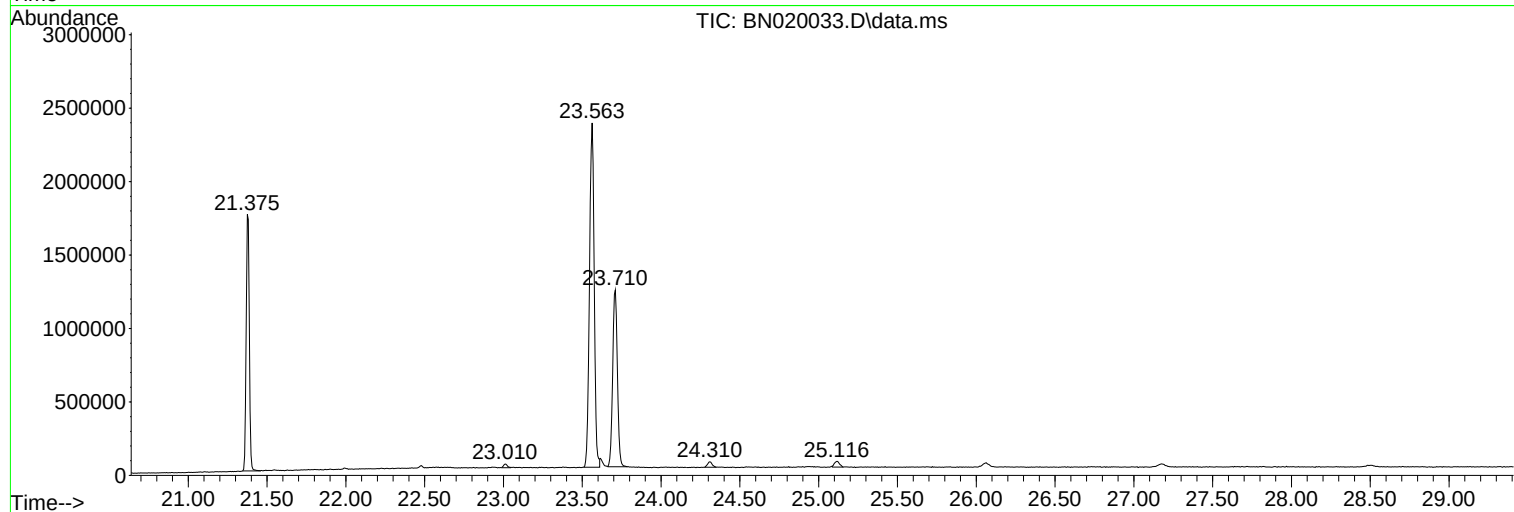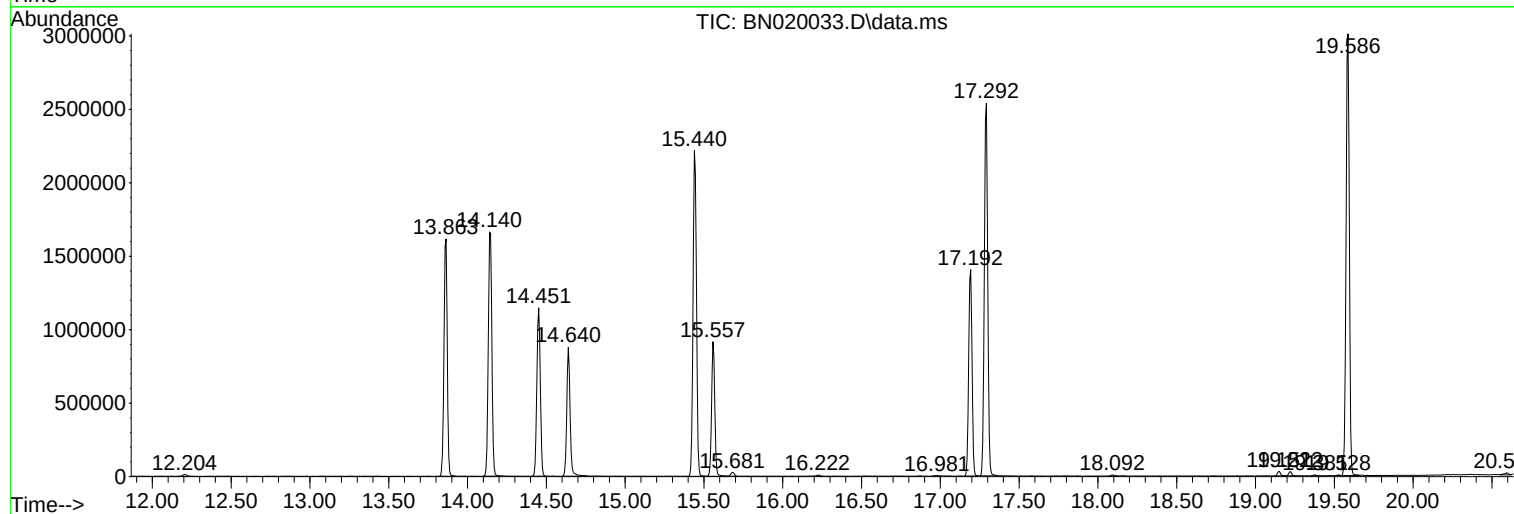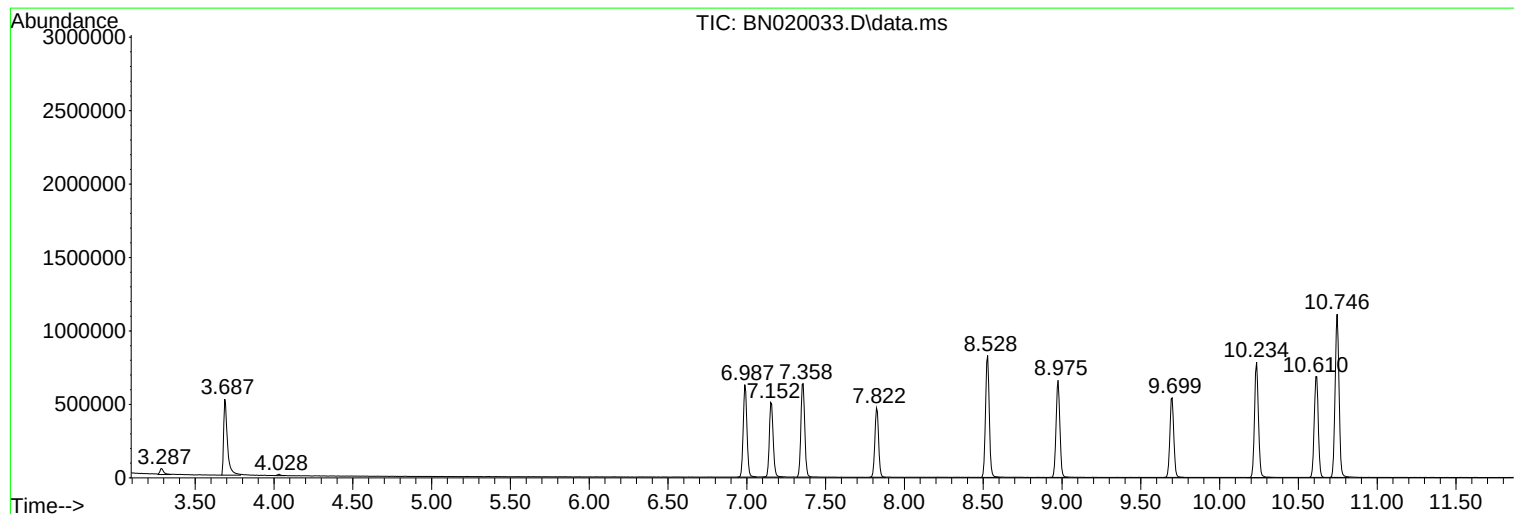

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020033.D
Acq On : 07 Jun 2022 18:04
Operator : CG/JU
Sample : PB145287BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060722\
Data File : BN020033.D
Acq On : 07 Jun 2022 18:04
Operator : CG/JU
Sample : PB145287BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK287

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc