

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006321.D
 Acq On : 13 Jun 2019 21:08
 Operator : JU/SJ
 Sample : K3213-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 14 01:06:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4244	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15932	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	8606	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.15	188	1392113	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.27
20) Perylene-d12	23.36	264	1235915	0.40	ng/ul	-0.13
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	7356	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.35	166	1677	0.043	ng/ul#	81




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006321.D
Acq On : 13 Jun 2019 21:08
Operator : JU/SJ
Sample : K3213-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 14 01:06:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

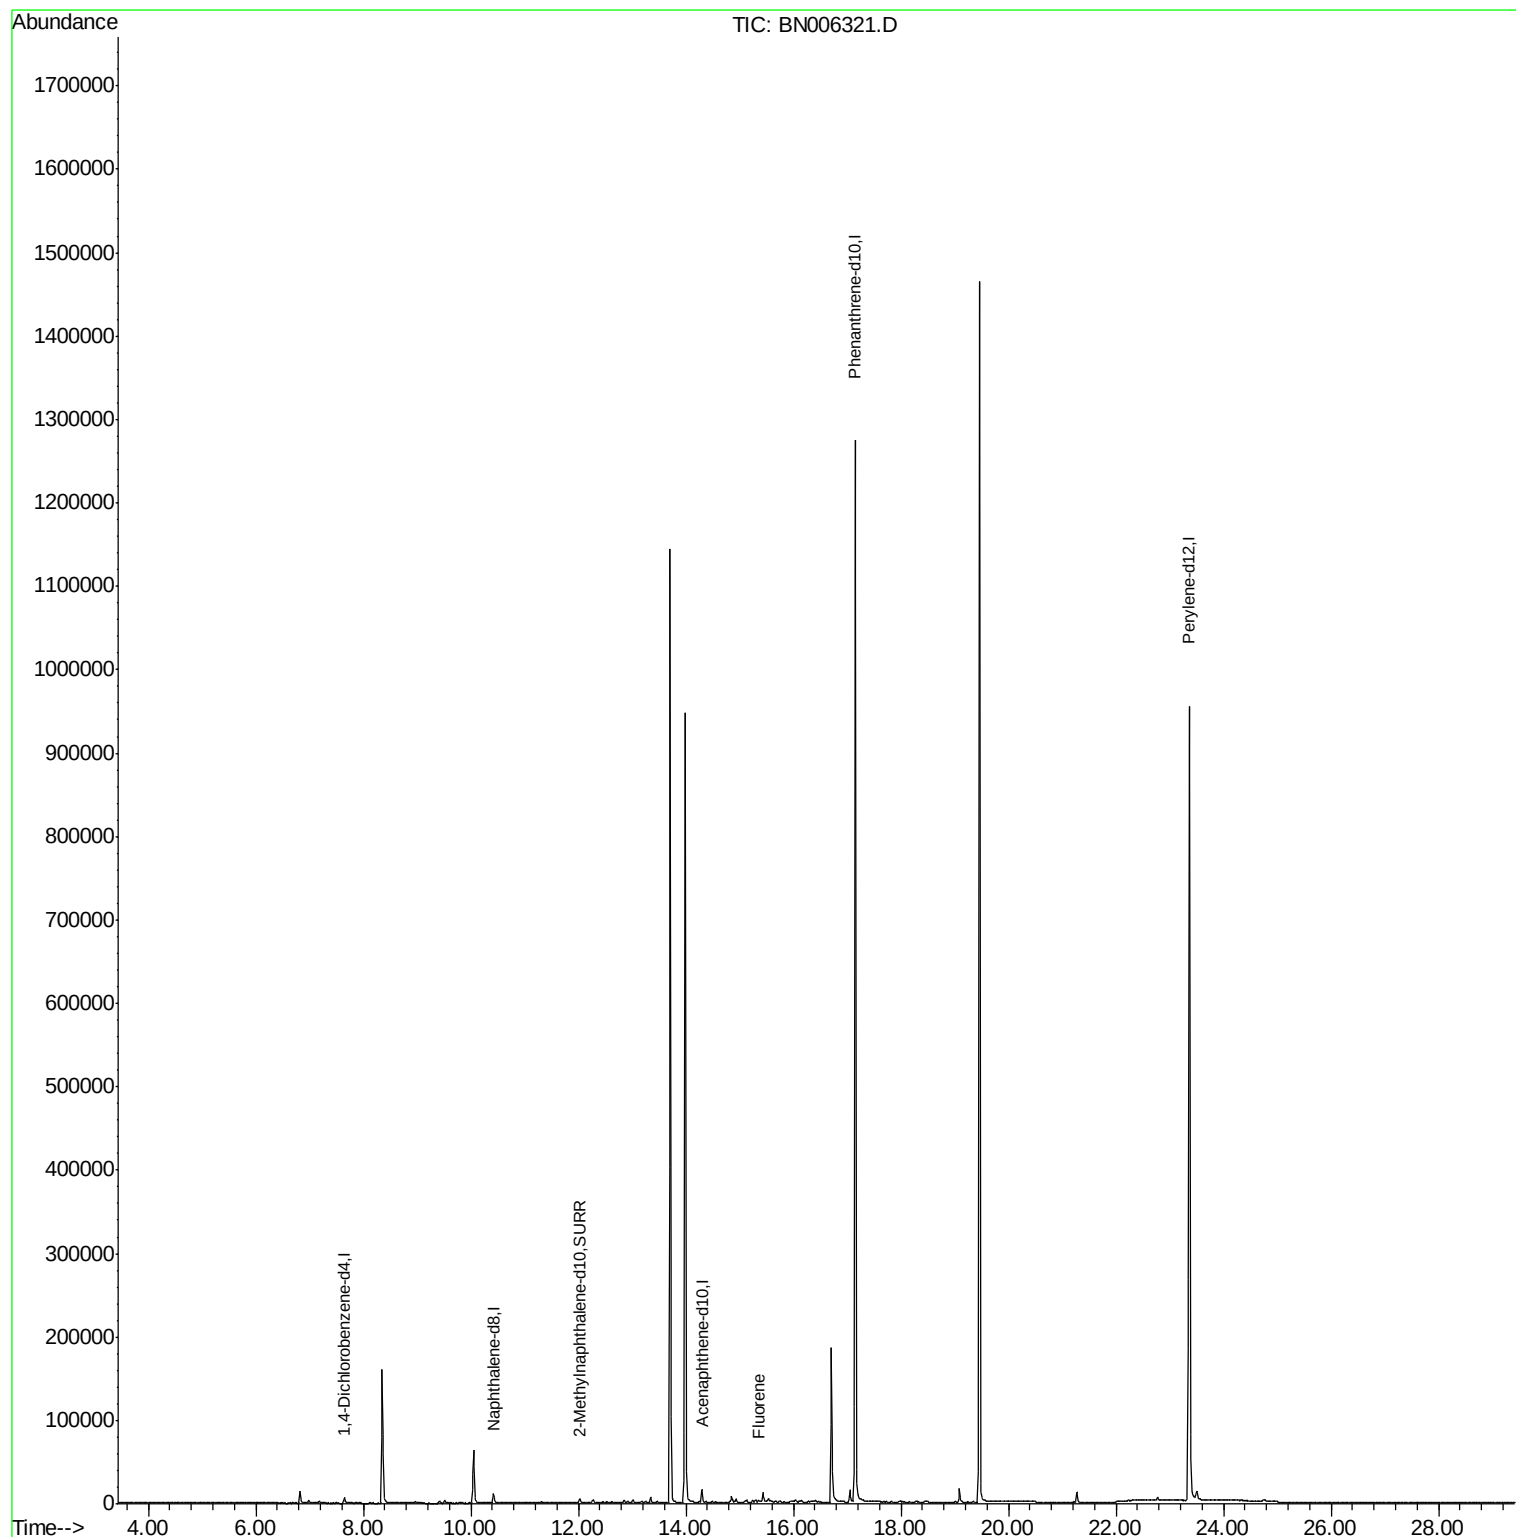

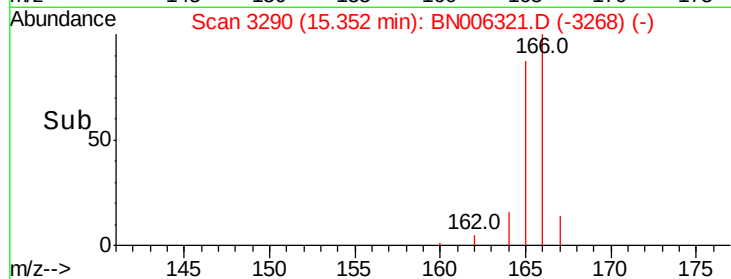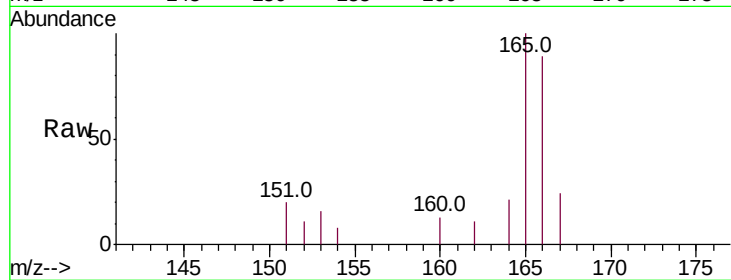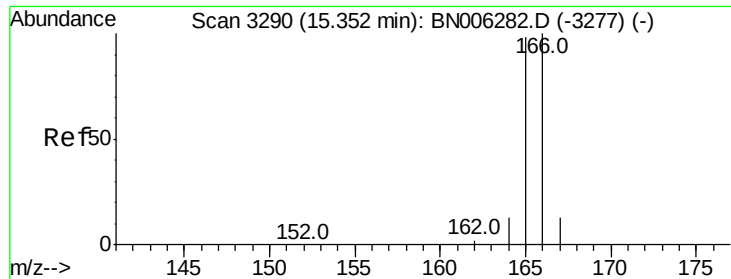

#9

Fluorene

Concen: 0.043 ng/ul

RT: 15.35 min Scan# 3290

Delta R.T. -0.00 min

Lab File: BN006321.D

Acq: 13 Jun 2019 21:08

Instrument :

BNA_N

ClientSampleId :

Tot Ion:166 Resp: 1677

Ion Ratio Lower Upper

166 100

165 112.7 76.4 114.6

167 26.8 11.0 16.6#

