


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006320.D
Acq On : 13 Jun 2019 20:34
Operator : JU/SJ
Sample : K3213-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB8K5

Manual Integrations
APPROVED

mohammad
6/14/2019 8:49:35 AM

Quant Time: Jun 14 02:00:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

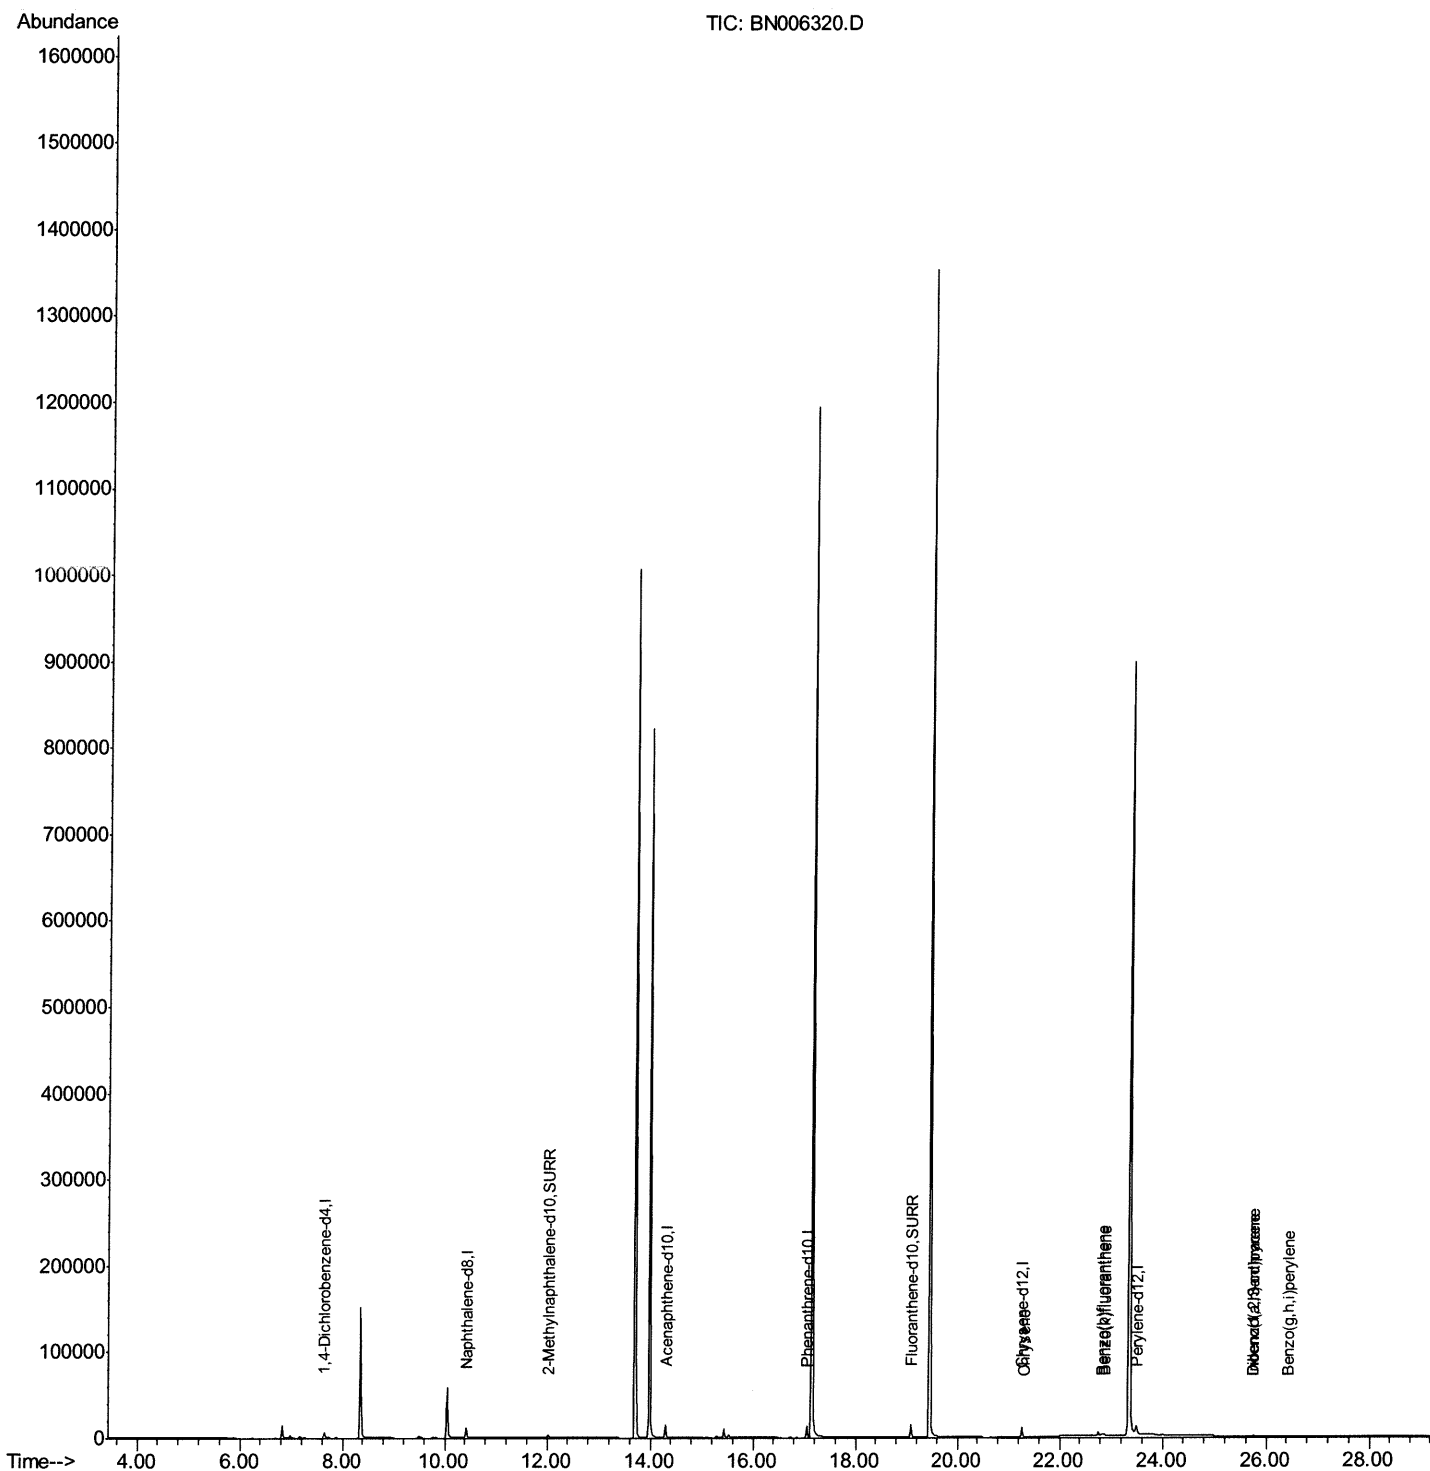

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:06:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

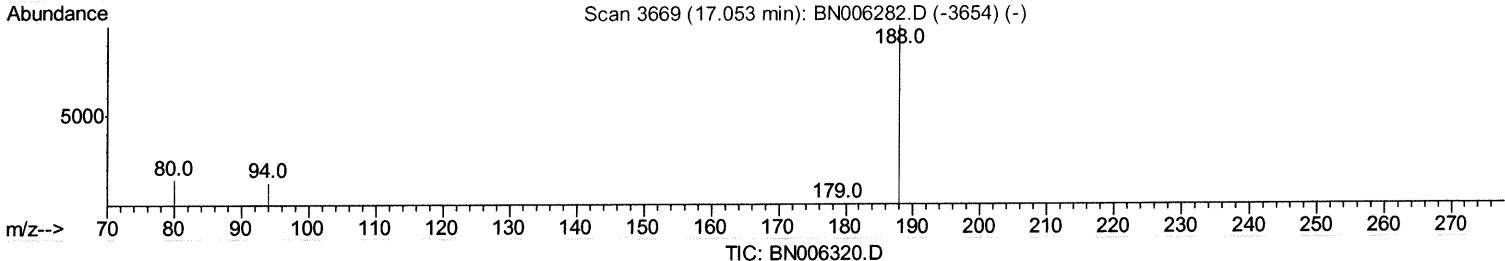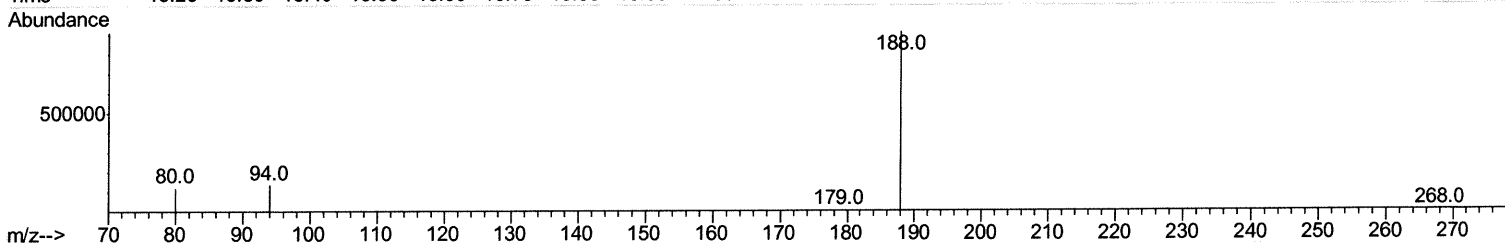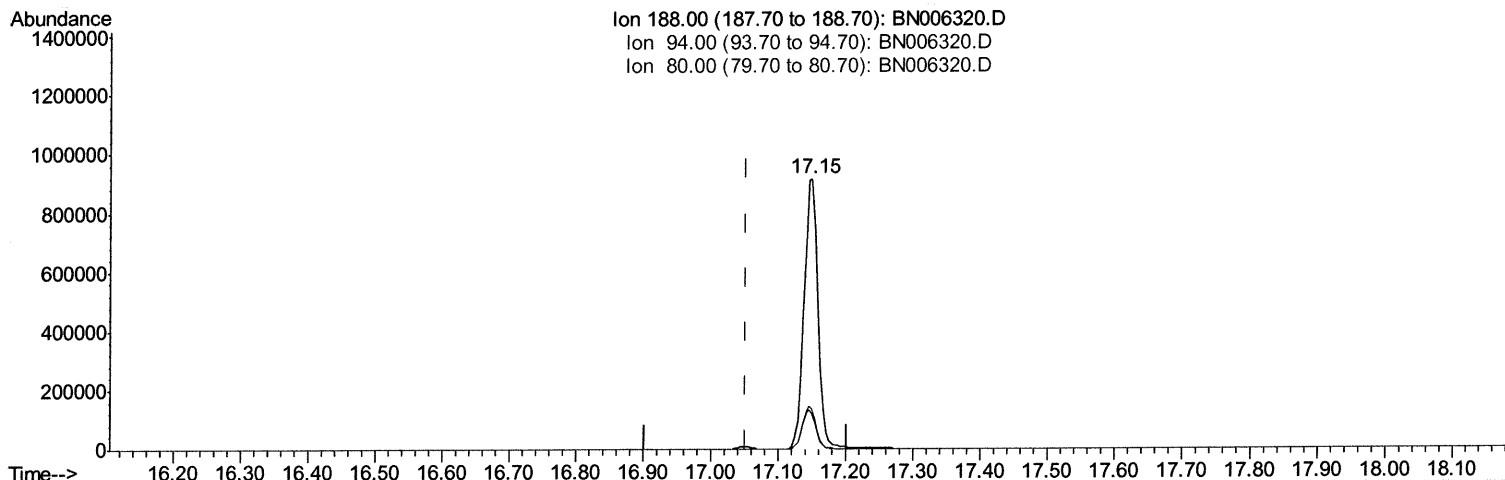

(10) Phenanthrene-d10 (I)

17.149min (+0.097) 0.40ng/ul

response 1293417

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	14.83
80.00	13.60	13.25
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:06:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

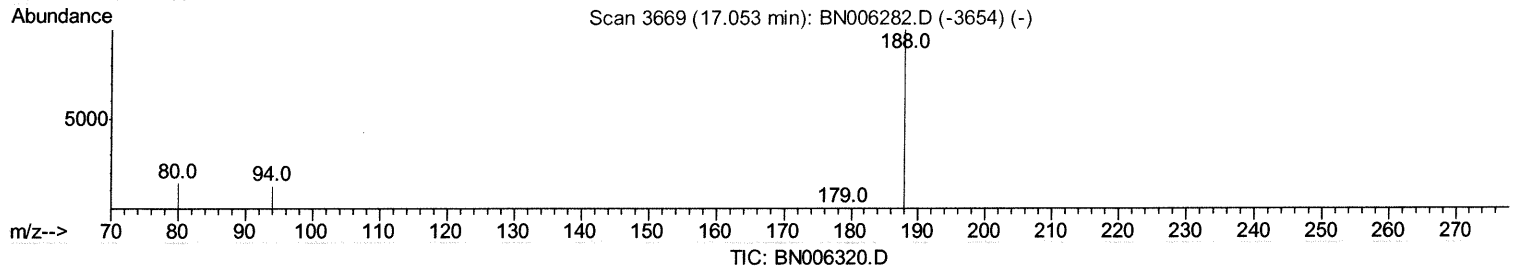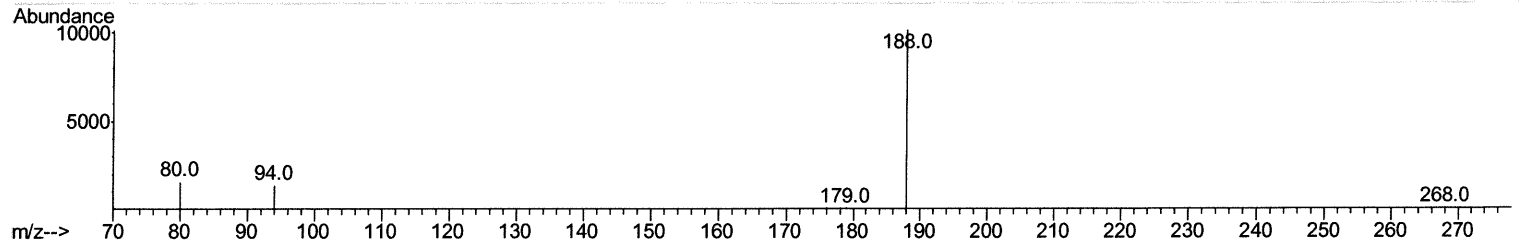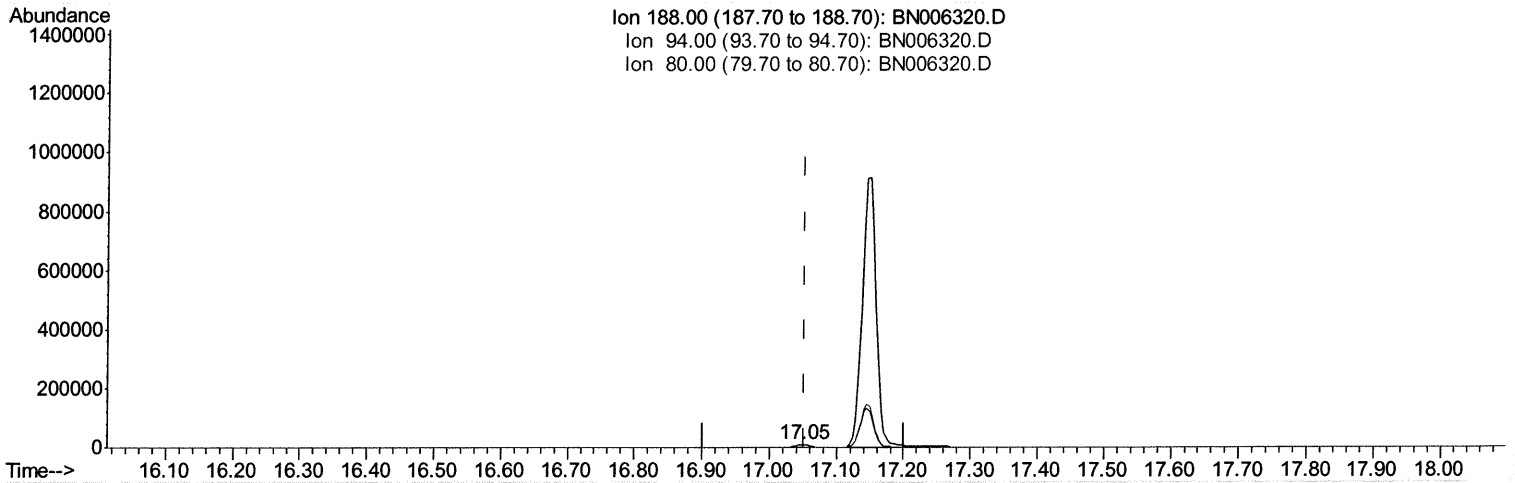

(10) Phenanthrene-d10 (I)

17.048min (-0.004) 0.40ng/ul m *JU* 06/14/19

response 15055

Ion	Exp%	Act%
188.00	100	100
94.00	13.00	13.66
80.00	13.60	15.54
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006320.D
Acq On : 13 Jun 2019 20:34
Operator : JU/SJ
Sample : K3213-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB8K5

Manual Integrations
APPROVED

mohammad
6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:54:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

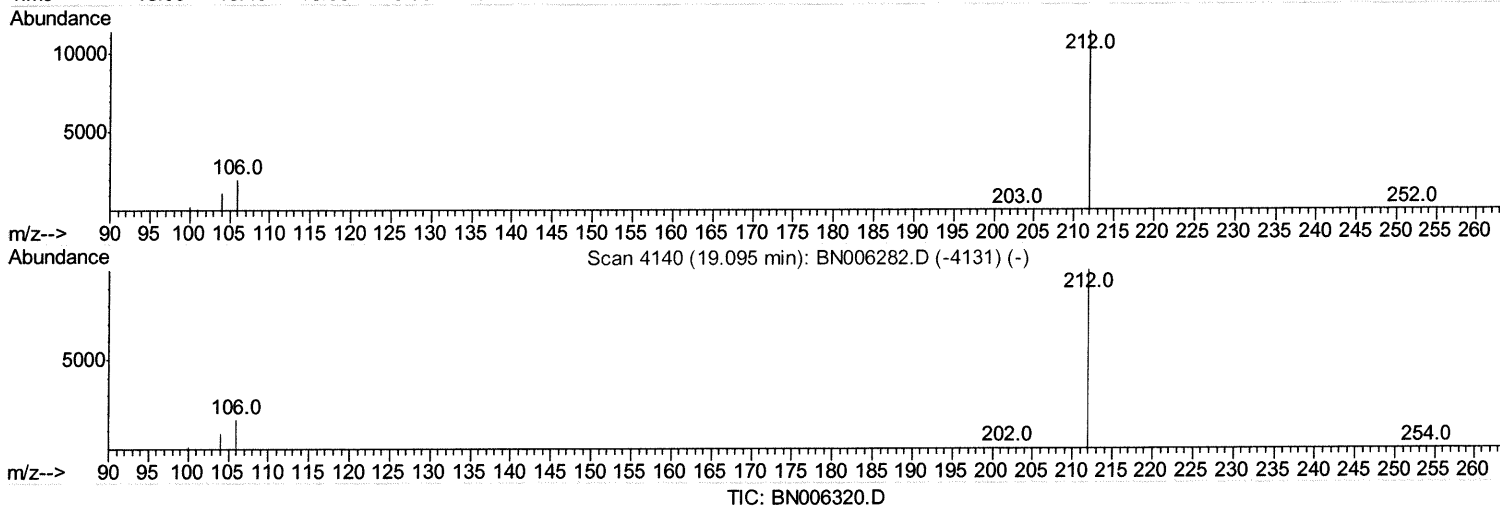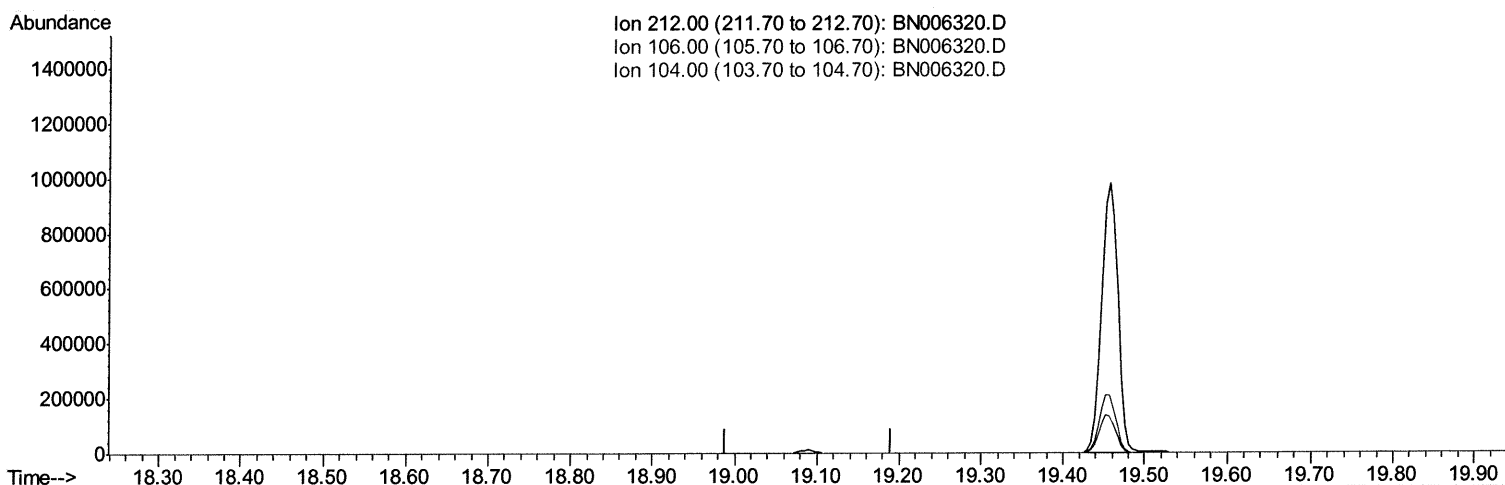

(14) Fluoranthene-d10 (SURR)

19.090min (-19.090) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:54:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

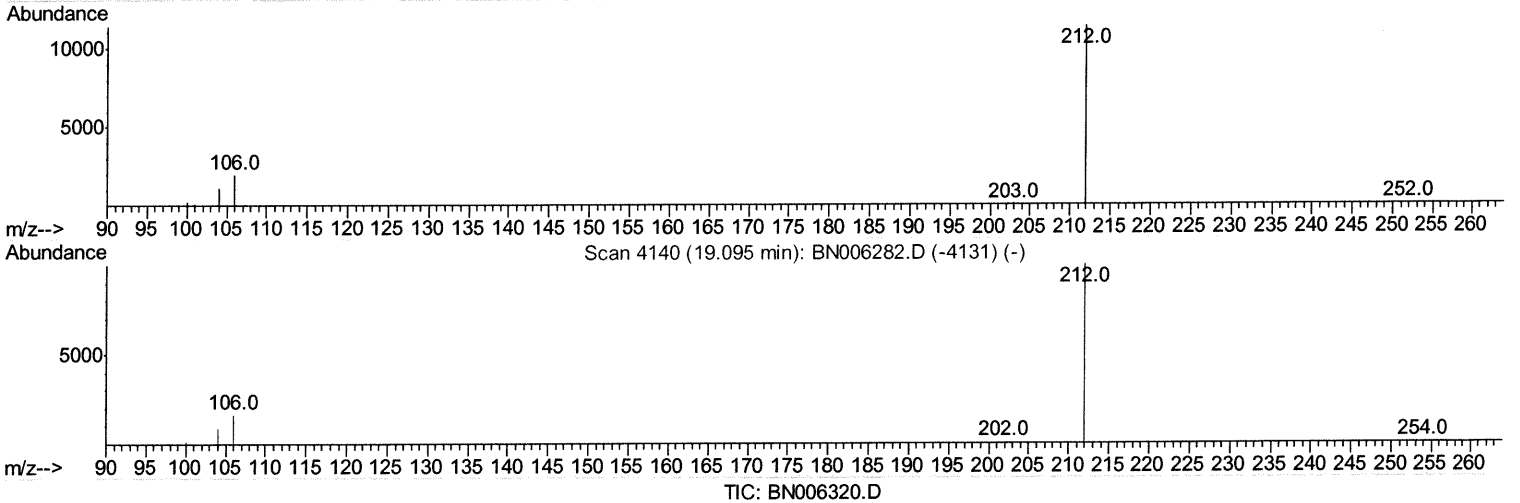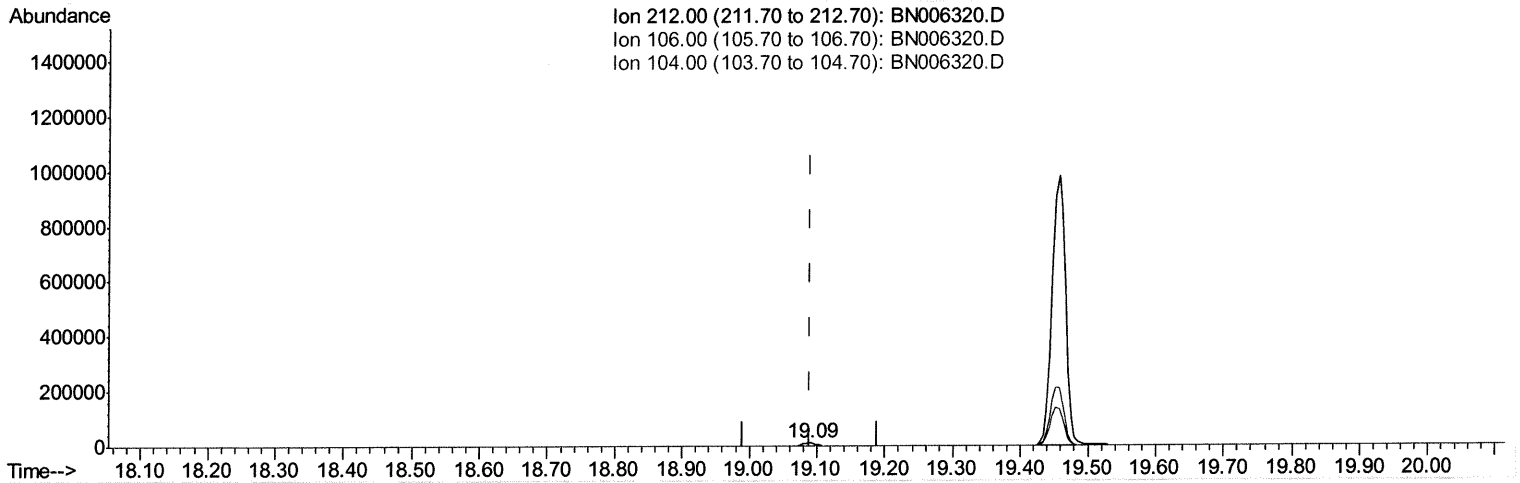

(14) Fluoranthene-d10 (SURR)

19.090min (-0.001) 0.38ng/ul m *JU 06/14/19*

response 15480

Ion	Exp%	Act%
212.00	100	100
106.00	18.10	0.00#
104.00	9.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:54:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

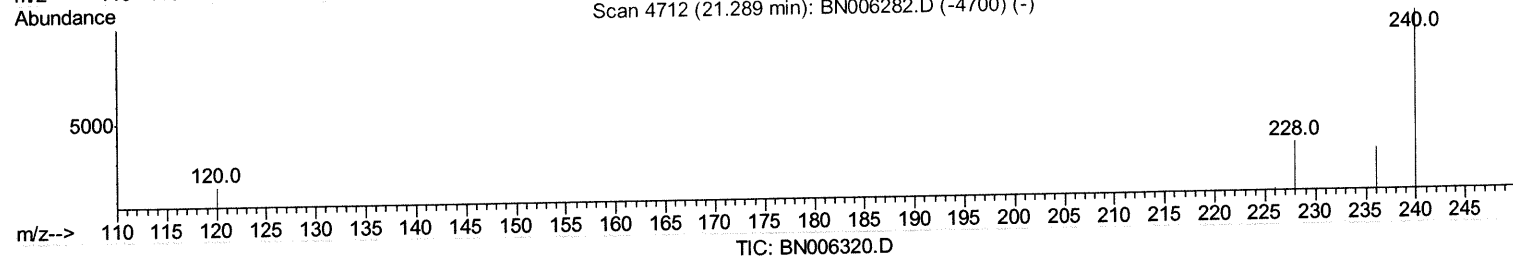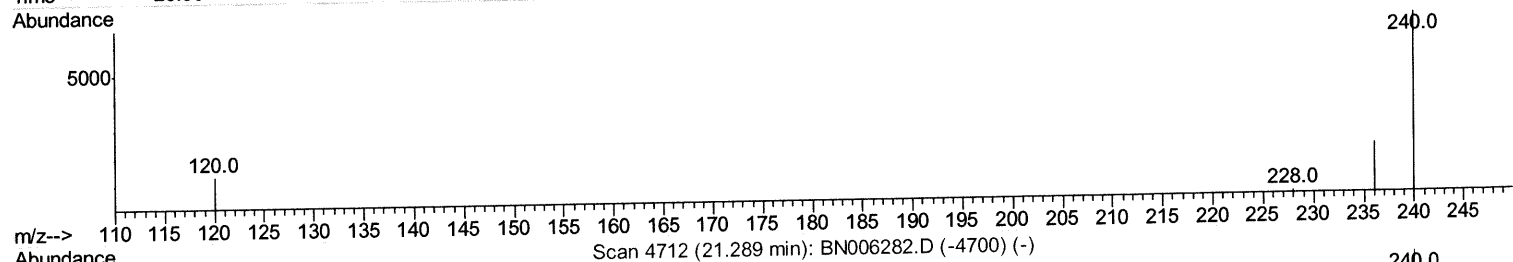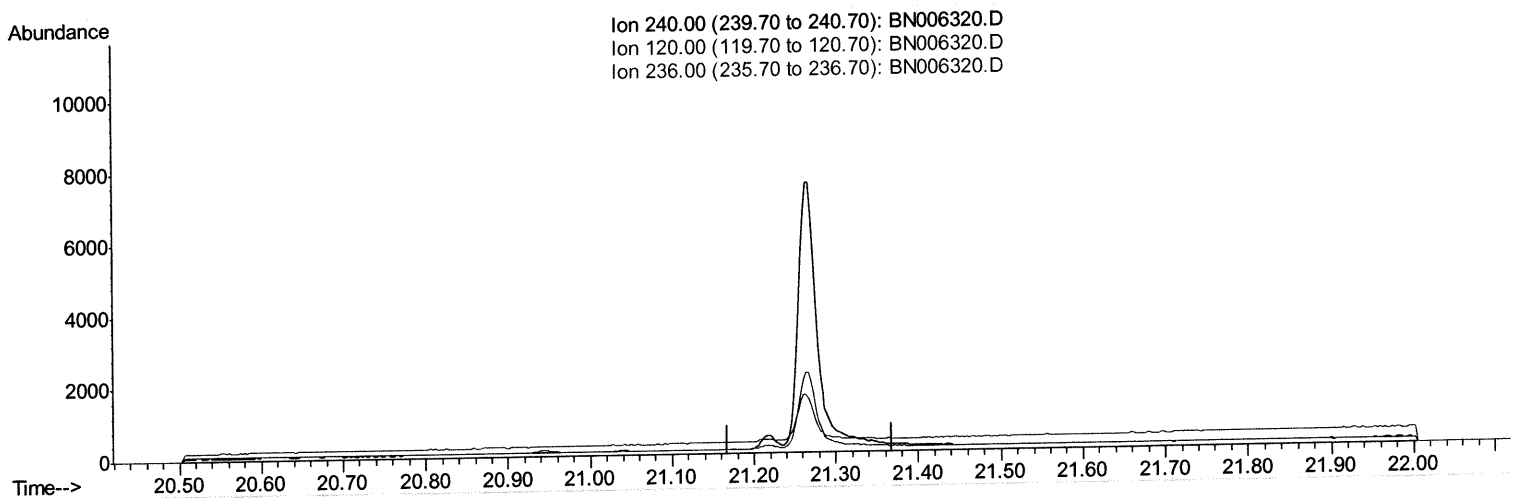

(16) Chrysene-d12 (I)

21.268min (-21.268) 0.00ng/ui

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.10	0.00#
236.00	30.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:54:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

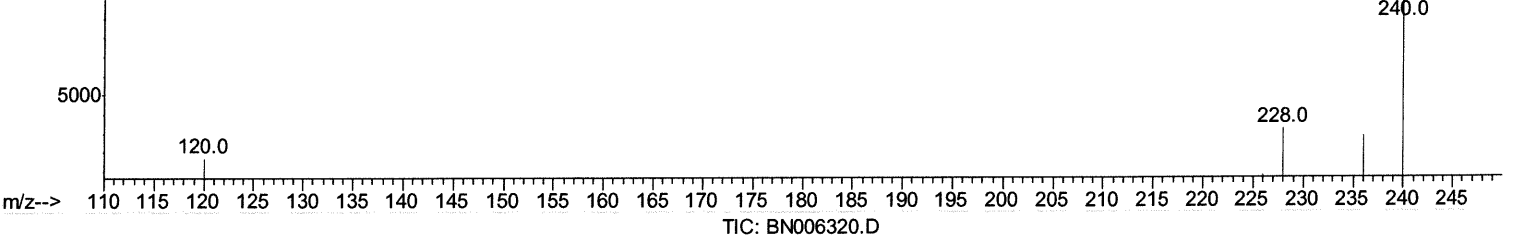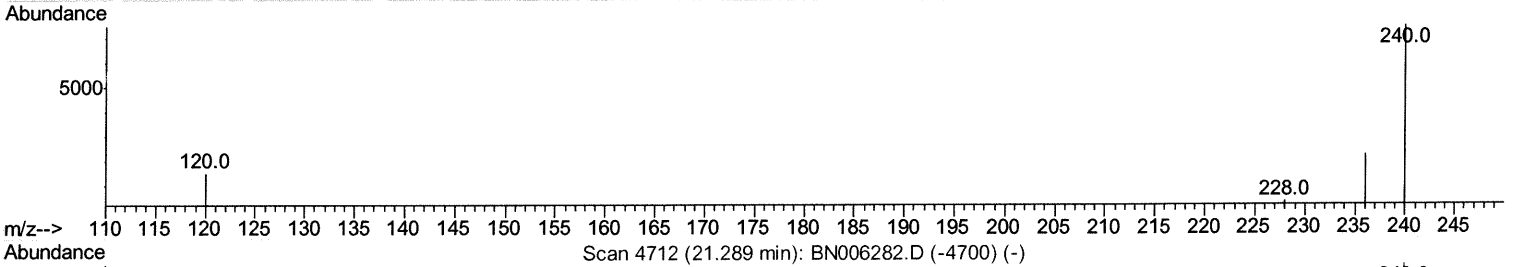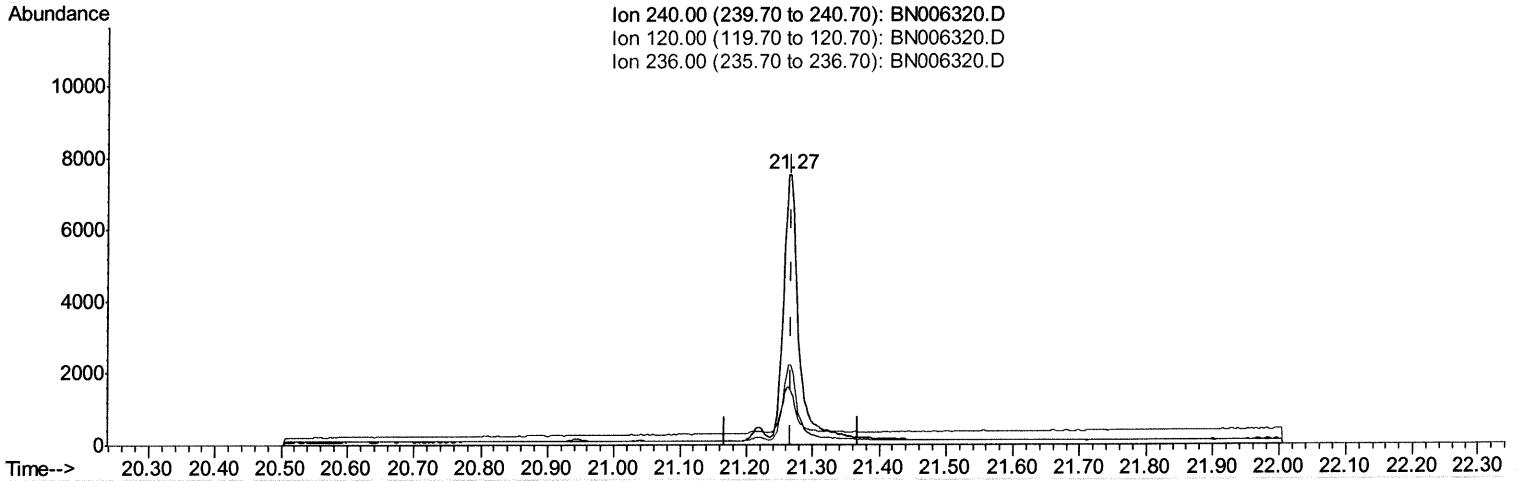

(16) Chrysene-d12 (I)

21.266min (-0.002) 0.40ng/ul m *JU* 06/19/19

response 11087

Ion	Exp%	Act%
240.00	100	100
120.00	20.10	20.10
236.00	30.10	29.65
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:56:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

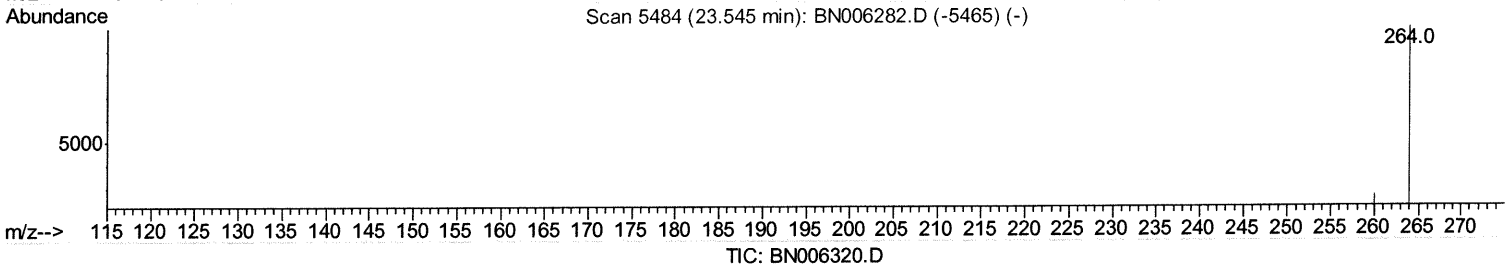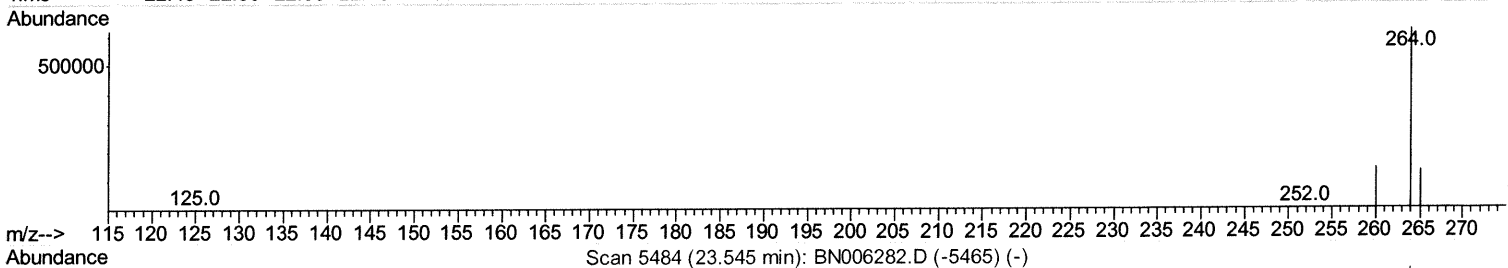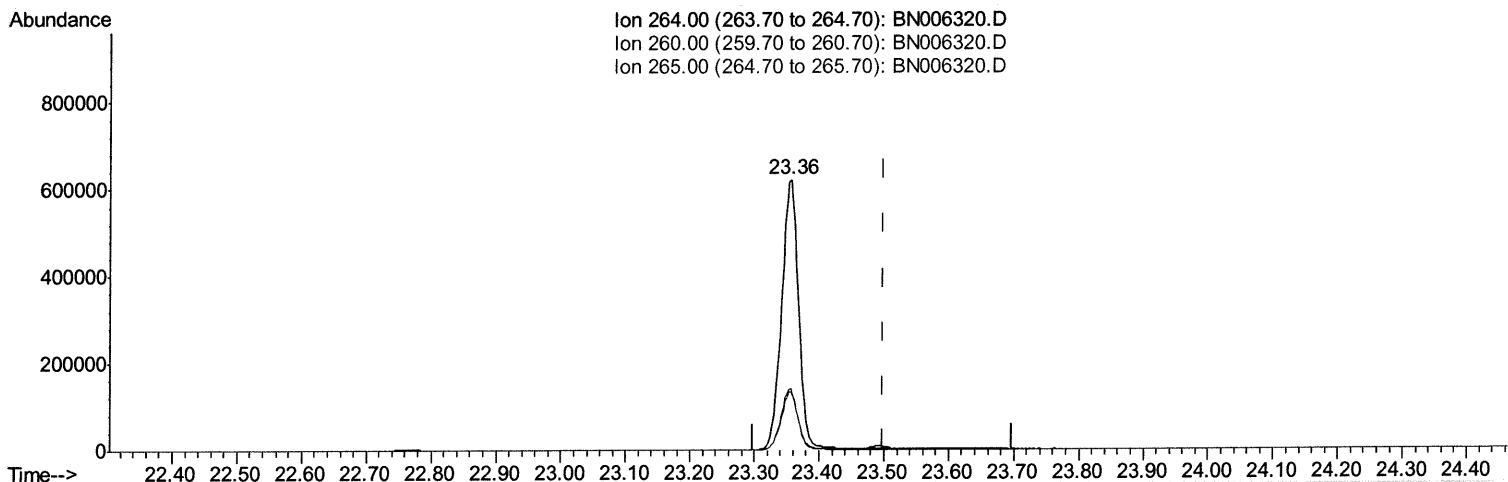

(20) Perylene-d12 (I)

23.356min (-0.142) 0.40ng/ul

response 1140305

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	22.54#
265.00	44.70	21.41#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:56:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

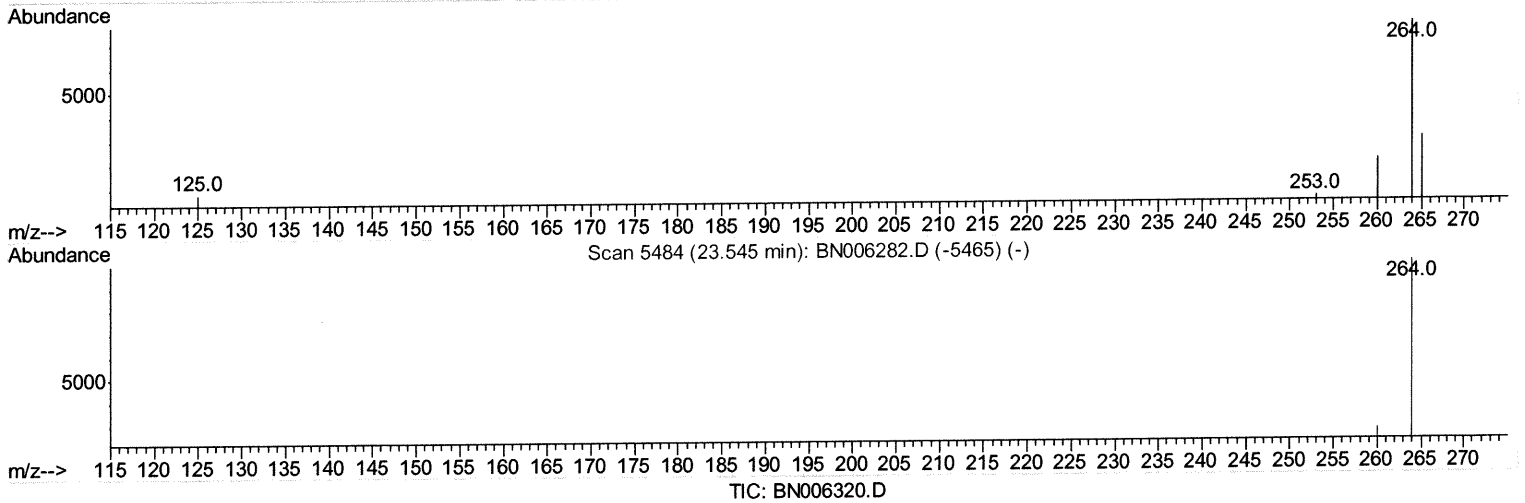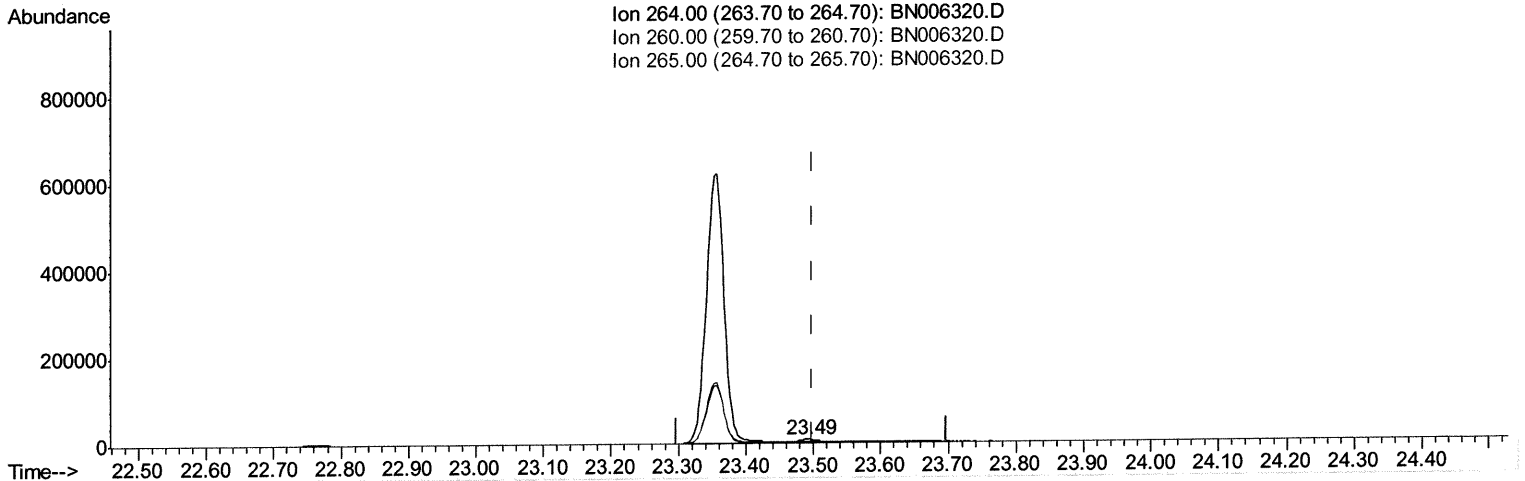

(20) Perylene-d12 (I)

23.494min (-0.005) 0.40ng/ul m *JU* 06/19/19

response 9885

Ion	Exp%	Act%
264.00	100	100
260.00	29.20	26.95
265.00	44.70	38.26
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1




Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

Ion 252.00 (251.70 to 252.70): BN006320.D
 Ion 253.00 (252.70 to 253.70): BN006320.D
 Ion 125.00 (124.70 to 125.70): BN006320.D

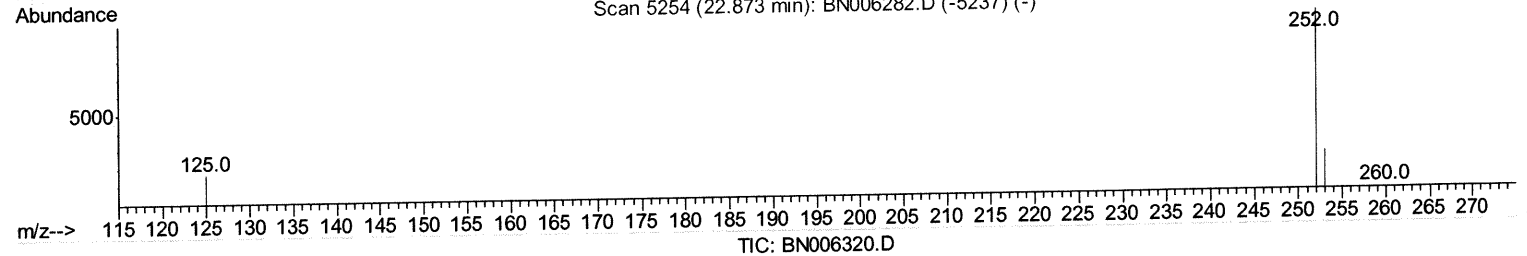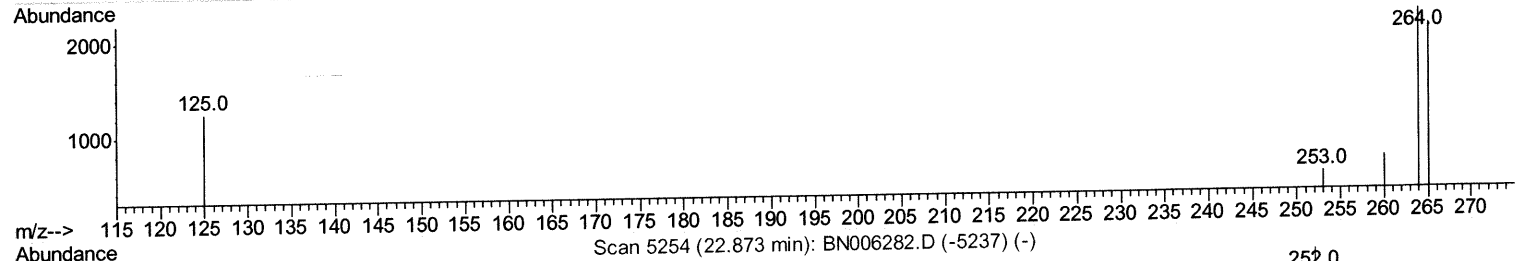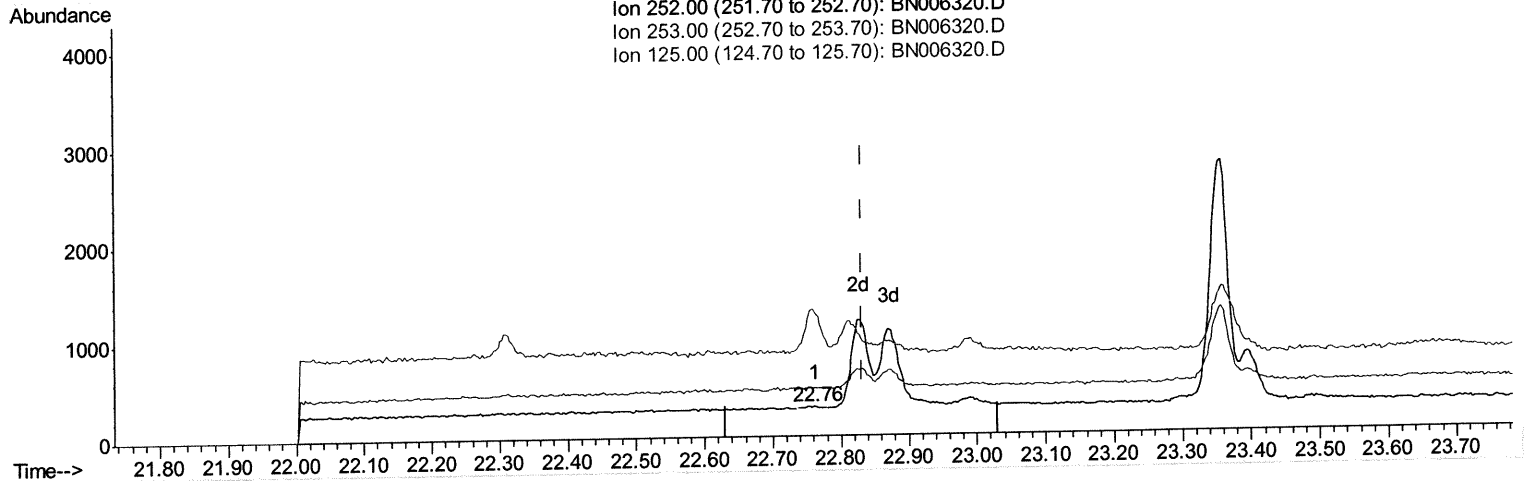

(21) Benzo(b)fluoranthene

22.763min (-0.069) 0.00ng/ul

response 50

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	164.00#
125.00	20.50	416.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006320.D
Acq On : 13 Jun 2019 20:34
Operator : JU/SJ
Sample : K3213-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
DB8K5

Manual Integrations
APPROVED

mohammad
6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

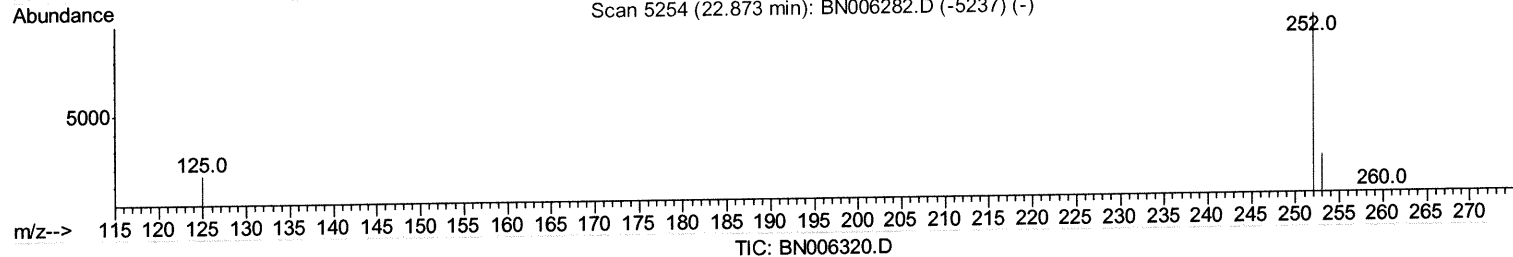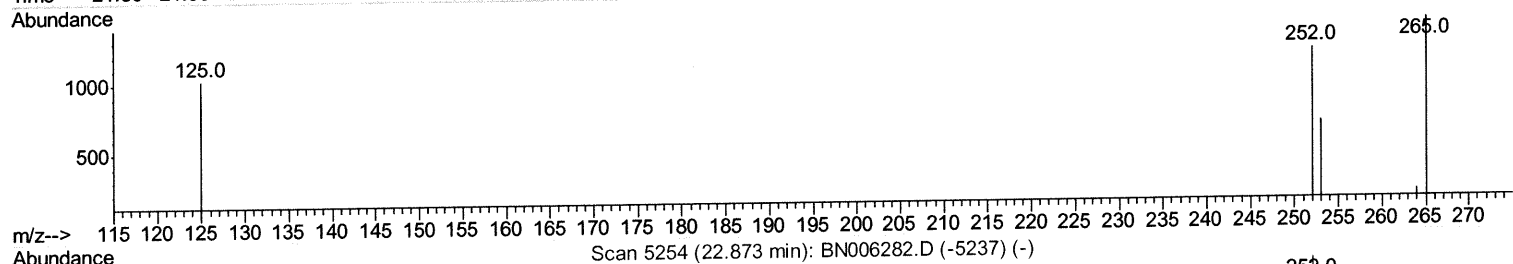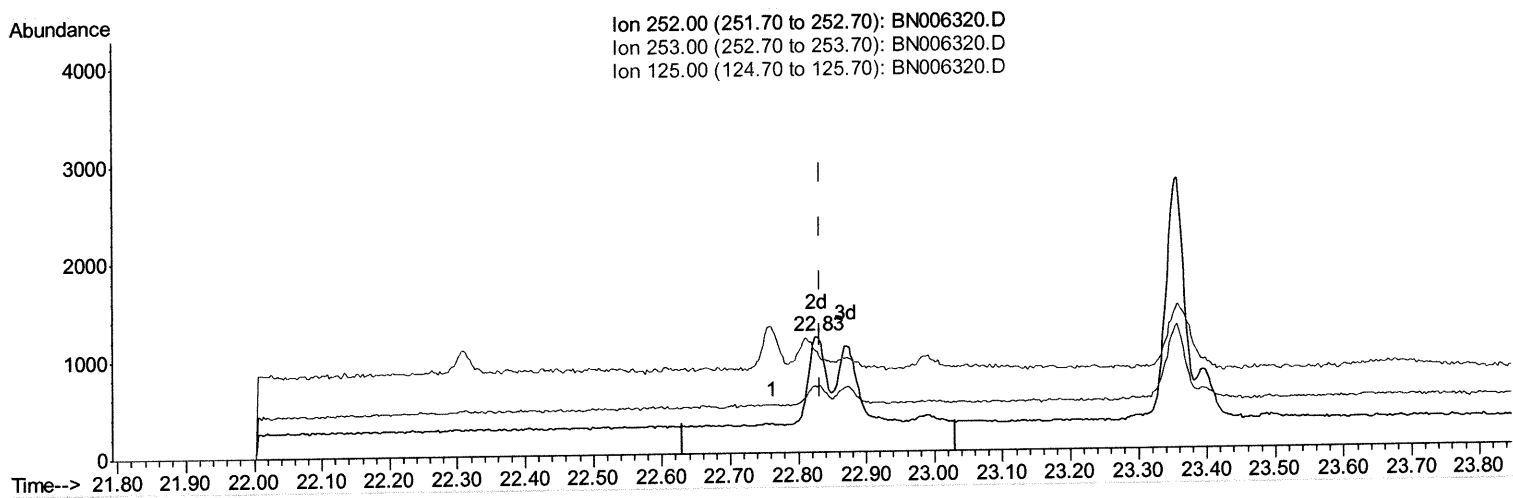

(21) Benzo(b)fluoranthene

22.827min (-0.005) 0.04ng/ul m

response 1579

Ion	Exp%	Act%
252.00	100	100
253.00	25.70	56.52#
125.00	20.50	86.88#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1




Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

Ion 252.00 (251.70 to 252.70): BN006320.D
 Ion 253.00 (252.70 to 253.70): BN006320.D
 Ion 125.00 (124.70 to 125.70): BN006320.D

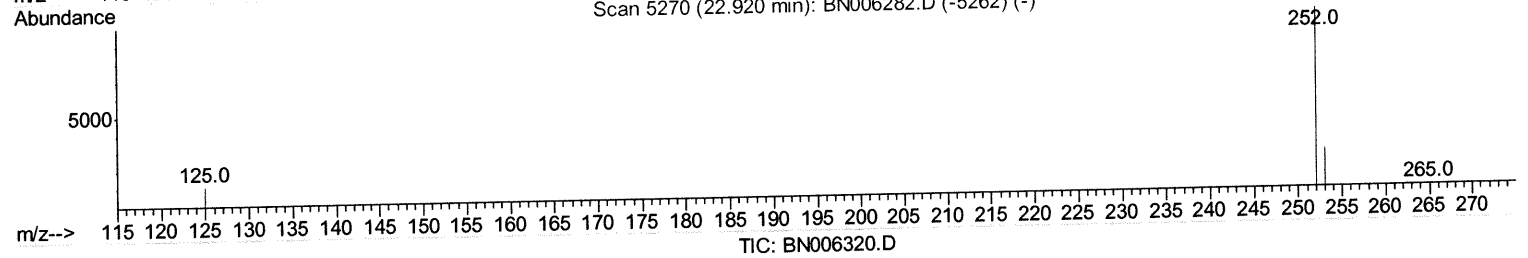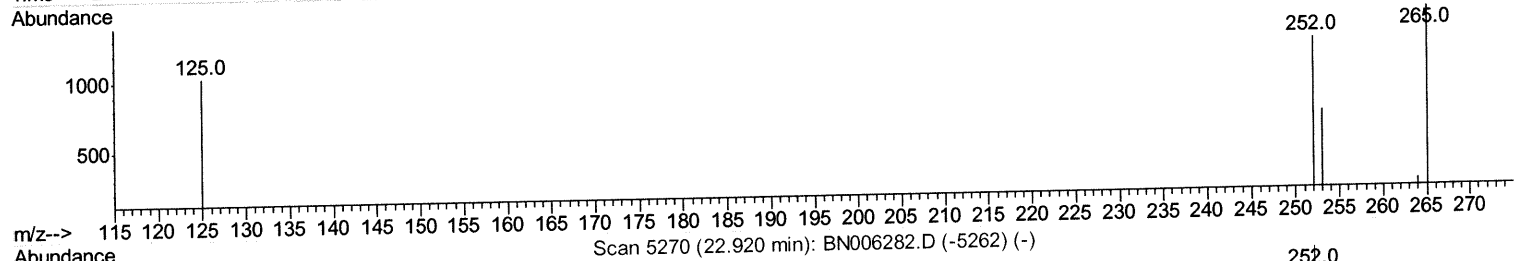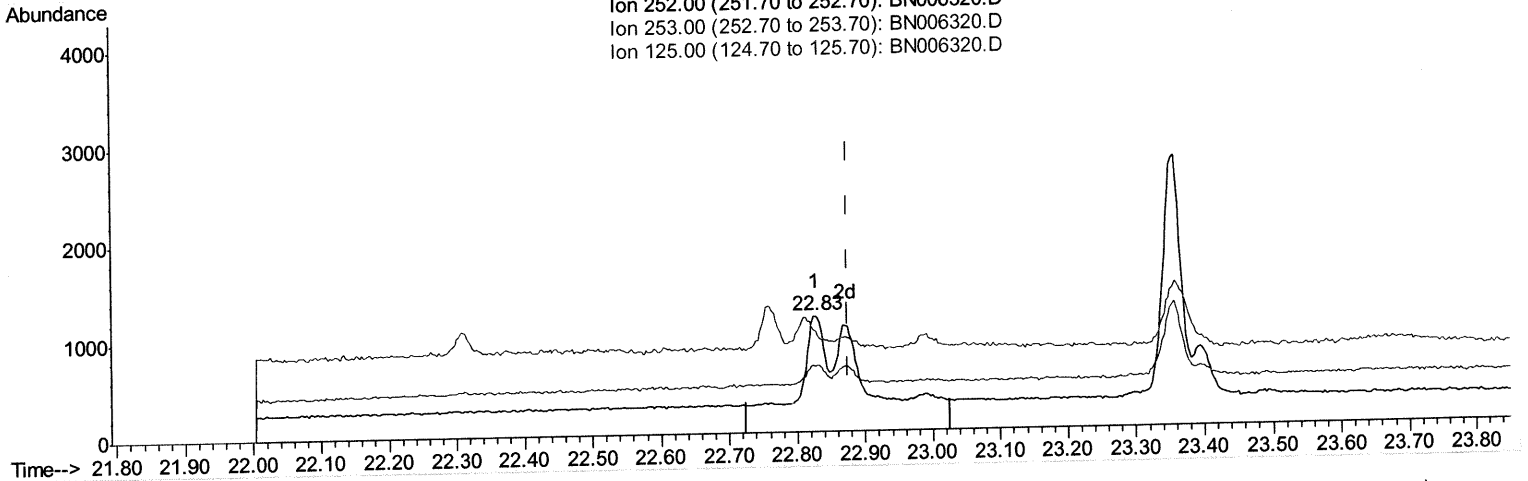

(22) Benzo(k)fluoranthene
 22.827min (-0.049) 0.04ng/ul
 response 1621

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	56.52#
125.00	17.90	86.88#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

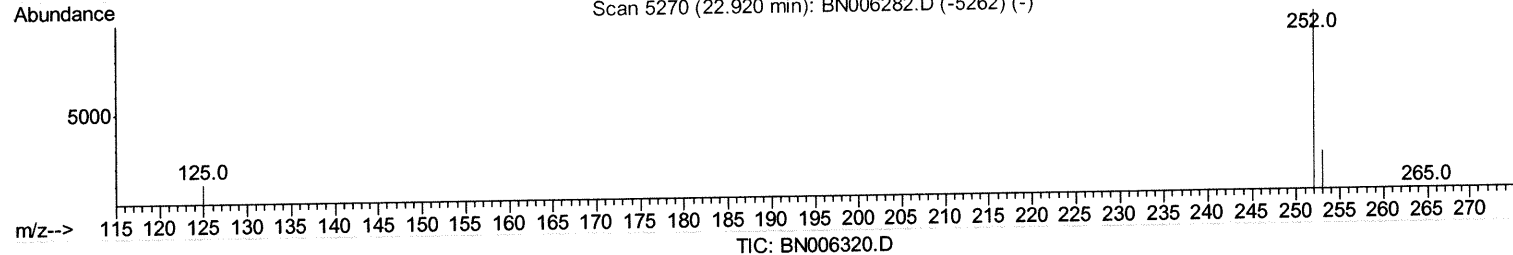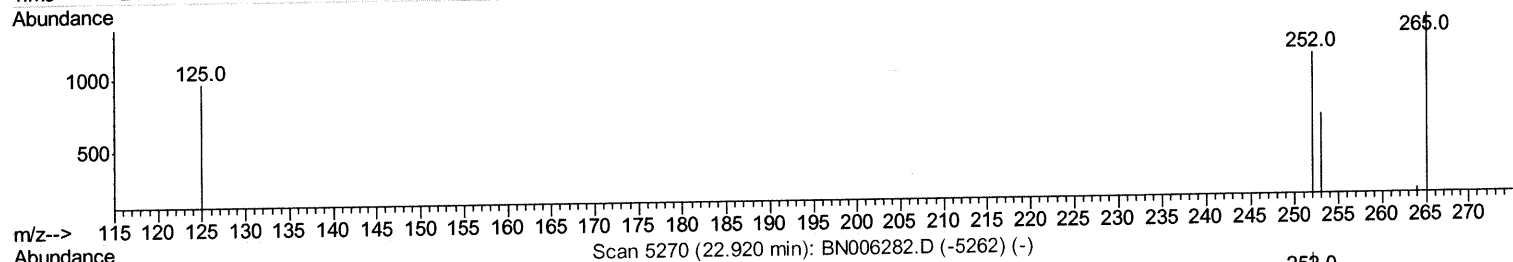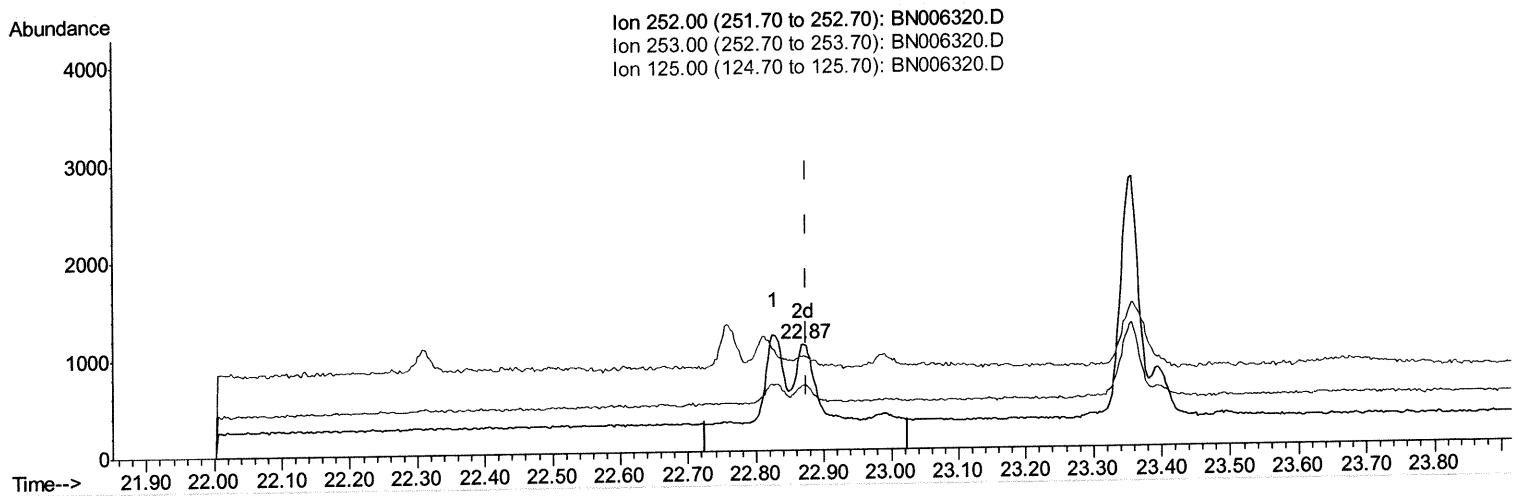

(22) Benzo(k)fluoranthene

22.871min (-0.005) 0.04ng/ul m 06/19/19

response 1443

Ion	Exp%	Act%
252.00	100	100
253.00	25.40	61.16#
125.00	17.90	89.02#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

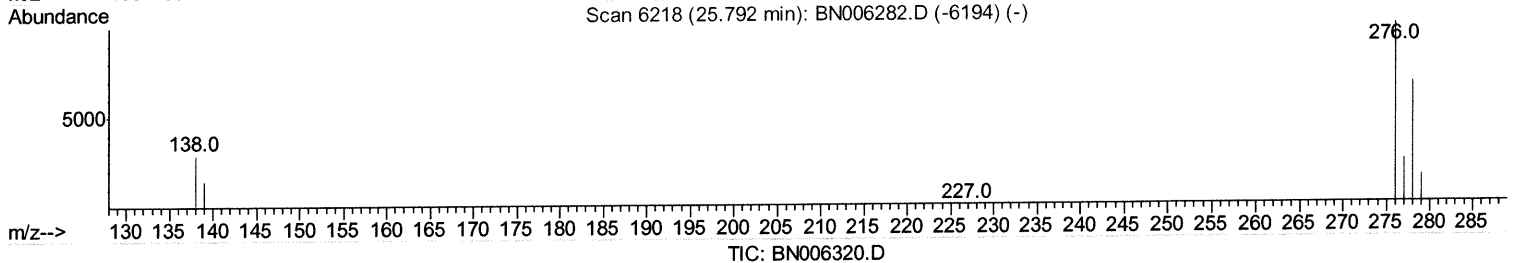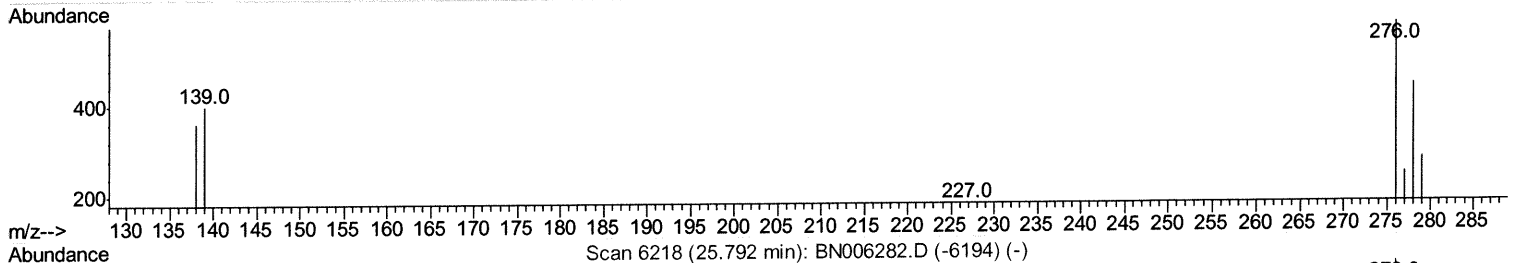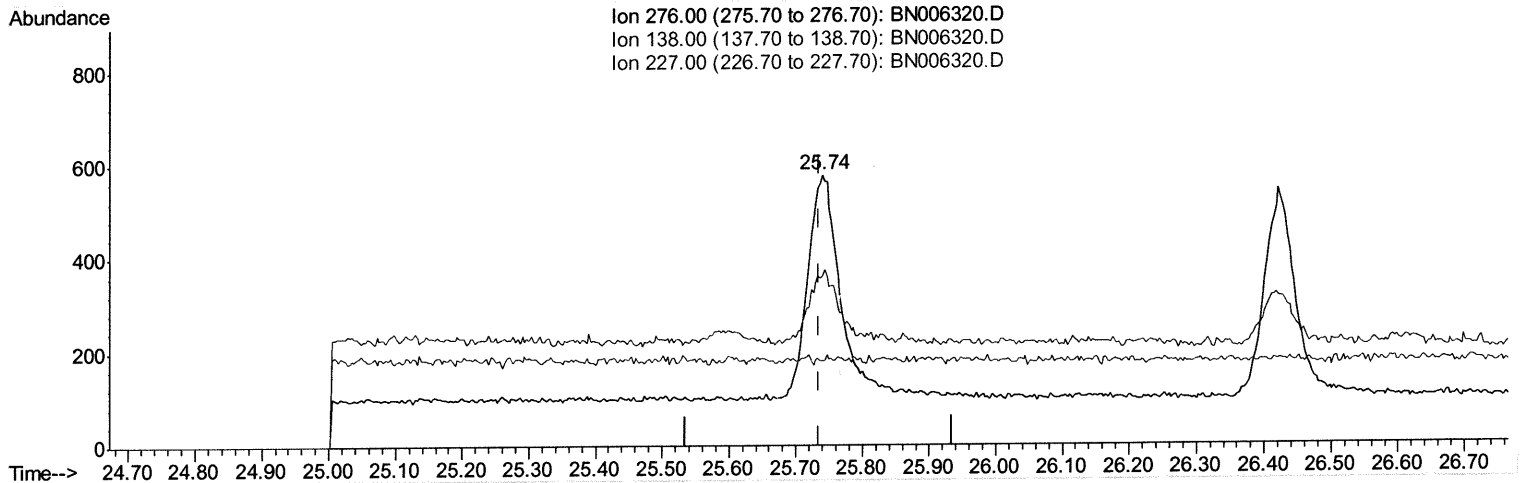

(24) Indeno(1,2,3-cd)pyrene

25.740min (+0.004) 0.03ng/ul

response 1329

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	31.30
227.00	0.40	0.38
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

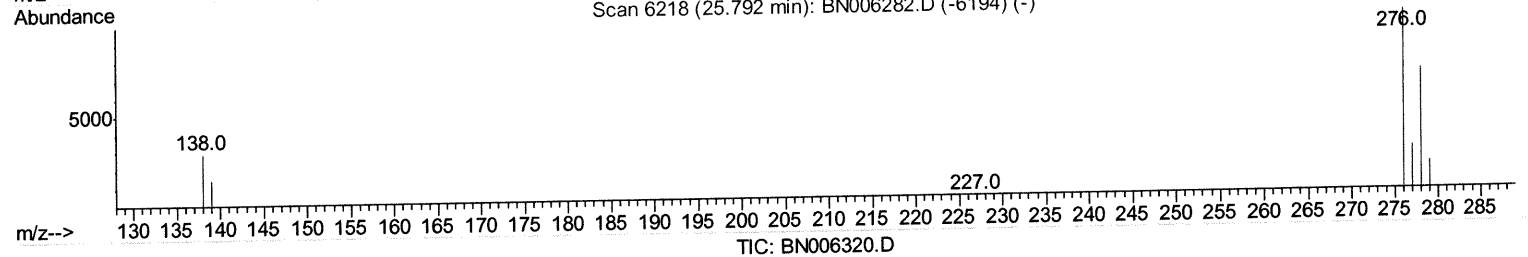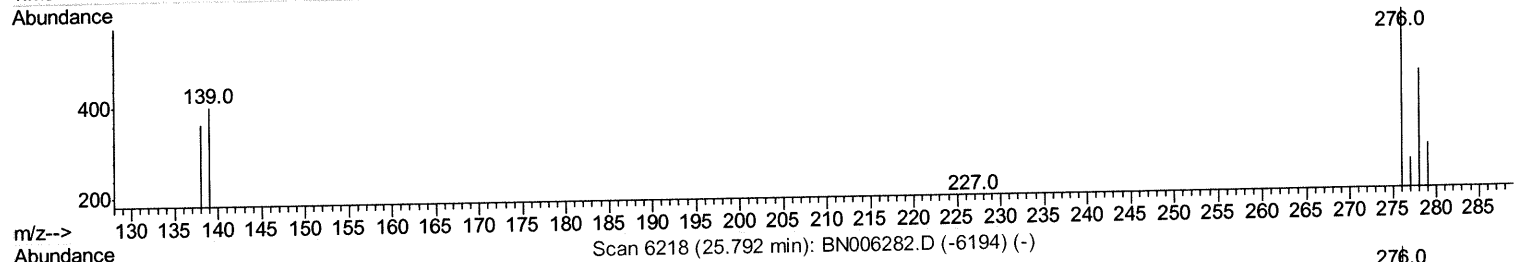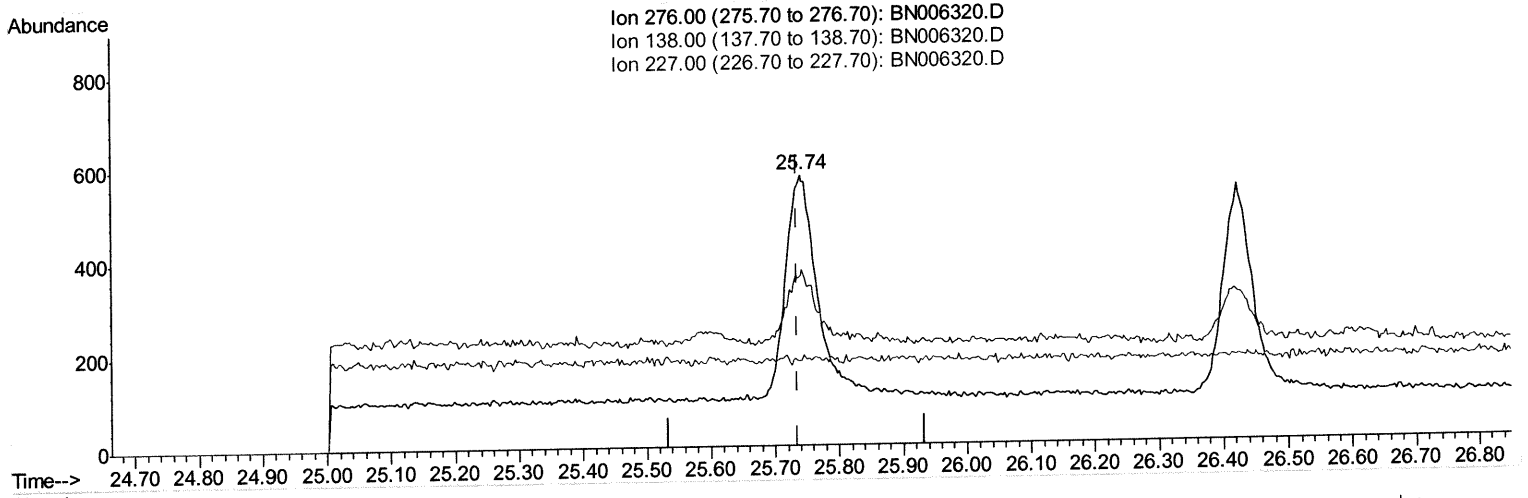

(24) Indeno(1,2,3-cd)pyrene

25.740min (+0.004) 0.04ng/ul m

response 1661

Ion	Exp%	Act%
276.00	100	100
138.00	32.00	25.05#
227.00	0.40	0.30#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

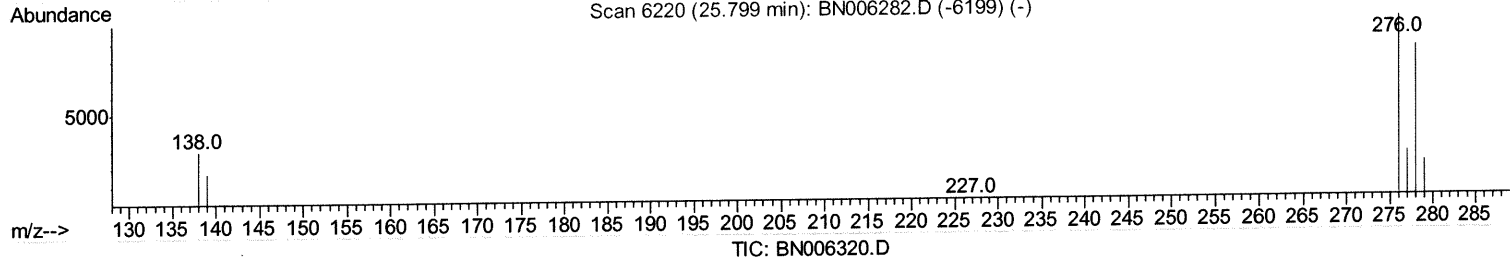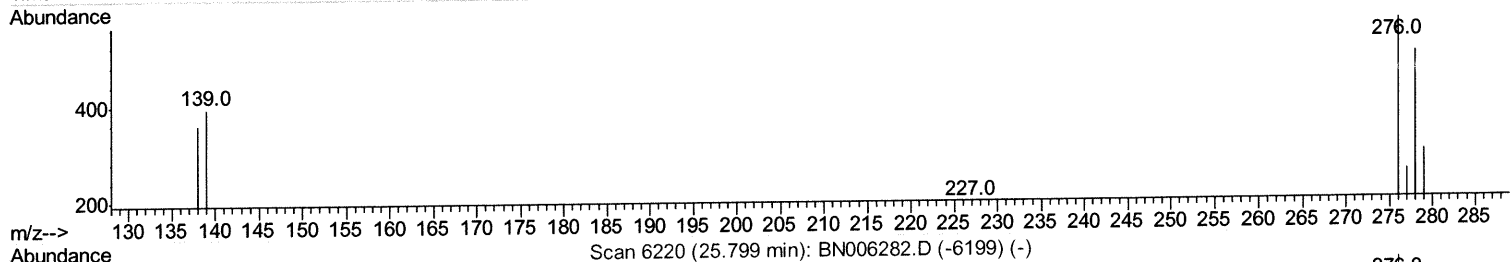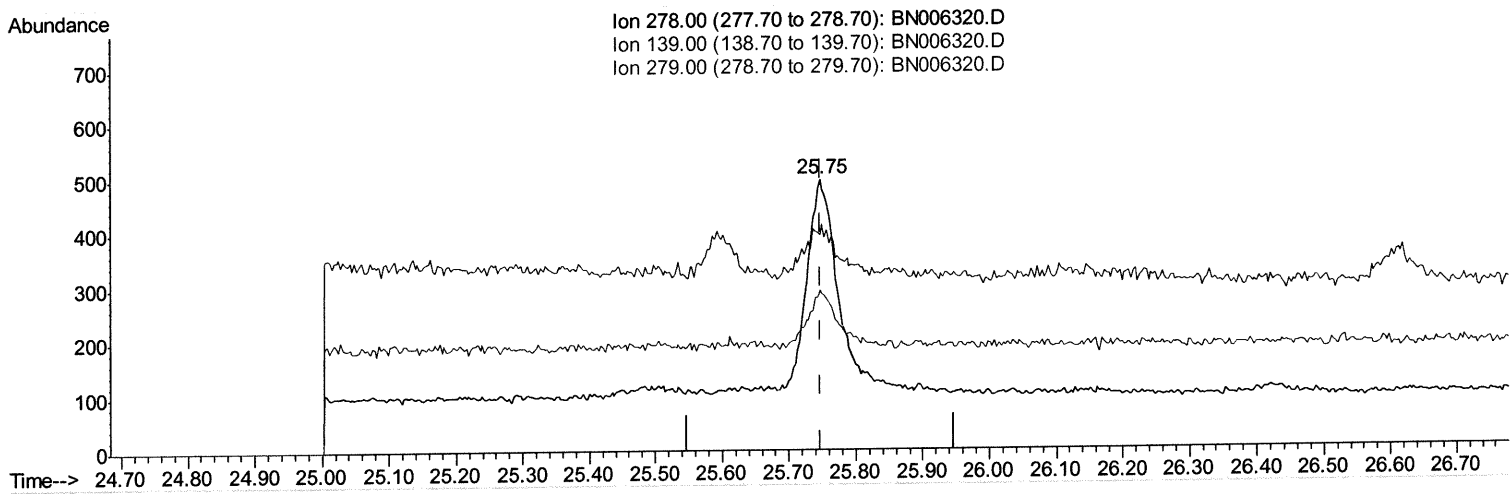

(25) Dibenzo(a,h)anthracene

25.746min (-0.002) 0.03ng/ul

response 1072

Ion	Exp%	Act%
278.00	100	100
139.00	26.50	79.60#
279.00	28.20	58.99#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006320.D
Acq On : 13 Jun 2019 20:34
Operator : JU/SJ
Sample : K3213-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB8K5

Manual Integrations
APPROVED

mohammad
6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

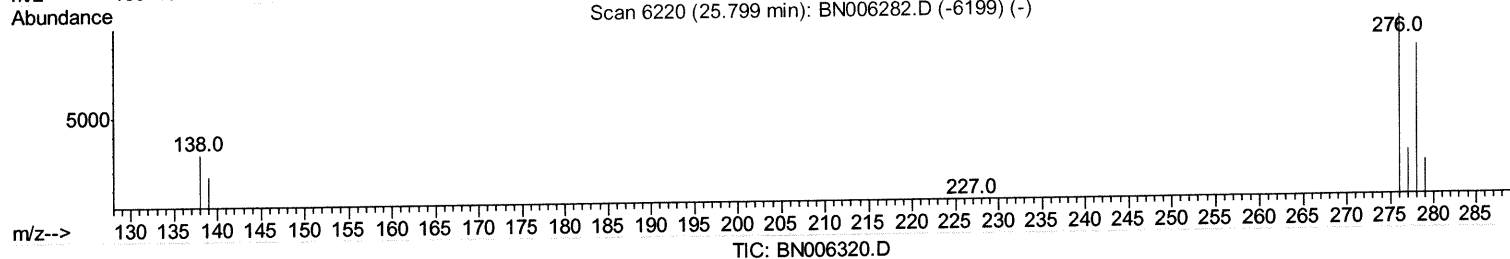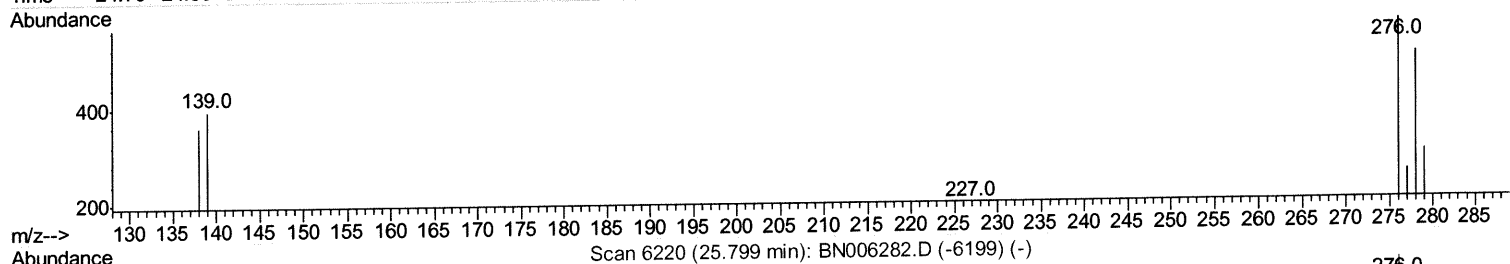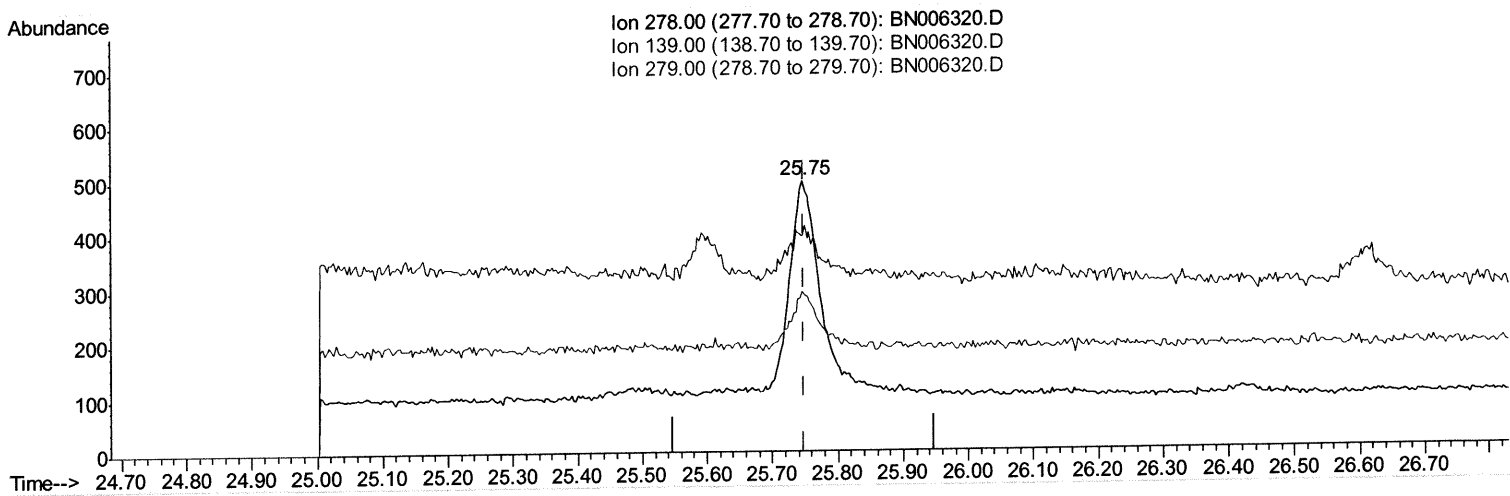

(25) Dibenzo(a,h)anthracene

25.746min (-0.002) 0.04ng/ul m

JU
06/14/19

response 1224

Ion	Exp%	Act%
278.00	100	100
139.00	26.50	79.60#
279.00	28.20	58.99#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

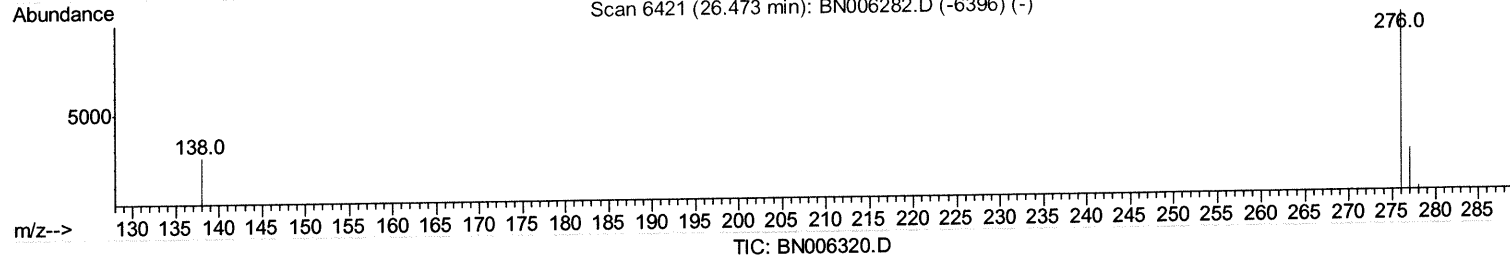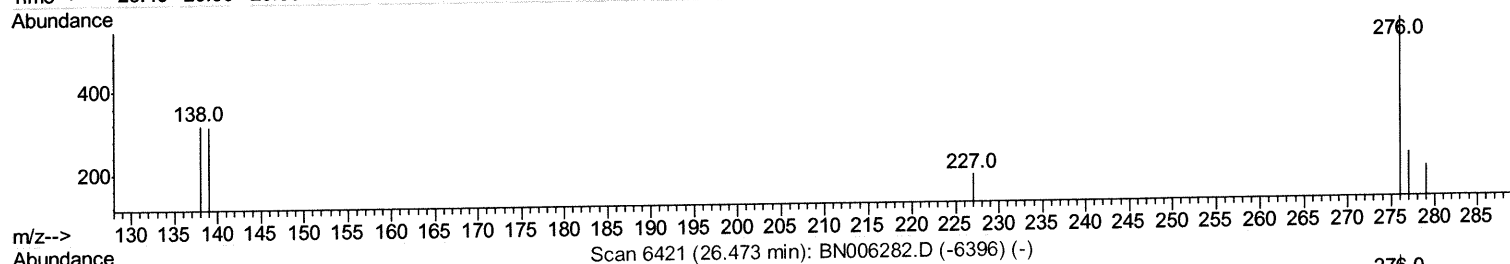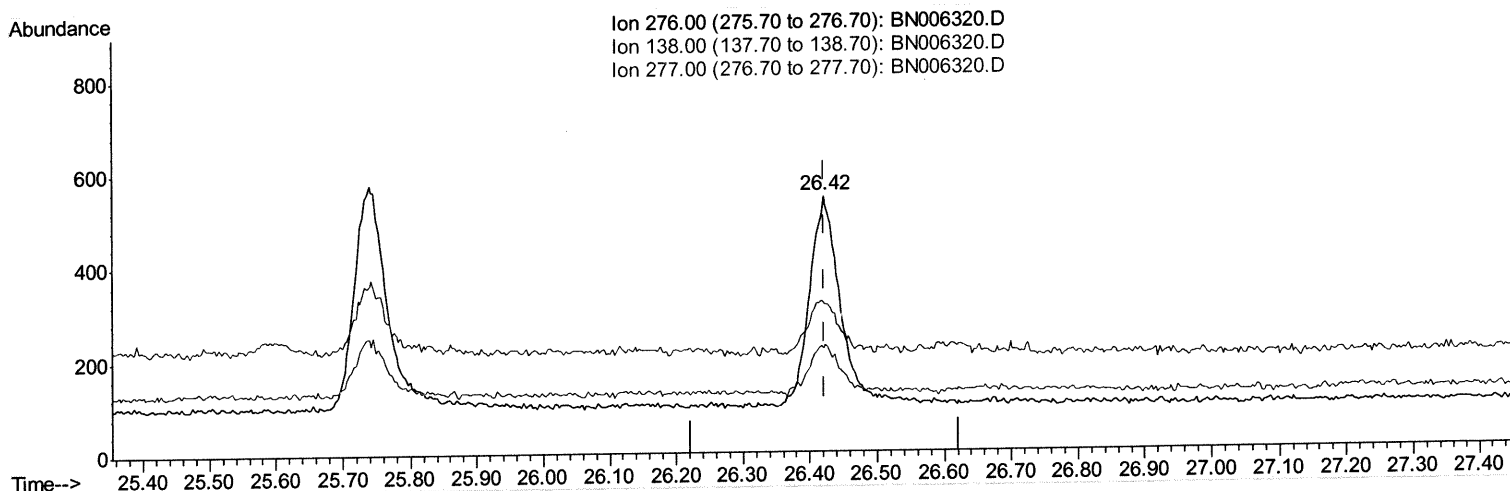

(26) Benzo(g,h,i)perylene

26.420min (-0.002) 0.03ng/ul

response 1198

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	58.24#
277.00	26.90	40.48#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 01:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

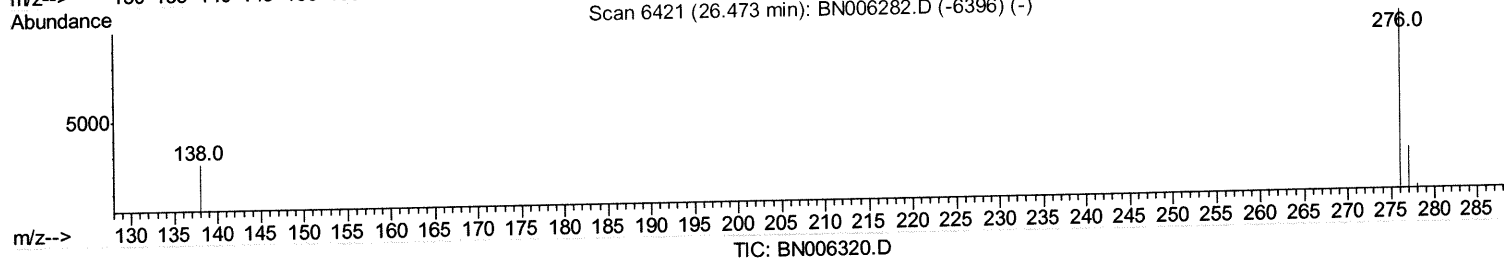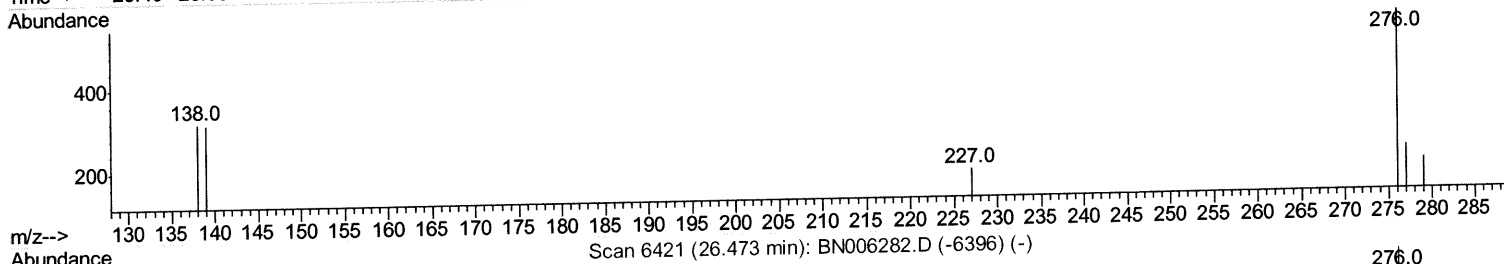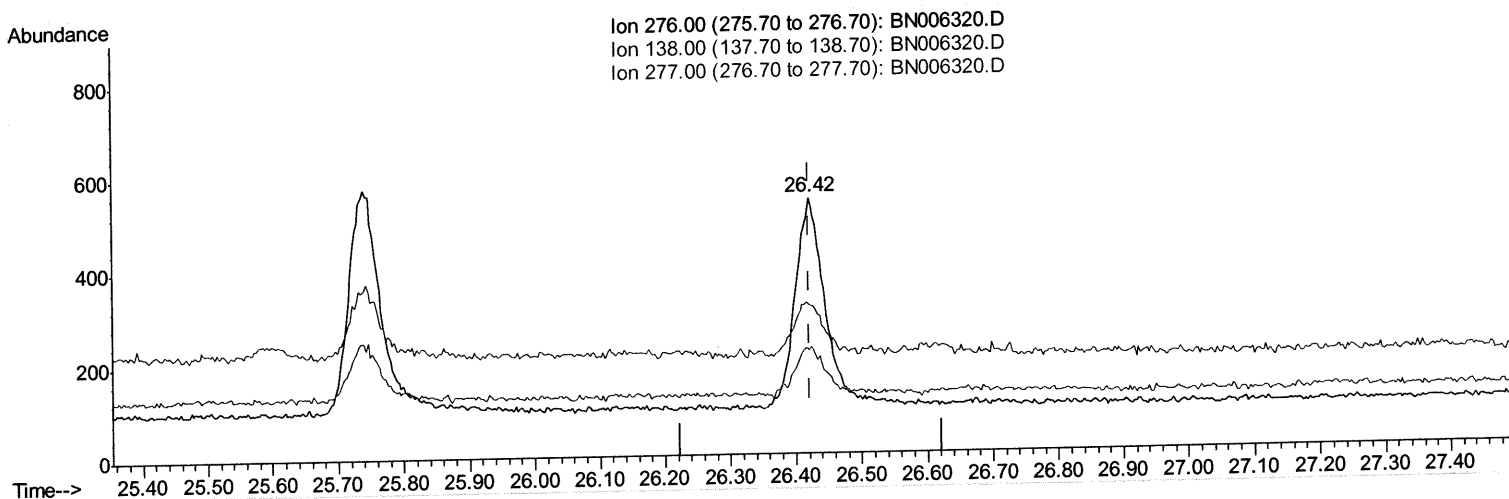

(26) Benzo(g,h,i)perylene

26.420min (-0.002) 0.04ng/ul m 06/19/19

response 1389

Ion	Exp%	Act%
276.00	100	100
138.00	30.30	58.24#
277.00	26.90	40.48#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006320.D
 Acq On : 13 Jun 2019 20:34
 Operator : JU/SJ
 Sample : K3213-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K5

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:35 AM

Quant Time: Jun 14 02:00:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4131	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15397	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	8109	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	15055m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	11087m>	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	9885m>	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	6588	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	15480m>	0.38	ng/ul	0.00
Target Compounds						
19) Chrysene	21.30	228	1536	0.033	ng/ul#	82
21) Benzo(b)fluoranthene	22.83	252	1579m>	0.038	ng/ul	
22) Benzo(k)fluoranthene	22.87	252	1443m>	0.036	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.74	276	1661m>	0.040	ng/ul	
25) Dibenzo(a,h)anthracene	25.75	278	1224m>	0.037	ng/ul	
26) Benzo(q,h,i)perylene	26.42	276	1389m>	0.040	ng/ul	

JU 06/19/19
 (#) = qualifier out of range (m) = manual integration (+) = signals summed