

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006303.D
 Acq On : 13 Jun 2019 10:13
 Operator : JU/SJ
 Sample : K3231-15DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8M2DL

Quant Time: Jun 13 16:00:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	5461	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	21028	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10189	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	19263	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	14719	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	18310	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	868	0.03	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	1897	0.04	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.71	266	7293	1.490	ng/ul	Ovalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006303.D
Acq On : 13 Jun 2019 10:13
Operator : JU/SJ
Sample : K3231-15DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DB8M2DL

Quant Time: Jun 13 16:00:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

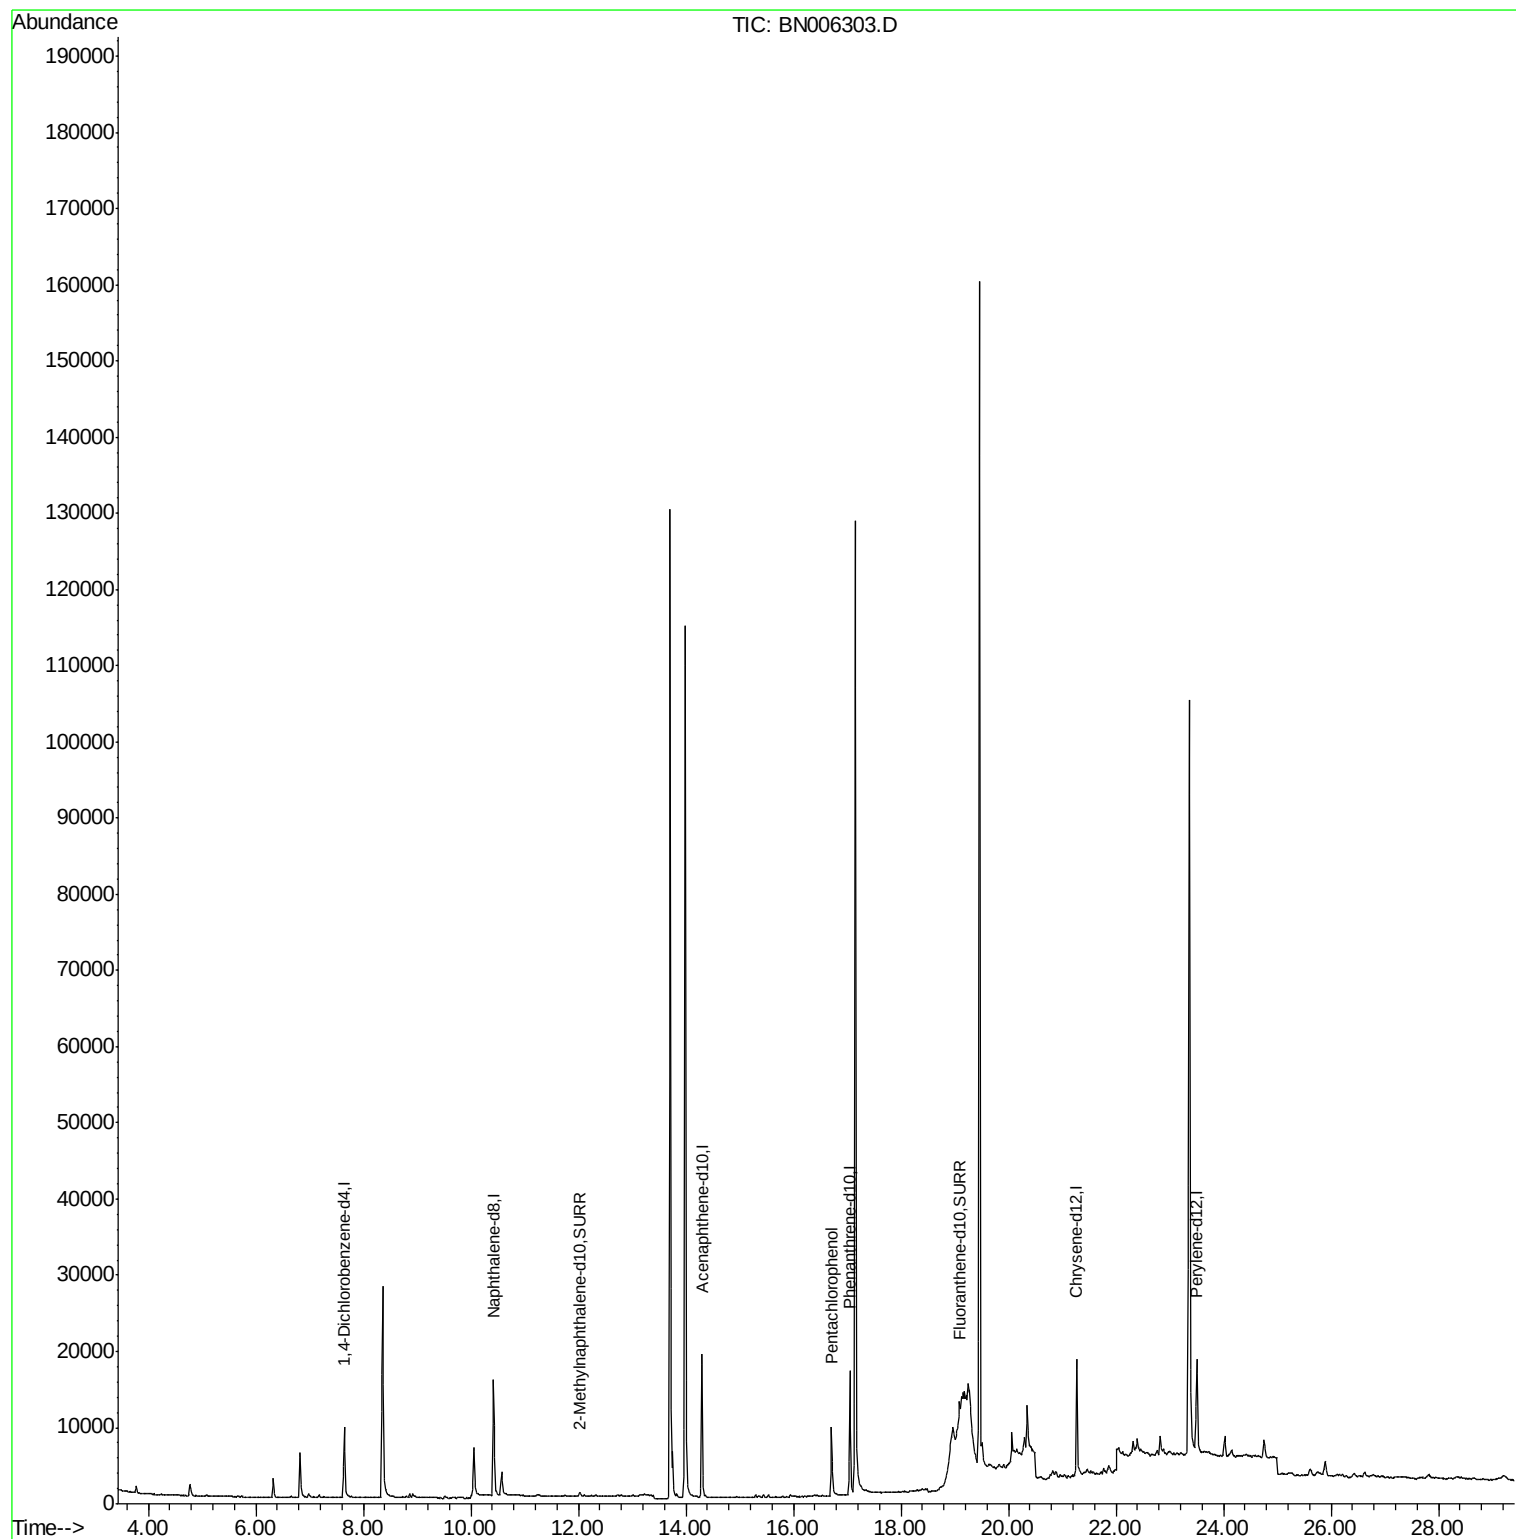


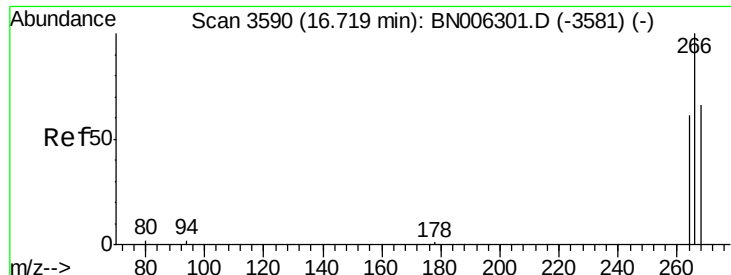

#11
 Pentachlorophenol
 Concen: 1.490 ng/ul
 RT: 16.71 min Scan# 3588
 Delta R.T. -0.01 min
 Lab File: BN006303.D
 Acq: 13 Jun 2019 10:13

Instrument :
 BNA_N
 ClientSampleId :
 DB8M2DL

Tot Ion	Ratio	Lower	Upper
266	100		
264	62.8	50.3	75.5
268	64.5	51.3	76.9

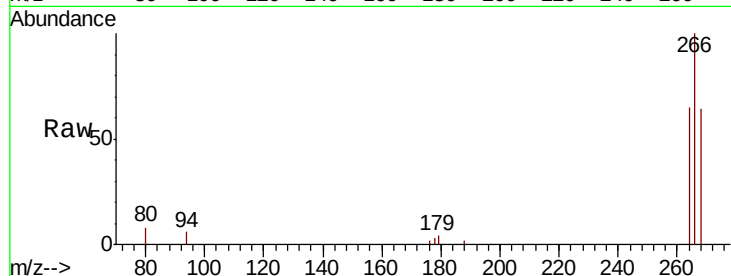

Abundance

Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

