

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006308.D
 Acq On : 13 Jun 2019 13:26
 Operator : JU/SJ
 Sample : K3213-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8J6

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:07 AM

Quant Time: Jun 13 16:12:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4979	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	18974	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	9811	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	17892m	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	12906m	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	11854m	0.40	ng/ul	0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	7897	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	16558m	0.34	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.71	266	11742m	2.583	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006308.D
Acq On : 13 Jun 2019 13:26
Operator : JU/SJ
Sample : K3213-08
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
DB8J6

Manual Integrations
APPROVED

mohammad
6/14/2019 8:49:07 AM

Quant Time: Jun 13 16:12:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

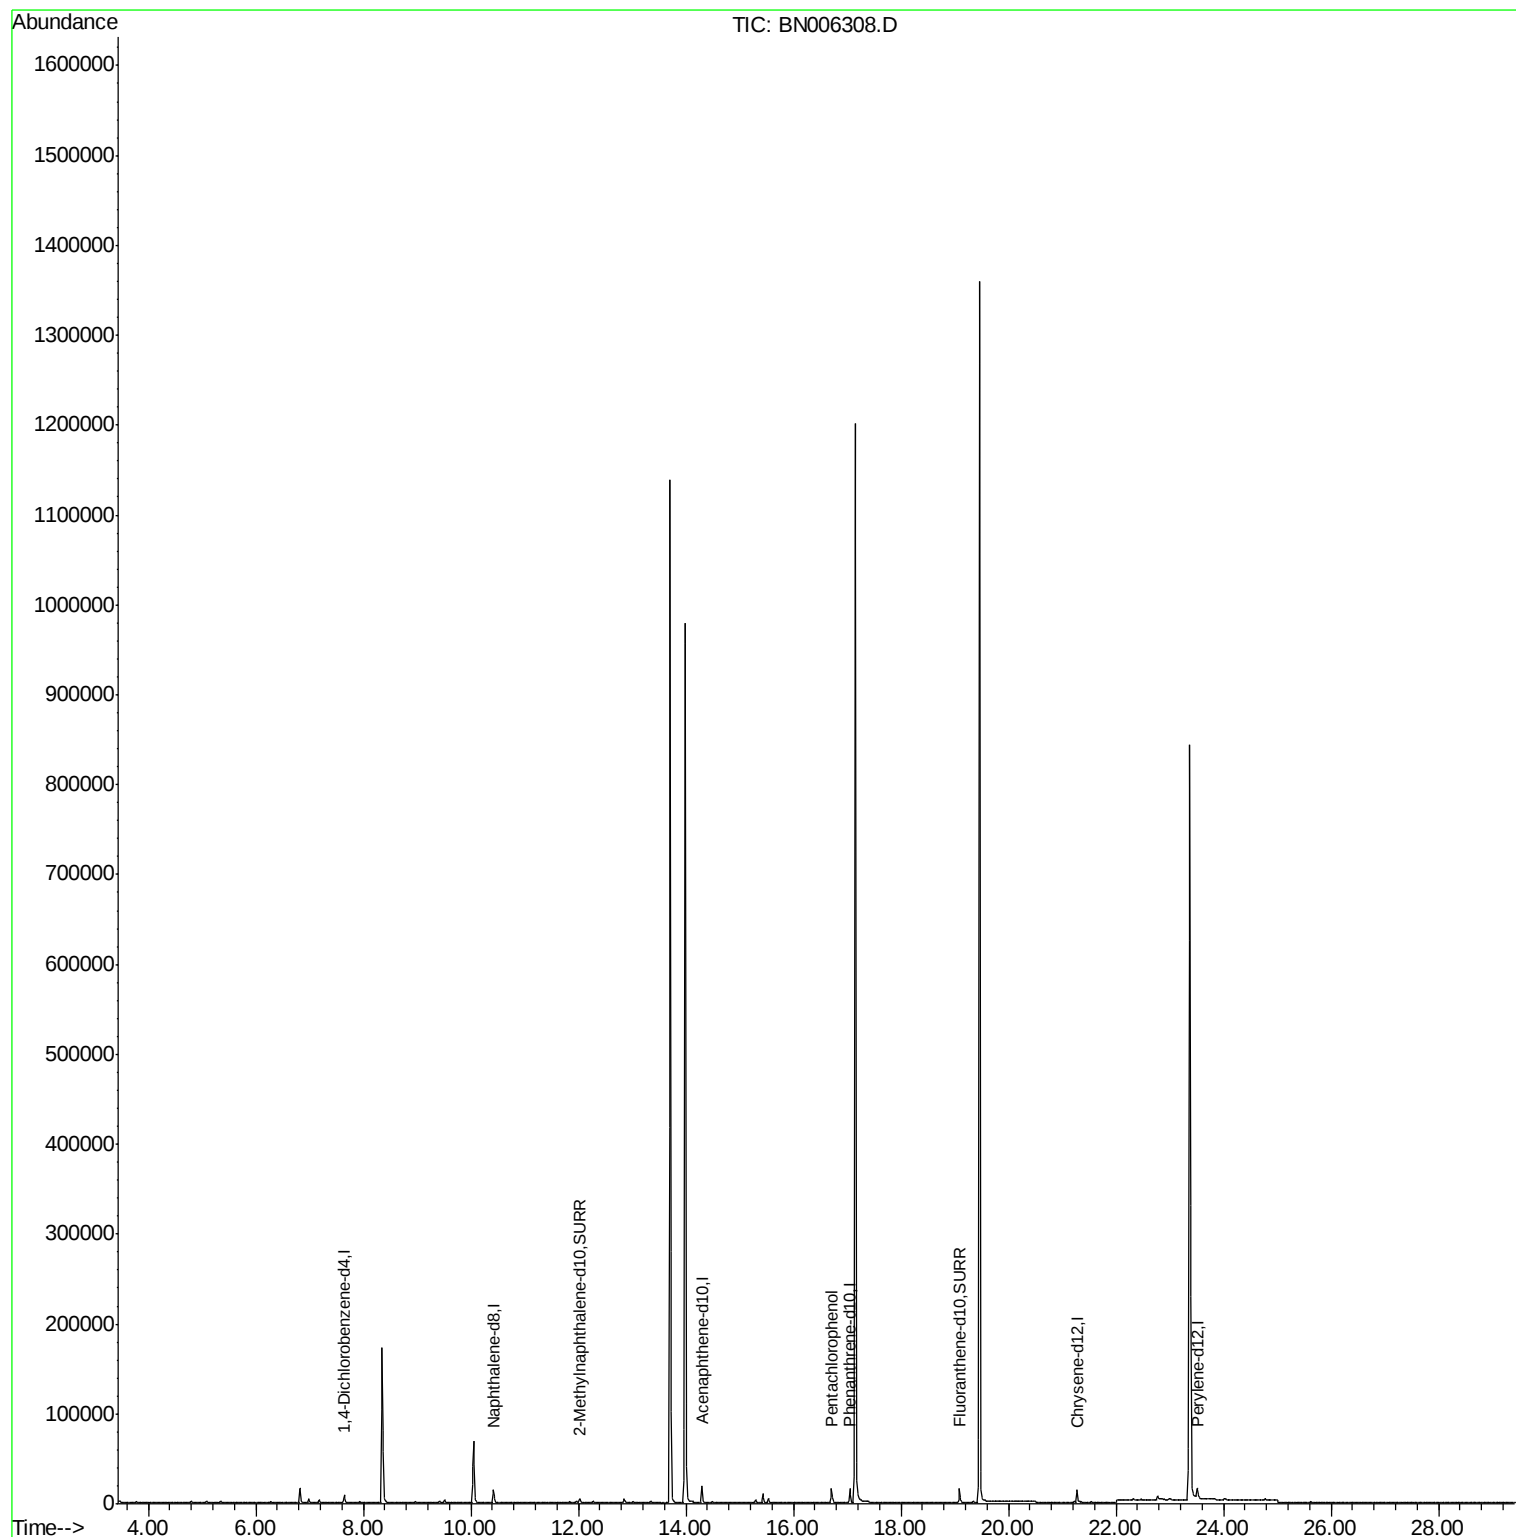

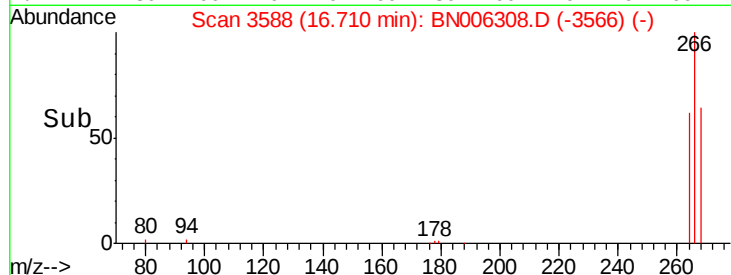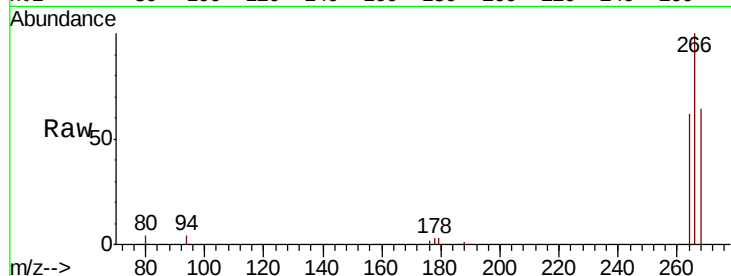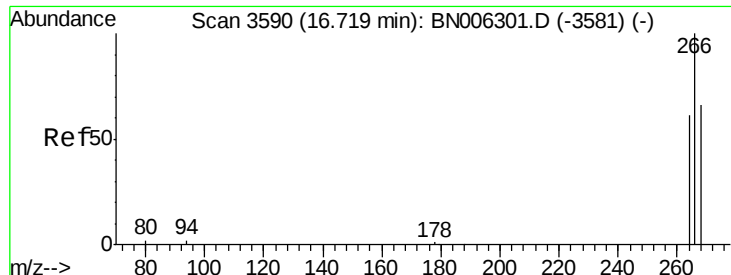

#11
 Pentachlorophenol
 Concen: 2.583 ng/ul m
 RT: 16.71 min Scan# 3588
 Delta R.T. -0.01 min
 Lab File: BN006308.D
 Acq: 13 Jun 2019 13:26

Instrument :
 BNA_N
 ClientSampleId :
 DB8J6

Tot Ion	Ratio	Resp	Lower	Upper
266	100			
264	0.0	50.3	75.5#	
268	0.0	51.3	76.9#	

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:07 AM

