

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
 Data File : BN006323.D
 Acq On : 13 Jun 2019 22:18
 Operator : JU/SJ
 Sample : K3213-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DB8K8

Manual Integrations
 APPROVED

mohammad
 6/14/2019 8:49:47 AM

Quant Time: Jun 14 02:14:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 11:20:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	4096	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15334	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	7994	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	14928m	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	11044m	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	9792m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	6895	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	15837m	0.39	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.71	266	12463m	3.286	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN061319\
Data File : BN006323.D
Acq On : 13 Jun 2019 22:18
Operator : JU/SJ
Sample : K3213-17
Misc :
ALS Vial : 14 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
DB8K8

Manual Integrations
APPROVED

mohammad
6/14/2019 8:49:47 AM

Quant Time: Jun 14 02:14:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN053019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 11:20:30 2019
Response via : Initial Calibration

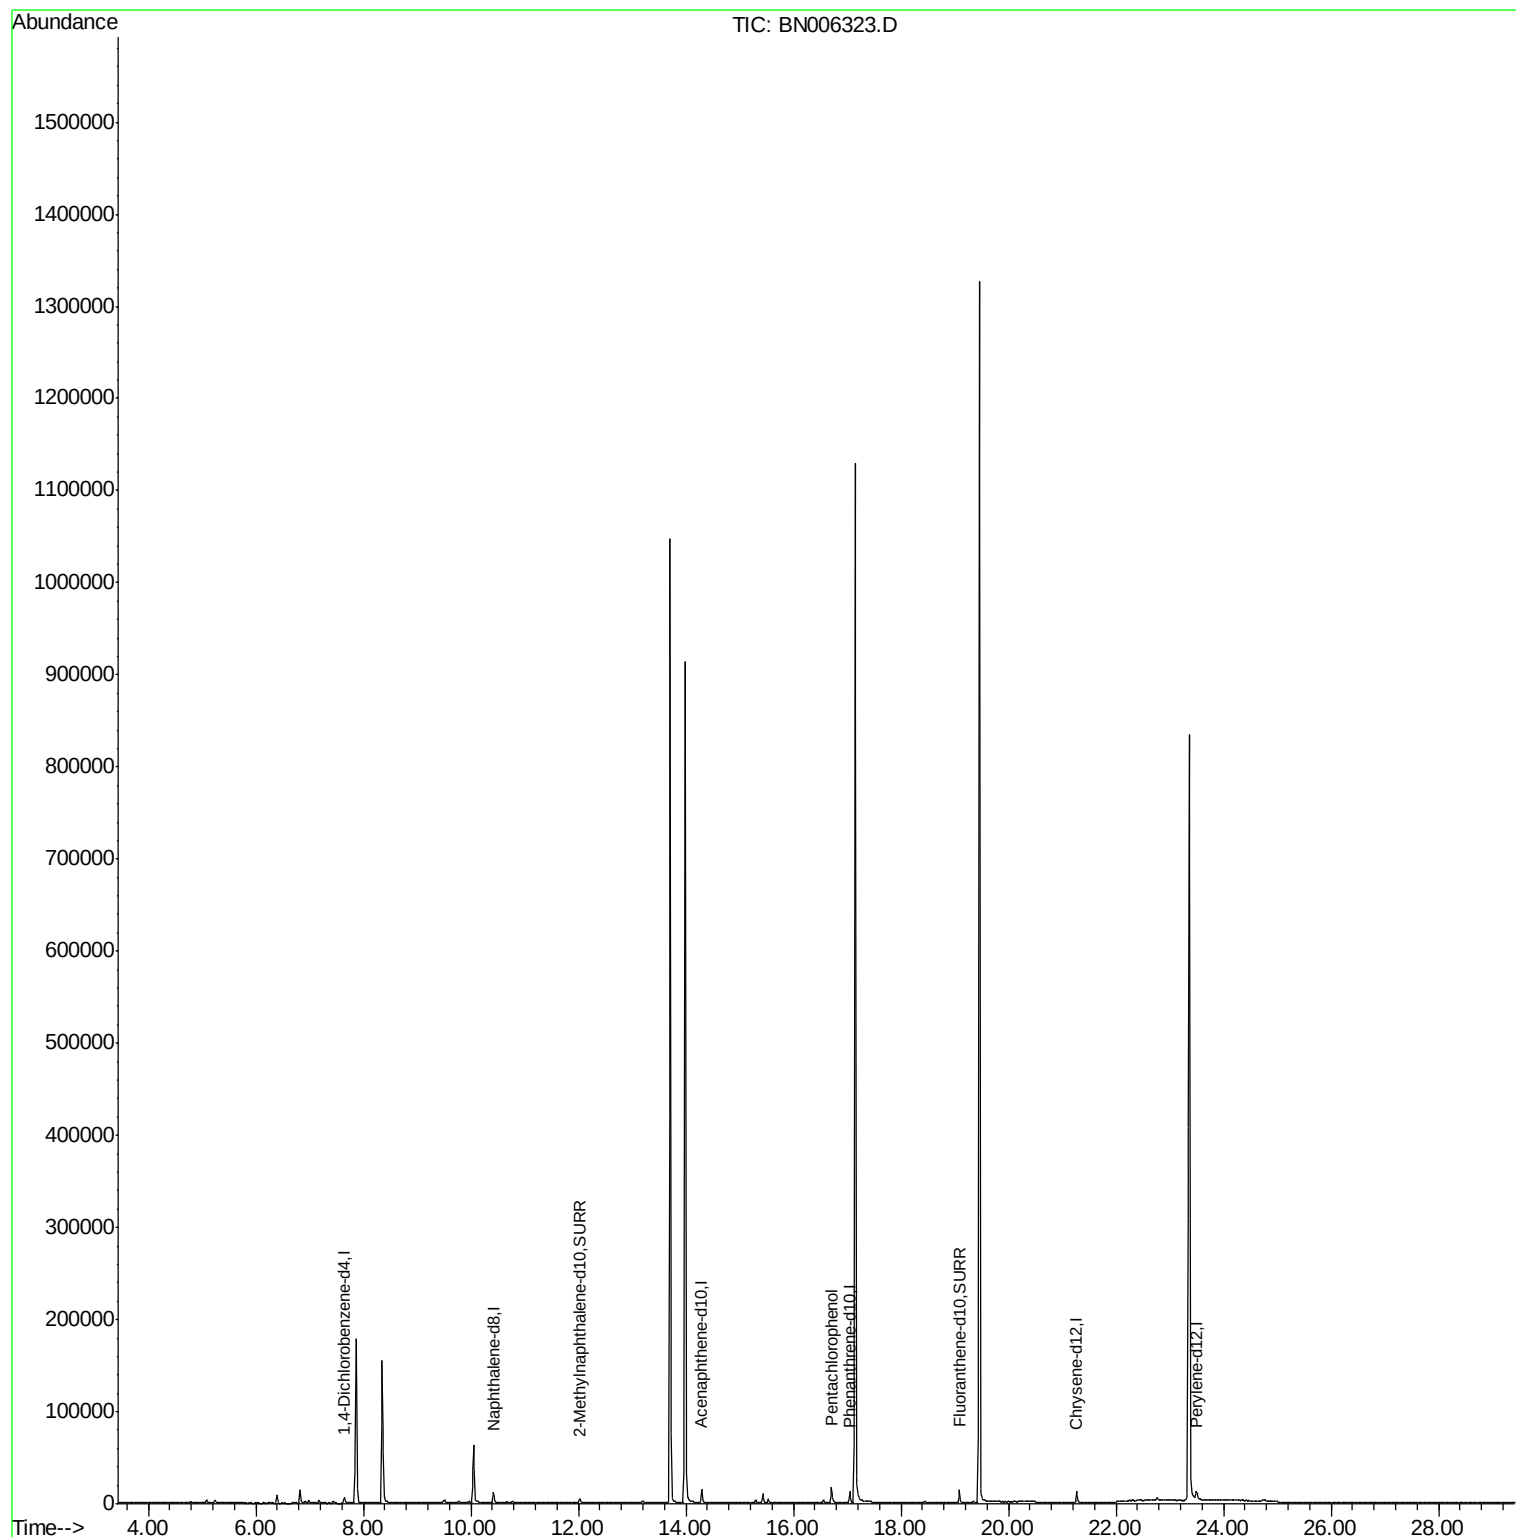

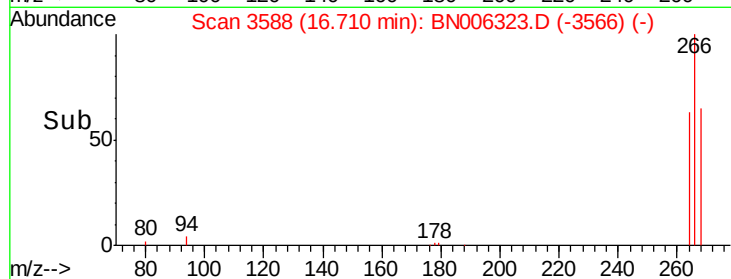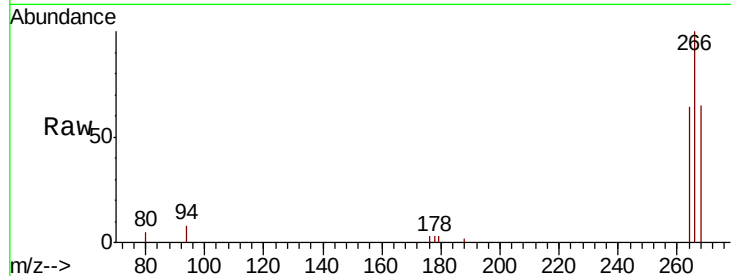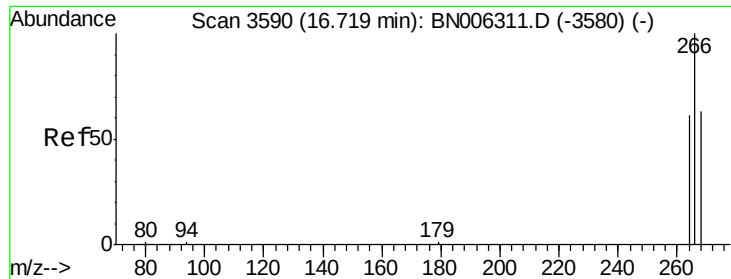

#11

Pentachlorophenol

Concen: 3.286 ng/ul m

RT: 16.71 min Scan# 3588

Delta R.T. -0.01 min

Lab File: BN006323.D

Acq: 13 Jun 2019 22:18

Instrument :

BNA_N

ClientSampleId :

DB8K8

Tot Ion:	266	Resp:	12463
Ion Ratio	Lower	Upper	
266	100		
264	0.0	50.3	75.5#
268	0.0	51.3	76.9#

Manual Integrations
APPROVED

mohammad
6/14/2019 8:49:47 AM

