

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020233.D
 Acq On : 17 Jun 2022 11:17
 Operator : CG/JU
 Sample : PB145516BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK516

Quant Time: Jun 17 22:56:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 22:53:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	155742	20.000	ng/ul	0.00
20) Naphthalene-d8	10.581	136	776742	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.422	164	548498	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	1144534	20.000	ng/ul	0.00
79) Chrysene-d12	21.351	240	992090	20.000	ng/ul	# 0.00
88) Perylene-d12	23.662	264	912390	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	22980	6.391	ng/uL	0.00
4) Pyridine-d5	3.664	84	323449	32.911	ng/ul	0.00
7) Phenol-d5	6.981	99	456291	35.407	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	273051	33.912	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	370945	35.425	ng/ul	0.00
15) 4-Methylphenol-d8	8.510	113	408533	36.641	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	189553	32.077	ng/ul	0.00
24) 2-Nitrophenol-d4	9.663	143	215454	34.355	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	383320	35.012	ng/ul	0.00
31) 4-Chloroaniline-d4	10.716	131	600880	33.892	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1314725	32.943	ng/ul	0.00
49) Acenaphthylene-d8	14.110	160	1532907	33.120	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143	222208	27.785	ng/ul	0.00
60) Fluorene-d10	15.410	176	1098169	33.252	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.533	200	202702	30.574	ng/ul	0.00
73) Anthracene-d10	17.263	188	1758520	35.205	ng/ul	0.00
81) Pyrene-d10	19.557	212	1929795	35.881	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.515	264	1550248	34.727	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.510	70	9914	1.145 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020233.D
Acq On : 17 Jun 2022 11:17
Operator : CG/JU
Sample : PB145516BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK516


Quant Time: Jun 17 22:56:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 22:53:31 2022
Response via : Initial Calibration

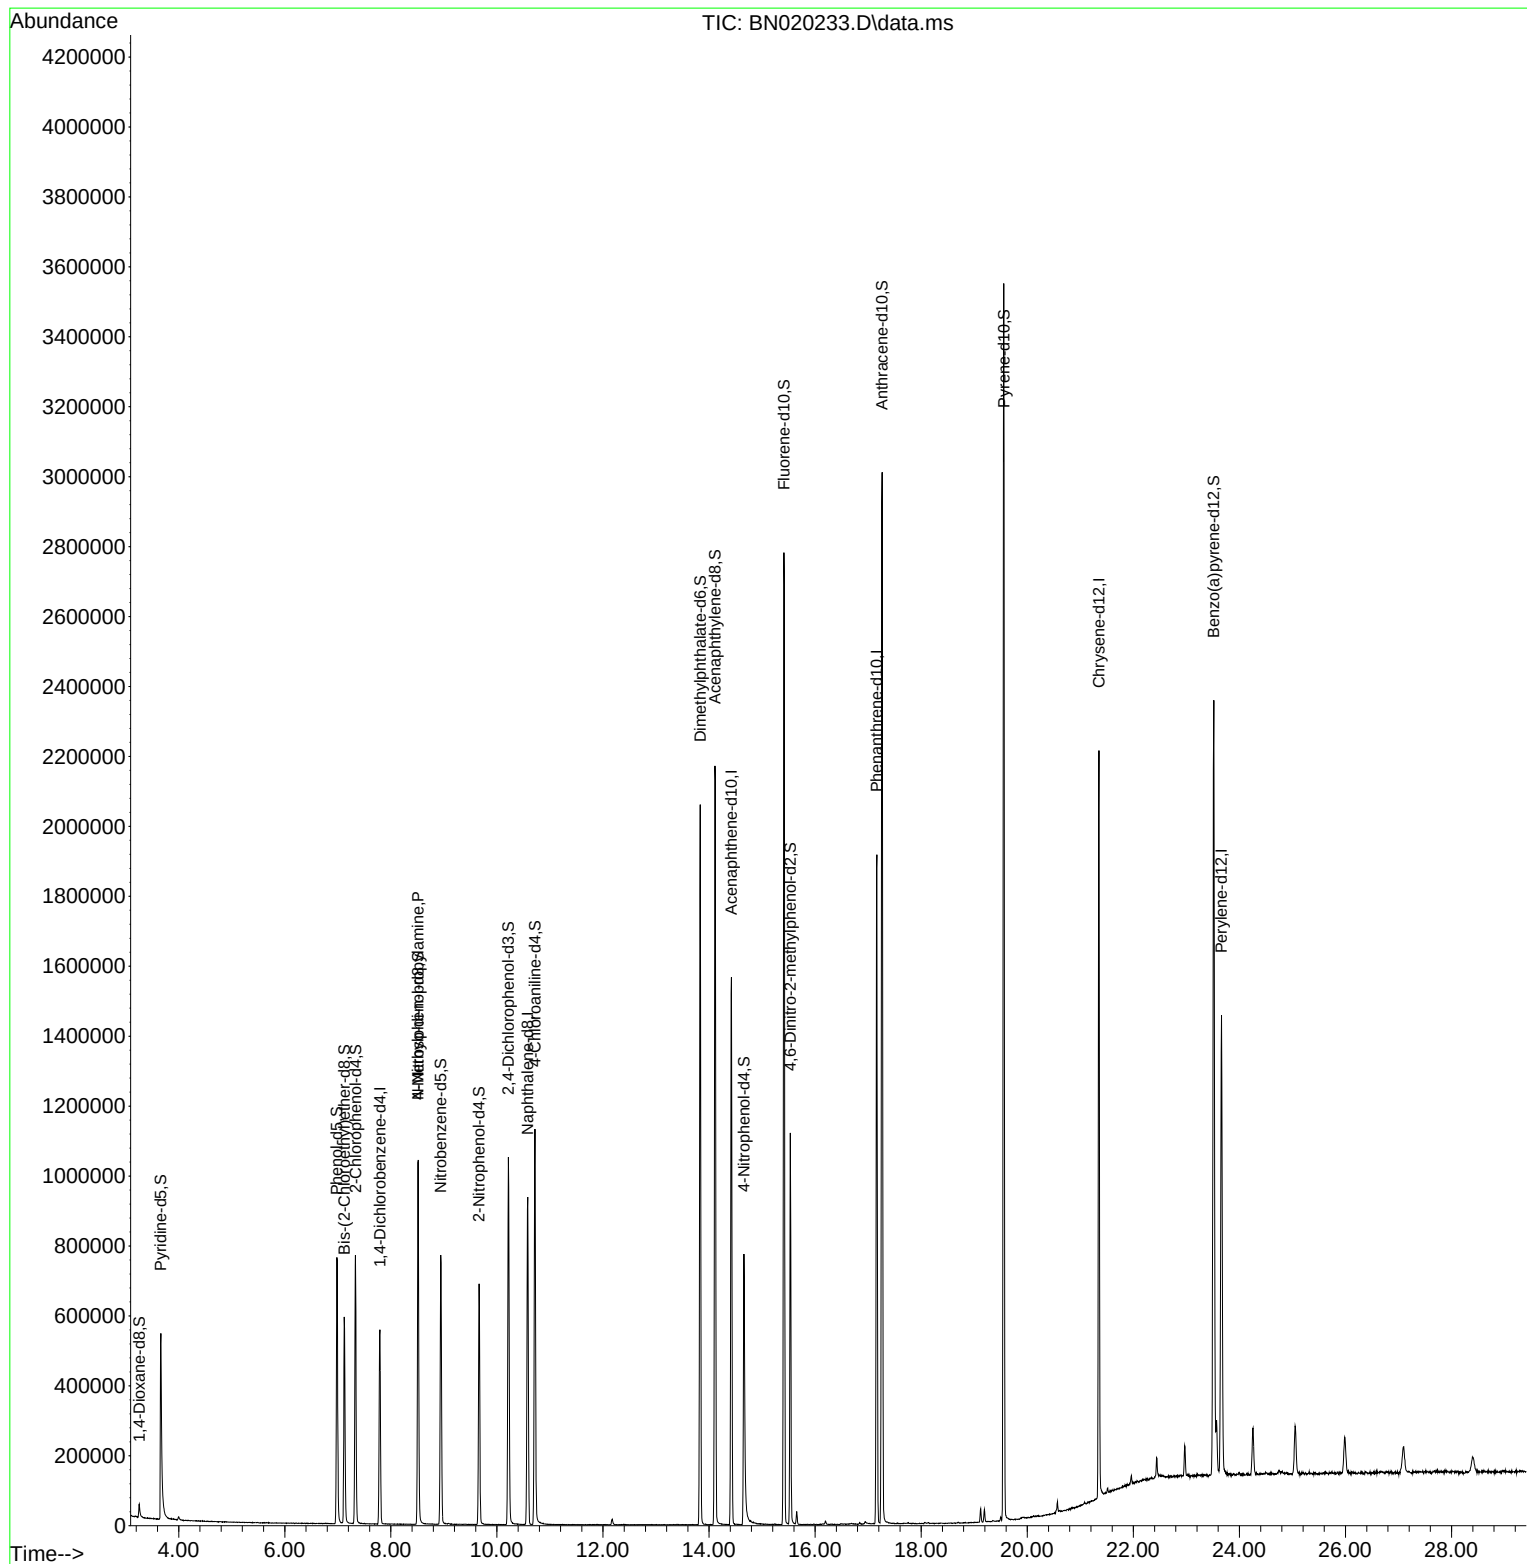

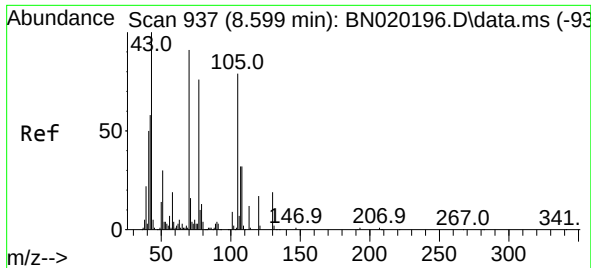

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.145 ng/ul
 RT: 8.510 min Scan# 91
 Delta R.T. -0.083 min
 Lab File: BN020233.D
 Acq: 17 Jun 2022 11:17

Instrument :
 BNA_N
 ClientSampleId :
 SBLK516

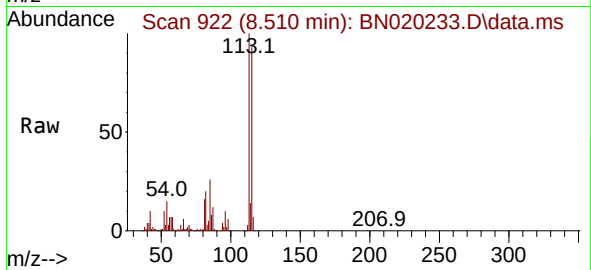

Tgt Ion:	70	Resp:	9914
Ion	Ratio	Lower	Upper
70	100		
42	395.5	47.8	71.6#
101	0.0	7.8	11.6#
130	0.0	15.8	23.8#

