

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020246.D
 Acq On : 17 Jun 2022 19:13
 Operator : CG/JU
 Sample : PB145516BS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS516

Quant Time: Jun 17 22:57:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 22:53:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	149686	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	741301	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.422	164	480214	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.163	188	985504	20.000	ng/u1	0.00
79) Chrysene-d12	21.357	240	818747	20.000	ng/u1	0.00
88) Perylene-d12	23.674	264	661151	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	22160	6.412	ng/uL	0.00
4) Pyridine-d5	3.664	84	321092	33.992	ng/u1	0.00
7) Phenol-d5	6.981	99	475233	38.368	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	275357	35.582	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	386296	38.384	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	414986	38.726	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	198396	35.179	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	221528	37.012	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	388641	37.195	ng/u1	0.00
31) 4-Chloroaniline-d4	10.716	131	550388	32.528	ng/u1	0.00
46) Dimethylphthalate-d6	13.840	166	1199220	34.321	ng/u1	0.01
49) Acenaphthylene-d8	14.116	160	1420279	35.050	ng/u1	0.00
54) 4-Nitrophenol-d4	14.657	143	237889	33.976	ng/u1	0.00
60) Fluorene-d10	15.416	176	996160	34.453	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.540	200	215419	37.736	ng/u1	0.00
73) Anthracene-d10	17.263	188	1501639	34.914	ng/u1	0.00
81) Pyrene-d10	19.557	212	1673852	37.711	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	1226418	37.913	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	47130	12.918	ng/uL#	91
5) Pyridine	3.681	79	340335	34.368	ng/u1	94
6) Benzaldehyde	6.928	77	281880	48.299	ng/u1	93
8) Phenol	7.011	94	510974	38.742	ng/u1	96
10) Bis(2-Chloroethyl)ether	7.216	93	379635	36.776	ng/u1	99
12) 2-Chlorophenol	7.363	128	408491	38.832	ng/u1	99
13) 2-Methylphenol	8.252	108	396473	39.102	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.322	45	594272	36.712	ng/u1	97
16) Acetophenone	8.610	105	612557	37.588	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.605	70	309316	37.155	ng/u1	93
18) 4-Methylphenol	8.581	108	443960	39.672	ng/u1	99
19) Hexachloroethane	8.869	117	151579	35.811	ng/u1	91
22) Nitrobenzene	8.987	77	462352	35.358	ng/u1	96
23) Isophorone	9.516	82	894728	34.655	ng/u1	98
25) 2-Nitrophenol	9.699	139	247349	37.400	ng/u1	96
26) 2,4-Dimethylphenol	9.775	107	479979	35.031	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.999	93	550373	34.834	ng/u1	99
29) 2,4-Dichlorophenol	10.246	162	407232	37.678	ng/u1	98
30) Naphthalene	10.634	128	1323970	34.461	ng/u1	99
32) 4-Chloroaniline	10.740	127	554474	32.762	ng/u1	99
33) Hexachlorobutadiene	10.922	225	207942	33.510	ng/u1	96
34) Caprolactam	11.504	113	107280	25.418	ng/u1	98
35) 4-Chloro-3-methylphenol	11.893	107	495260	38.807	ng/u1	97
36) 2-Methylnaphthalene	12.246	142	916749	35.295	ng/u1	98


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020246.D
 Acq On : 17 Jun 2022 19:13
 Operator : CG/JU
 Sample : PB145516BS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SLCS516

Quant Time: Jun 17 22:57:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 22:53:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.463	142	936428	35.329	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.616	216	420304	34.317	ng/ul	98
40) Hexachlorocyclopentadiene	12.598	237	212482	28.520	ng/ul	96
41) 2,4,6-Trichlorophenol	12.863	196	318038	37.660	ng/ul	92
42) 2,4,5-Trichlorophenol	12.951	196	350668	37.492	ng/ul	100
43) 1,1'-Biphenyl	13.257	154	1225122	34.453	ng/ul	99
44) 2-Chloronaphthalene	13.298	162	946370	35.082	ng/ul	99
45) 2-Nitroaniline	13.504	65	329907	39.311	ng/ul	96
47) Dimethylphthalate	13.887	163	1233691	35.073	ng/ul	99
48) 2,6-Dinitrotoluene	14.004	165	265020	38.535	ng/ul	96
50) Acenaphthylene	14.145	152	1556827	34.702	ng/ul	99
51) 3-Nitroaniline	14.328	138	277934	38.227	ng/ul	100
52) Acenaphthene	14.487	153	1012084	34.537	ng/ul	98
53) 2,4-Dinitrophenol	14.540	184	161794	36.745	ng/ul	100
55) 4-Nitrophenol	14.675	109	198844	33.270	ng/ul	97
56) Dibenzofuran	14.822	168	1431917	34.684	ng/ul	97
57) 2,4-Dinitrotoluene	14.793	165	392012	38.497	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.057	232	262018	35.687	ng/ul	92
59) Diethylphthalate	15.251	149	1271893	35.121	ng/ul	98
61) Fluorene	15.469	166	1111471	34.598	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.469	204	504823	34.122	ng/ul	93
63) 4-Nitroaniline	15.492	138	285250	41.986	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.557	198	222944	38.520	ng/ul	98
67) N-Nitrosodiphenylamine	15.681	169	1027013	36.351	ng/ul	97
68) 4-Bromophenyl-phenylether	16.357	248	317209	36.961	ng/ul#	91
69) Hexachlorobenzene	16.481	284	354876	35.972	ng/ul#	92
70) Atrazine	16.634	200	364394	36.965	ng/ul	95
71) Pentachlorophenol	16.822	266	223290	36.340	ng/ul	97
72) Phenanthrene	17.210	178	1834857	35.280	ng/ul	99
74) Anthracene	17.298	178	1858851	35.545	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.228	216	458000	34.705	ng/ul	99
76) Pentachlorobenzene	14.745	250	421103	36.104	ng/ul	98
77) Carbazole	17.569	167	1752427	36.834	ng/ul	96
78) Di-n-butylphthalate	18.139	149	2196094	37.226	ng/ul	99
80) Fluoranthene	19.228	202	2108666	39.335	ng/ul	97
82) Pyrene	19.592	202	2097006	38.129	ng/ul	97
83) Butylbenzylphthalate	20.492	149	1033190	41.743	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.275	252	564767	36.116	ng/ul#	97
85) Benzo(a)anthracene	21.339	228	1836473	35.521	ng/ul	94
86) Bis(2-ethylhexyl)phtha...	21.280	149	1451817	41.572	ng/ul	99
87) Chrysene	21.392	228	1780433	35.200	ng/ul	100
89) Di-n-octyl phthalate	22.174	149	2608402	48.473	ng/ul	100
90) Benzo(b)fluoranthene	22.969	252	1663926	40.100	ng/ul	98
91) Benzo(k)fluoranthene	23.016	252	1566967	39.669	ng/ul	96
93) Benzo(a)pyrene	23.569	252	1553914	38.687	ng/ul	93
94) Indeno(1,2,3-cd)pyrene	26.045	276	1570606	38.006	ng/ul	92
95) Dibenzo(a,h)anthracene	26.062	278	1320752	37.418	ng/ul#	95
96) Benzo(g,h,i)perylene	26.780	276	1341934	38.453	ng/ul#	95





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
 1,4-Dioxane
 Concen: 12.918 ng/uL
 RT: 3.293 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13




Instrument :
 BNA_N
 ClientSampleId :
 SLCS516


Tgt Ion: 88 Resp: 47130
 Ion Ratio Lower Upper
 88 100
 43 35.1 22.4 33.6#
 58 83.1 61.0 91.4



#5
 Pyridine
 Concen: 34.368 ng/uL
 RT: 3.681 min Scan# 101
 Delta R.T. -0.000 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13

Tgt Ion: 79 Resp: 340335
 Ion Ratio Lower Upper
 79 100
 52 88.7 65.0 97.4
 51 41.0 31.6 47.4


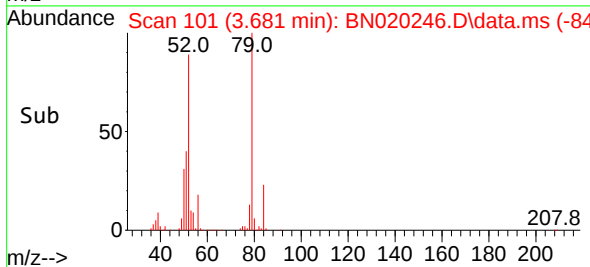

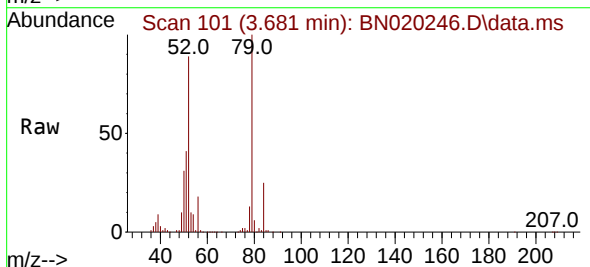




#6
Benzaldehyde
Concen: 48.299 ng/ul
RT: 6.928 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion: 77 Resp: 281880
Ion Ratio Lower Upper
77 100
105 98.4 74.7 112.1
106 95.3 70.2 105.4



#8
Phenol
Concen: 38.742 ng/ul
RT: 7.011 min Scan# 667
Delta R.T. -0.000 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion: 94 Resp: 510974
Ion Ratio Lower Upper
94 100
65 31.2 23.6 35.4
66 42.2 31.2 46.8

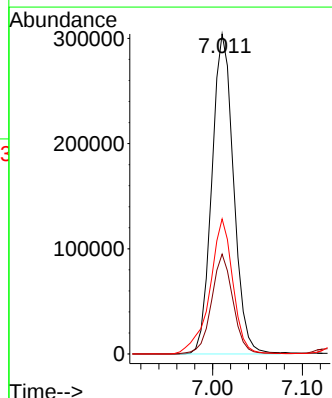







#10
 Bis(2-Chloroethyl)ether
 Concen: 36.776 ng/ul
 RT: 7.216 min Scan# 702
 Delta R.T. 0.006 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13

Instrument :
 BNA_N
 ClientSampleId :
 SLCS516

Tgt Ion: 93 Resp: 379635




Ion	Ratio	Lower	Upper
93	100		
63	79.1	63.4	95.0
95	31.2	26.2	39.2

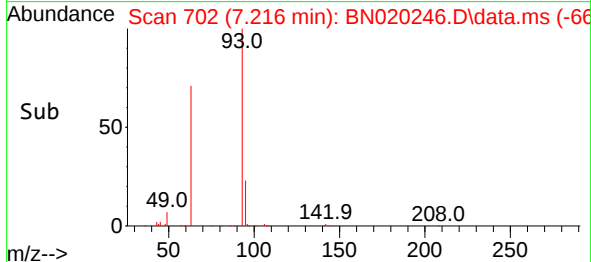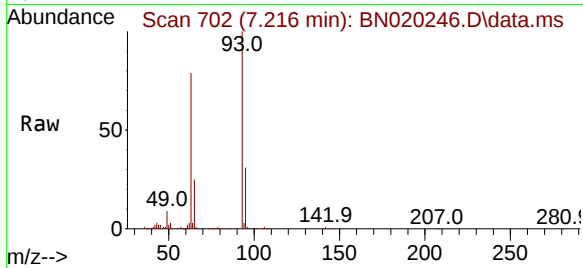


#12
 2-Chlorophenol
 Concen: 38.832 ng/ul
 RT: 7.363 min Scan# 727
 Delta R.T. -0.000 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13

Tgt Ion: 128 Resp: 408491

Ion	Ratio	Lower	Upper
128	100		
64	47.7	38.6	57.8
130	31.7	25.0	37.4


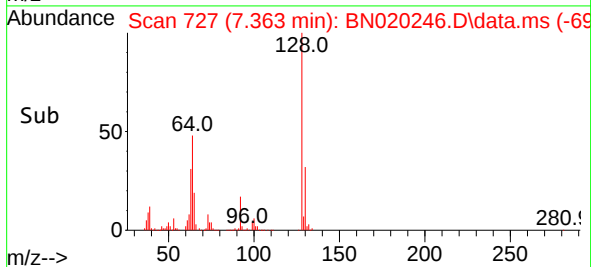

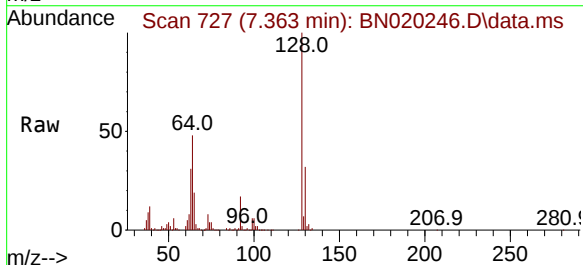




#13
2-Methylphenol
Concen: 39.102 ng/ul
RT: 8.252 min Scan# 81
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:108 Resp: 396473
Ion Ratio Lower Upper
108 100
107 90.4 71.5 107.3

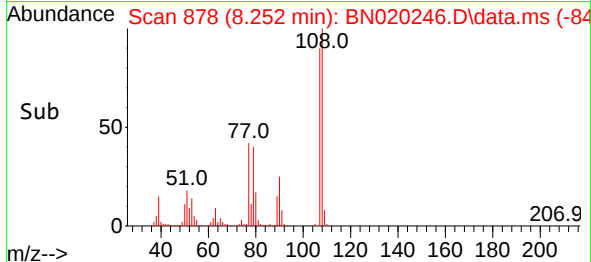

#14
2,2'-oxybis(1-Chloropropane)
Concen: 36.712 ng/ul
RT: 8.322 min Scan# 890
Delta R.T. -0.000 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion: 45 Resp: 594272
Ion Ratio Lower Upper
45 100
77 12.5 10.9 16.3
79 9.7 8.6 13.0


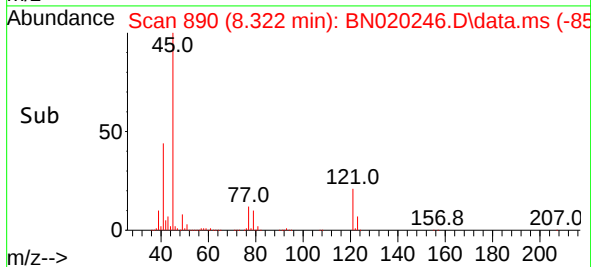

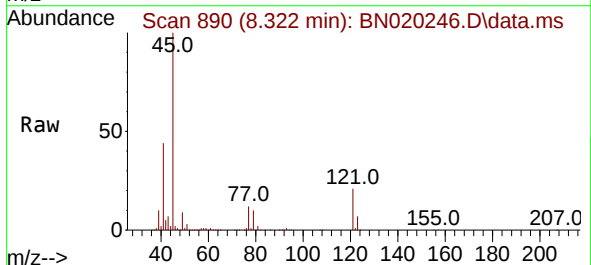




#16
Acetophenone
Concen: 37.588 ng/ul
RT: 8.610 min Scan# 91
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:105 Resp: 612557
Ion Ratio Lower Upper
105 100
77 78.8 63.5 95.3
51 30.7 23.5 35.3



#17
N-Nitroso-di-n-propylamine
Concen: 37.155 ng/ul
RT: 8.605 min Scan# 938
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion: 70 Resp: 309316
Ion Ratio Lower Upper
70 100
42 65.3 47.8 71.6
101 10.4 7.8 11.6
130 22.9 15.8 23.8


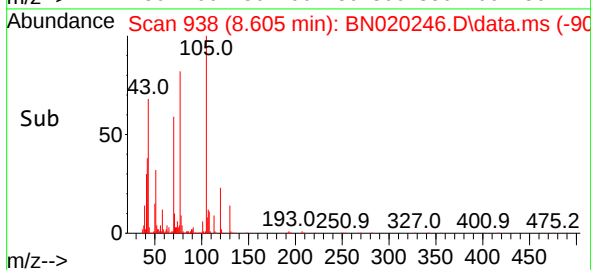






#18
4-Methylphenol
Concen: 39.672 ng/ul
RT: 8.581 min Scan# 911
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:108 Resp: 443960
Ion Ratio Lower Upper
108 100
107 111.4 88.0 132.0

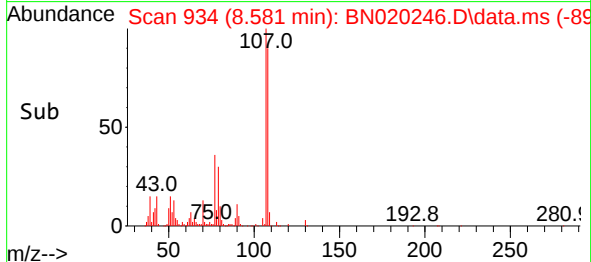

#19
Hexachloroethane
Concen: 35.811 ng/ul
RT: 8.869 min Scan# 983
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:117 Resp: 151579
Ion Ratio Lower Upper
117 100
201 91.4 83.2 124.8
199 59.3 50.2 75.4


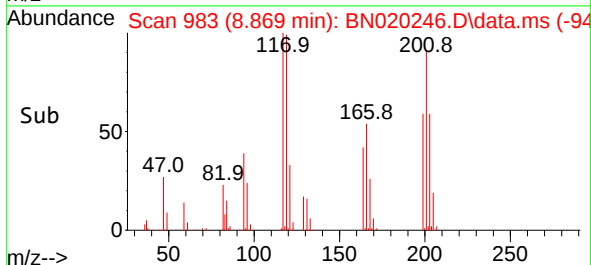
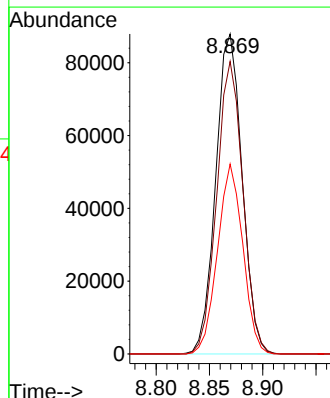
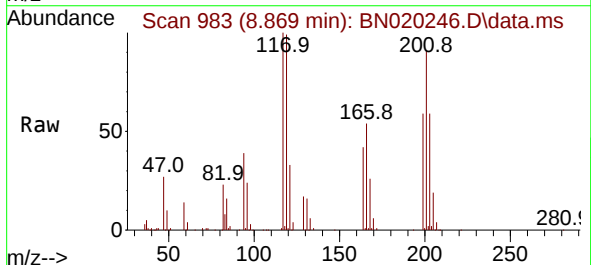




#22
Nitrobenzene
Concen: 35.358 ng/ul
RT: 8.987 min Scan# 1003
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion: 77 Resp: 462352
Ion Ratio Lower Upper
77 100
123 46.3 34.5 51.7
65 14.7 11.1 16.7

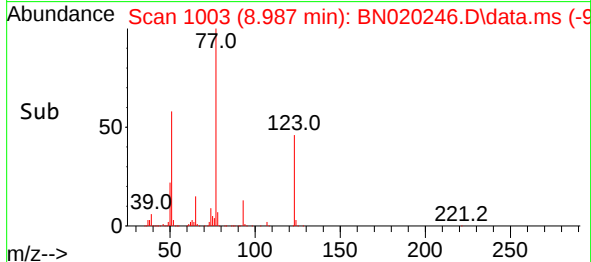

#23
Isophorone
Concen: 34.655 ng/ul
RT: 9.516 min Scan# 1093
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion: 82 Resp: 894728
Ion Ratio Lower Upper
82 100
95 7.6 5.8 8.8
138 18.3 13.8 20.8

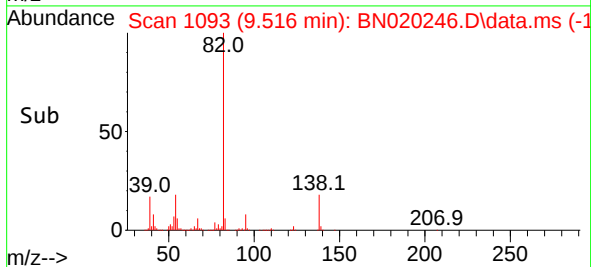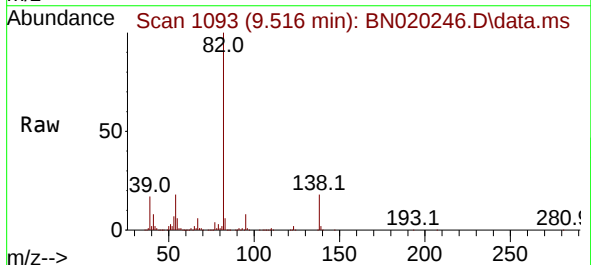

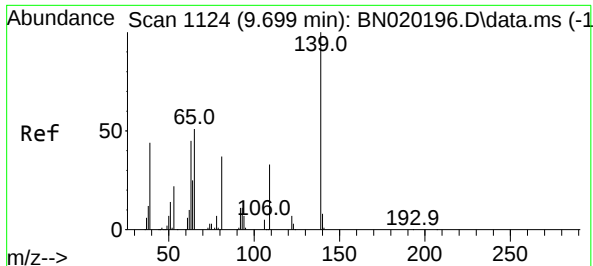

#25

2-Nitrophenol

Concen: 37.400 ng/ul

RT: 9.699 min Scan# 1124

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:139 Resp: 247349

Ion Ratio Lower Upper

139 100

65 51.0 43.7 65.5

109 31.1 25.8 38.6

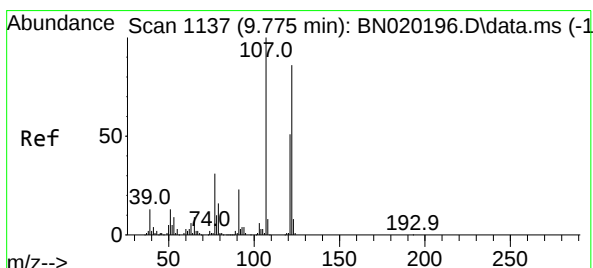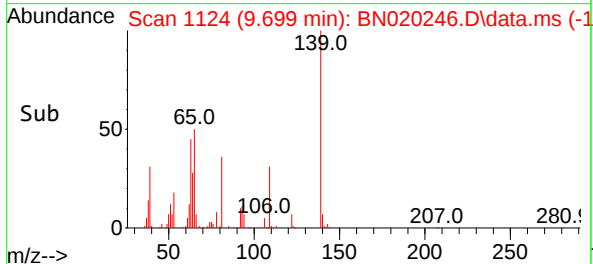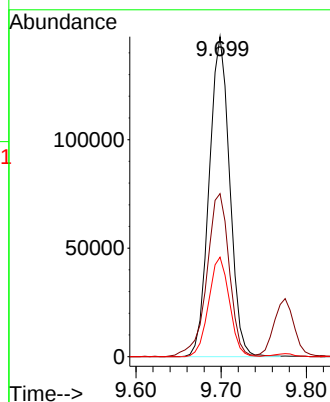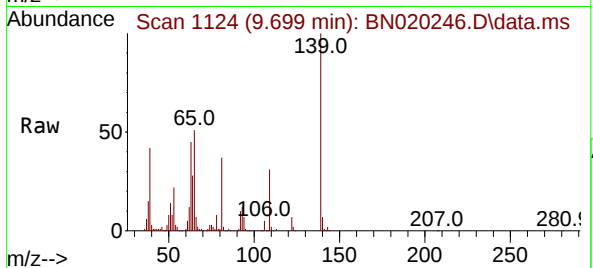

#26

2,4-Dimethylphenol

Concen: 35.031 ng/ul

RT: 9.775 min Scan# 1137

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion:107 Resp: 479979


Ion Ratio Lower Upper

107 100

121 48.8 38.3 57.5

122 85.2 66.3 99.5

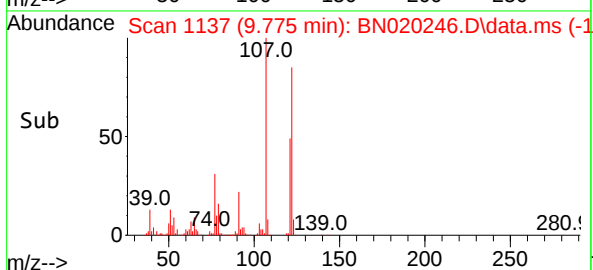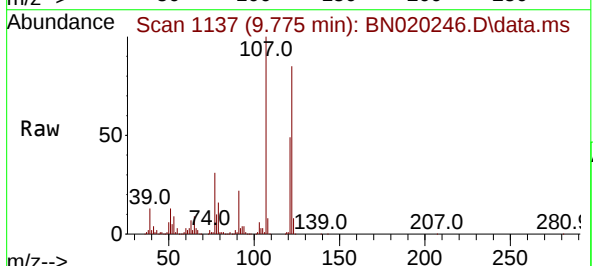

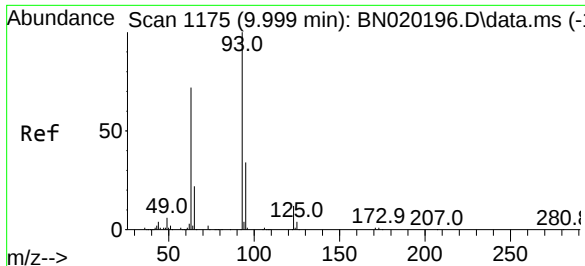

#27

Bis(2-Chloroethoxy)methane

Concen: 34.834 ng/ul

RT: 9.999 min Scan# 1175

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion: 93 Resp: 550373

Ion Ratio Lower Upper

93 100

95 32.0 25.4 38.0

123 11.3 8.3 12.5

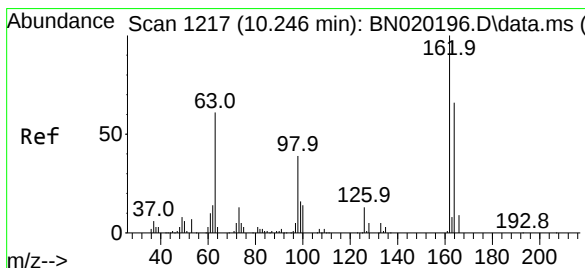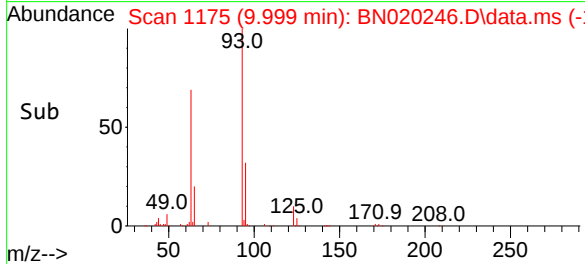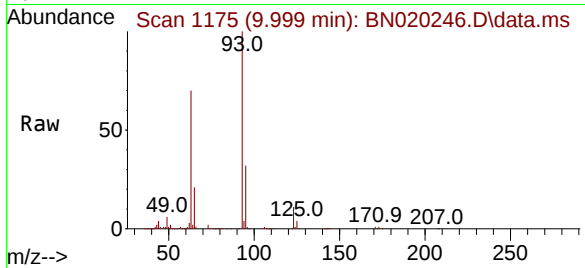

#29

2,4-Dichlorophenol

Concen: 37.678 ng/ul

RT: 10.246 min Scan# 1217

Delta R.T. -0.000 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion: 162 Resp: 407232


Ion Ratio Lower Upper

162 100

164 63.6 52.9 79.3

98 37.5 29.8 44.8


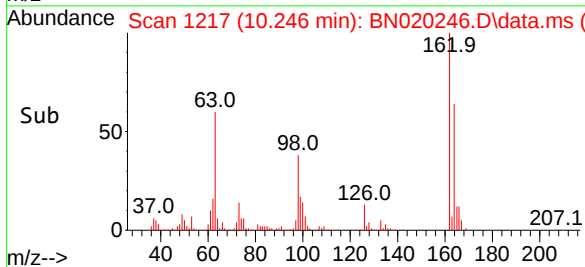

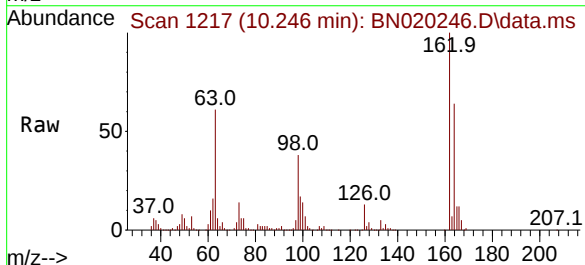




#30
Naphthalene
Concen: 34.461 ng/ul
RT: 10.634 min Scan# 1283
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:128 Resp: 1323970
Ion Ratio Lower Upper
128 100
129 10.7 8.7 13.1
127 12.7 10.6 16.0

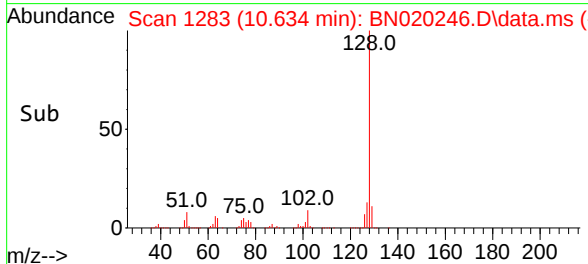

#32
4-Chloroaniline
Concen: 32.762 ng/ul
RT: 10.740 min Scan# 1301
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:127 Resp: 554474
Ion Ratio Lower Upper
127 100
129 32.0 26.1 39.1


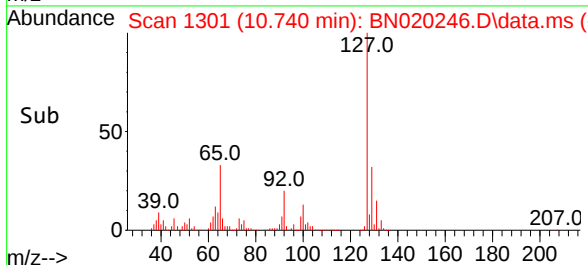

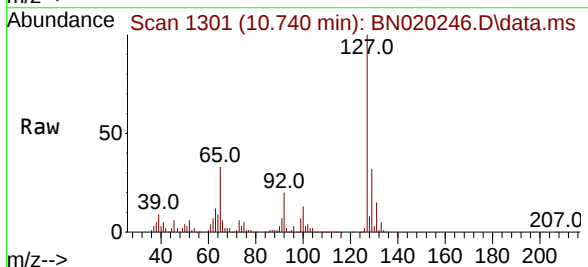




#33
Hexachlorobutadiene
Concen: 33.510 ng/ul
RT: 10.922 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:225 Resp: 207942
Ion Ratio Lower Upper
225 100
223 60.3 51.8 77.6
227 61.0 50.6 76.0



#34
Caprolactam
Concen: 25.418 ng/ul
RT: 11.504 min Scan# 1431
Delta R.T. 0.023 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:113 Resp: 107280
Ion Ratio Lower Upper
113 100
55 179.4 145.5 218.3
56 134.5 106.5 159.7


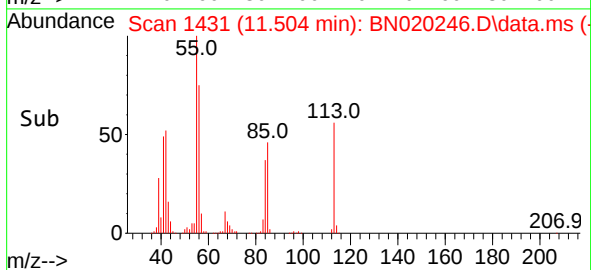

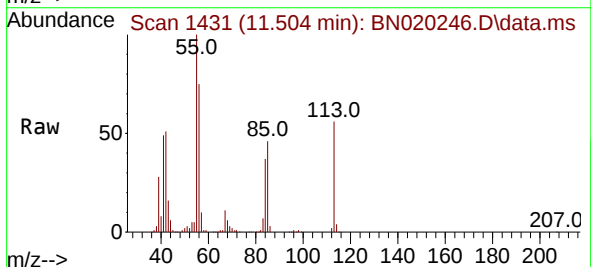




#35
4-Chloro-3-methylphenol
Concen: 38.807 ng/ul
RT: 11.893 min Scan# 1497
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:107 Resp: 495260
Ion Ratio Lower Upper
107 100
144 25.3 20.6 31.0
142 74.6 62.2 93.4



#36
2-Methylnaphthalene
Concen: 35.295 ng/ul
RT: 12.246 min Scan# 1557
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:142 Resp: 916749
Ion Ratio Lower Upper
142 100
141 89.8 70.6 105.8

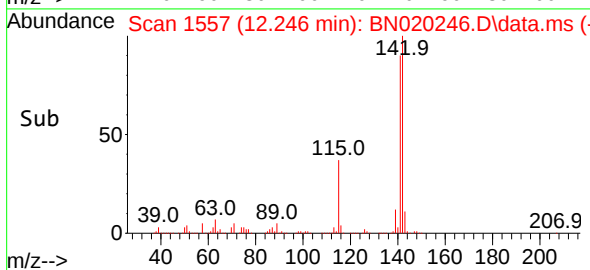



#37

1-Methylnaphthalene

Concen: 35.329 ng/ul

RT: 12.463 min Scan# 11

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:142 Resp: 936428

Ion Ratio Lower Upper

142 100

141 89.9 70.9 106.3

116 3.7 3.1 4.7

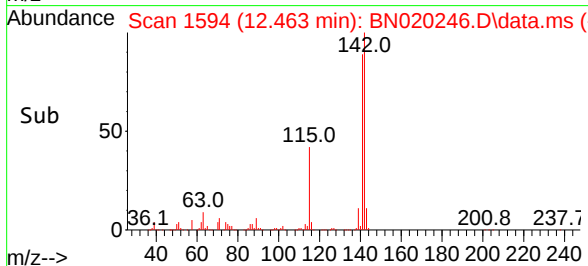

#39

1,2,4,5-Tetrachlorobenzene

Concen: 34.317 ng/ul

RT: 12.616 min Scan# 1620

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Tgt Ion:216 Resp: 420304




Ion Ratio Lower Upper


216 100

214 79.8 63.4 95.0

179 24.4 17.8 26.8

108 21.1 15.1 22.7


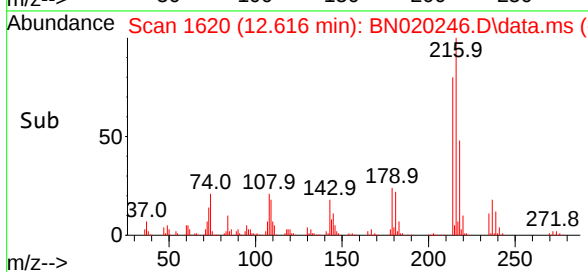

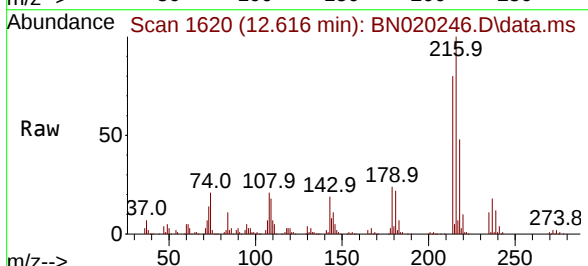




#40
Hexachlorocyclopentadiene
Concen: 28.520 ng/ul
RT: 12.598 min Scan# 1617
Delta R.T. -0.000 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:237 Resp: 212482
Ion Ratio Lower Upper
237 100
235 64.5 48.8 73.2
272 12.6 9.3 13.9

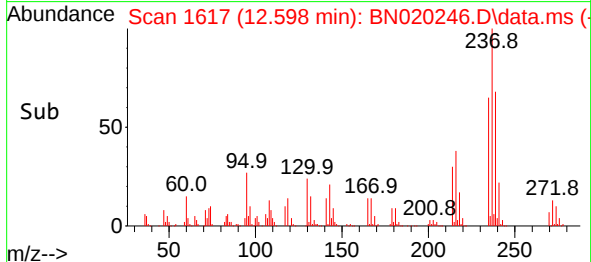

#41
2,4,6-Trichlorophenol
Concen: 37.660 ng/ul
RT: 12.863 min Scan# 1662
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:196 Resp: 318038
Ion Ratio Lower Upper
196 100
198 90.0 79.8 119.8
200 30.2 25.0 37.6

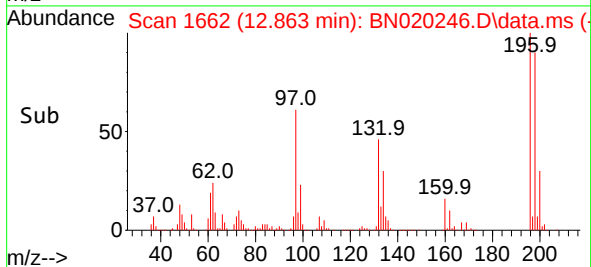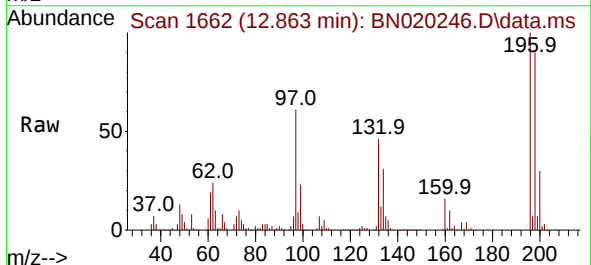



#42

2,4,5-Trichlorophenol

Concen: 37.492 ng/ul

RT: 12.951 min Scan# 1

Delta R.T. -0.000 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:196 Resp: 350668

Ion Ratio Lower Upper

196 100

198 97.2 77.6 116.4

200 31.2 24.4 36.6



#43

1,1'-Biphenyl

Concen: 34.453 ng/ul

RT: 13.257 min Scan# 1729

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion:154 Resp: 1225122


Ion Ratio Lower Upper

154 100

153 40.2 31.5 47.3

76 13.1 10.5 15.7

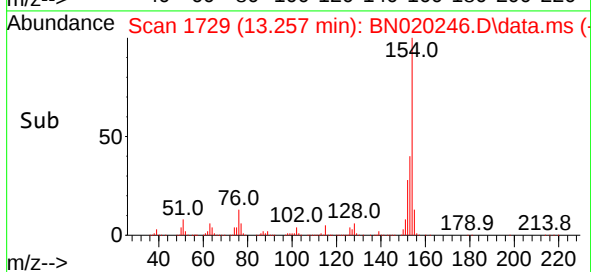



#44

2-Chloronaphthalene

Concen: 35.082 ng/ul

RT: 13.298 min Scan# 11

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:162 Resp: 946370

Ion Ratio Lower Upper

162 100

164 31.9 25.8 38.6

127 40.2 31.4 47.2



#45

2-Nitroaniline

Concen: 39.311 ng/ul

RT: 13.504 min Scan# 1771

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion: 65 Resp: 329907


Ion Ratio Lower Upper

65 100

92 67.5 54.1 81.1

138 102.7 77.0 115.4


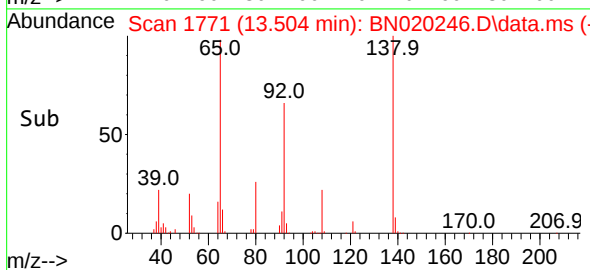






#47
Dimethylphthalate
Concen: 35.073 ng/ul
RT: 13.887 min Scan# 1836
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:163 Resp: 1233691
Ion Ratio Lower Upper
163 100
194 3.8 3.4 5.0
164 9.8 7.7 11.5

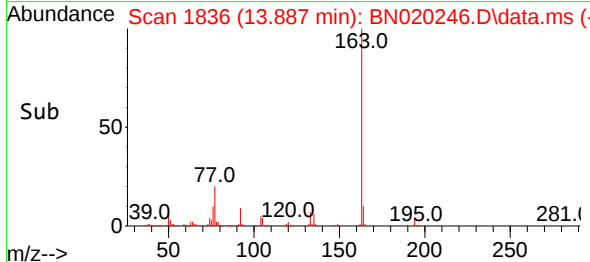

#48
2,6-Dinitrotoluene
Concen: 38.535 ng/ul
RT: 14.004 min Scan# 1856
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:165 Resp: 265020
Ion Ratio Lower Upper
165 100
89 59.4 50.6 75.8
121 22.5 17.9 26.9


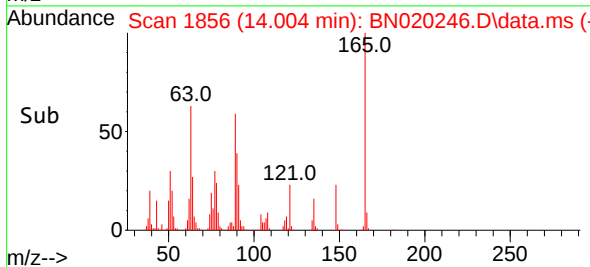

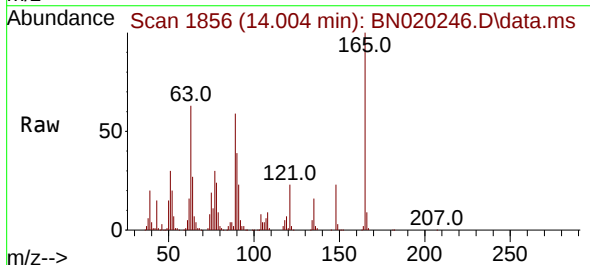




#50
Acenaphthylene
Concen: 34.702 ng/ul
RT: 14.145 min Scan# 1880
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:152 Resp: 1556827
Ion Ratio Lower Upper
152 100
151 20.5 16.0 24.0
153 13.6 10.7 16.1

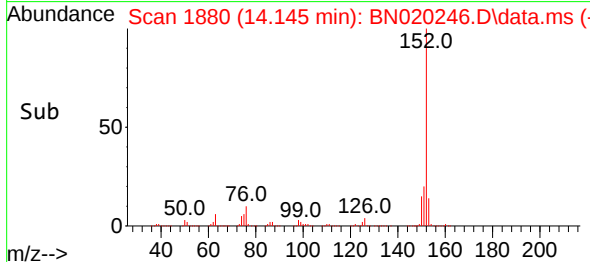

#51
3-Nitroaniline
Concen: 38.227 ng/ul
RT: 14.328 min Scan# 1911
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:138 Resp: 277934
Ion Ratio Lower Upper
138 100
108 11.3 8.6 12.8
92 116.0 92.9 139.3


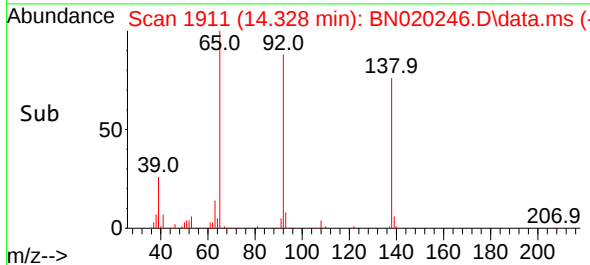

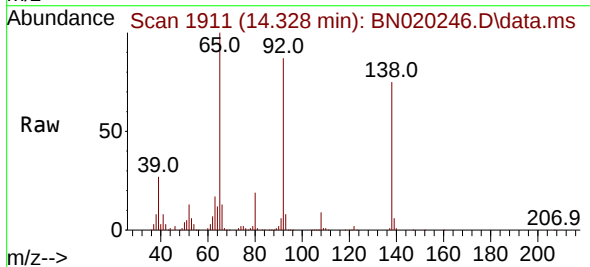




#52
Acenaphthene
Concen: 34.537 ng/ul
RT: 14.487 min Scan# 1938
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:153 Resp: 1012084
Ion Ratio Lower Upper
153 100
152 46.2 38.4 57.6
154 88.9 69.7 104.5

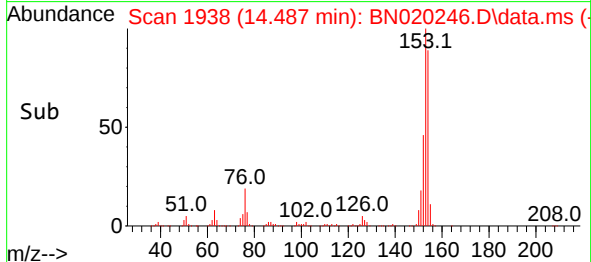

#53
2,4-Dinitrophenol
Concen: 36.745 ng/ul
RT: 14.540 min Scan# 1947
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:184 Resp: 161794
Ion Ratio Lower Upper
184 100
63 69.2 55.9 83.9
154 66.4 53.1 79.7


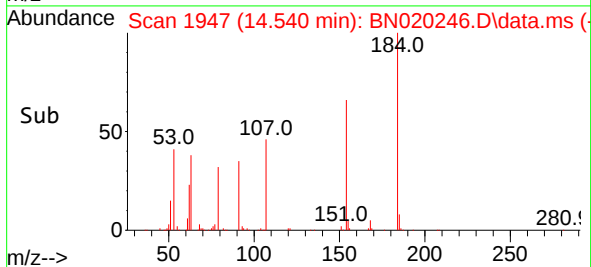

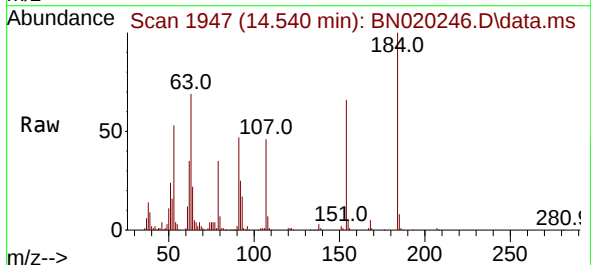




#55
4-Nitrophenol
Concen: 33.270 ng/ul
RT: 14.675 min Scan# 1970
Delta R.T. -0.000 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:109 Resp: 198844
Ion Ratio Lower Upper
109 100
139 129.0 100.1 150.1
65 133.3 104.6 157.0

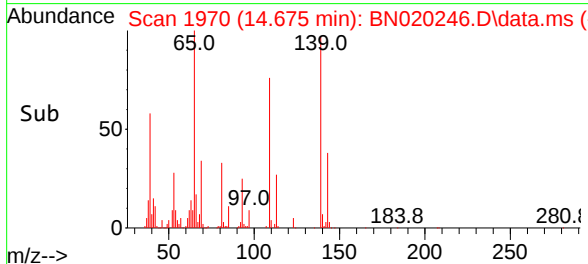

#56
Dibenzofuran
Concen: 34.684 ng/ul
RT: 14.822 min Scan# 1995
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:168 Resp: 1431917
Ion Ratio Lower Upper
168 100
139 40.8 31.1 46.7


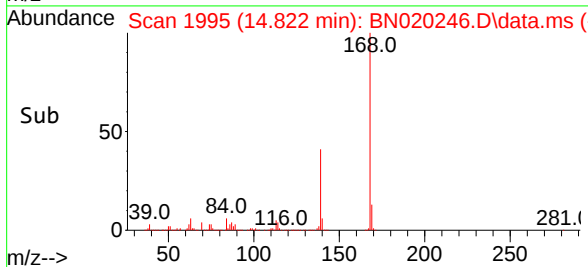

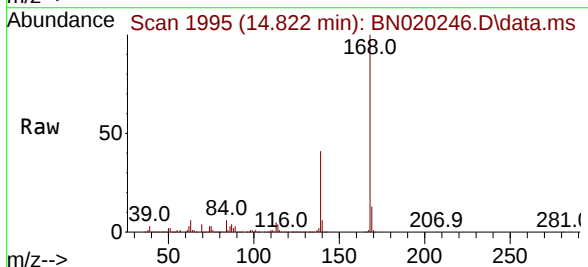




#57
2,4-Dinitrotoluene
Concen: 38.497 ng/ul
RT: 14.793 min Scan# 1989
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:165 Resp: 392012
Ion Ratio Lower Upper
165 100
63 46.4 36.3 54.5
182 3.1 2.3 3.5

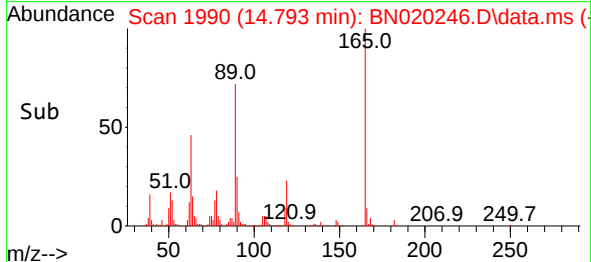

#58
2,3,4,6-Tetrachlorophenol
Concen: 35.687 ng/ul
RT: 15.057 min Scan# 2035
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:232 Resp: 262018
Ion Ratio Lower Upper
232 100
131 55.1 38.5 57.7
130 2.8 2.2 3.2
166 35.3 25.8 38.8


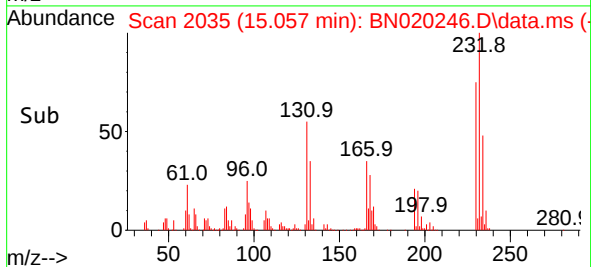

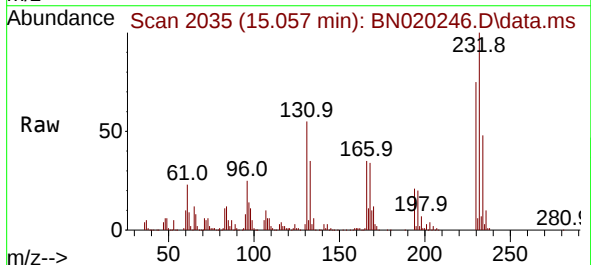




#59
Diethylphthalate
Concen: 35.121 ng/ul
RT: 15.251 min Scan# 2068
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:149 Resp: 1271893
Ion Ratio Lower Upper
149 100
177 20.8 17.8 26.8
150 12.6 10.5 15.7

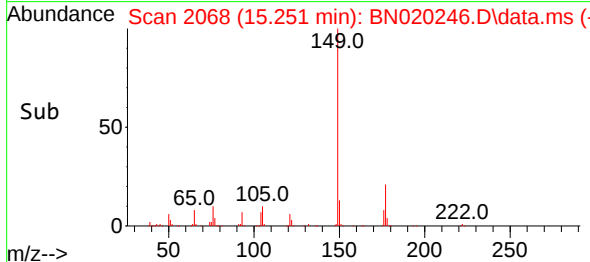

#61
Fluorene
Concen: 34.598 ng/ul
RT: 15.469 min Scan# 2105
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:166 Resp: 1111471
Ion Ratio Lower Upper
166 100
165 96.2 77.7 116.5
167 13.7 11.1 16.7


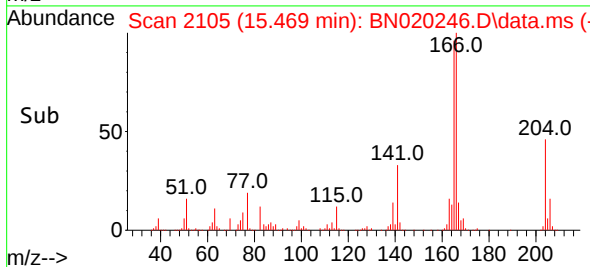

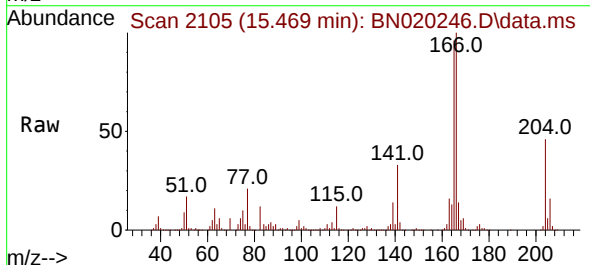




#62
4-Chlorophenyl-phenylether
Concen: 34.122 ng/ul
RT: 15.469 min Scan# 2104
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:204 Resp: 504823
Ion Ratio Lower Upper
204 100
206 33.9 26.7 40.1
141 71.1 50.2 75.2

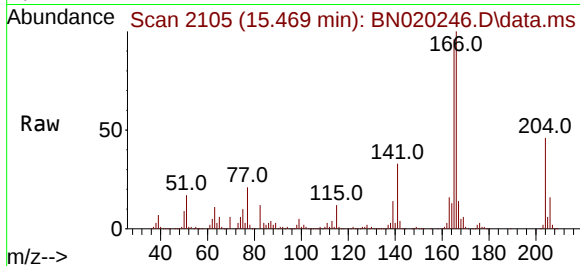

#63
4-Nitroaniline
Concen: 41.986 ng/ul
RT: 15.492 min Scan# 2109
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:138 Resp: 285250
Ion Ratio Lower Upper
138 100
92 53.1 41.0 61.6
108 85.0 65.3 97.9


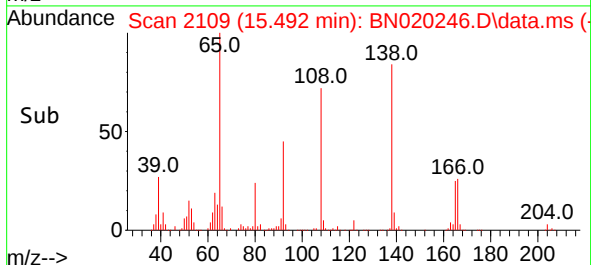
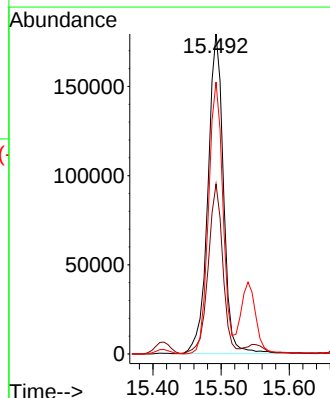
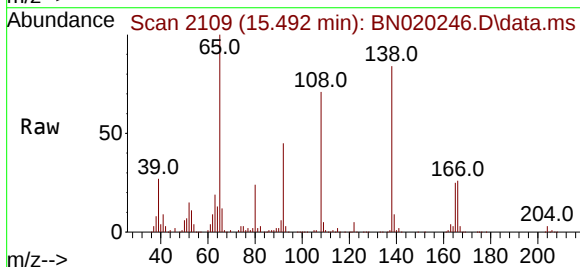




#66
 4,6-Dinitro-2-methylphenol
 Concen: 38.520 ng/ul
 RT: 15.557 min Scan# 2119
 Delta R.T. 0.012 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13




Instrument :
 BNA_N
 ClientSampleId :
 SLCS516


Tgt Ion:198 Resp: 222944
 Ion Ratio Lower Upper
 198 100
 182 3.6 3.0 4.4
 77 26.3 20.1 30.1



#67
 N-Nitrosodiphenylamine
 Concen: 36.351 ng/ul
 RT: 15.681 min Scan# 2141
 Delta R.T. 0.006 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13

Tgt Ion:169 Resp: 1027013
 Ion Ratio Lower Upper
 169 100
 168 67.6 52.4 78.6
 167 36.5 27.5 41.3









#68
4-Bromophenyl-phenylether
Concen: 36.961 ng/ul
RT: 16.357 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:248 Resp: 317209
Ion Ratio Lower Upper
248 100
250 97.0 77.8 116.8
141 95.8 62.6 93.8#

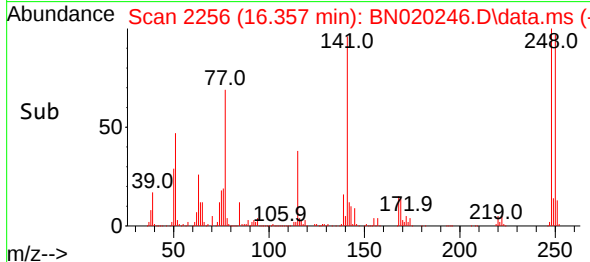

#69
Hexachlorobenzene
Concen: 35.972 ng/ul
RT: 16.481 min Scan# 2277
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:284 Resp: 354876
Ion Ratio Lower Upper
284 100
142 43.3 27.8 41.8#
249 32.9 25.7 38.5

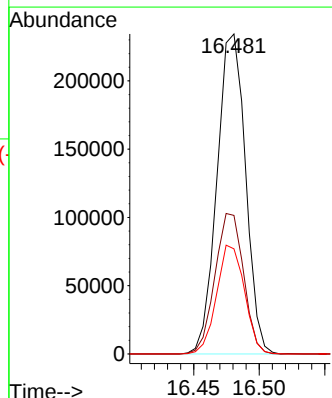



#70

Atrazine

Concen: 36.965 ng/ul

RT: 16.634 min Scan# 21

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:200 Resp: 364394

Ion Ratio Lower Upper

200 100

173 28.4 20.5 30.7

215 45.2 38.9 58.3



#71

Pentachlorophenol

Concen: 36.340 ng/ul

RT: 16.822 min Scan# 2335

Delta R.T. -0.000 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion:266 Resp: 223290


Ion Ratio Lower Upper

266 100

264 60.0 50.2 75.2

268 63.4 49.3 73.9

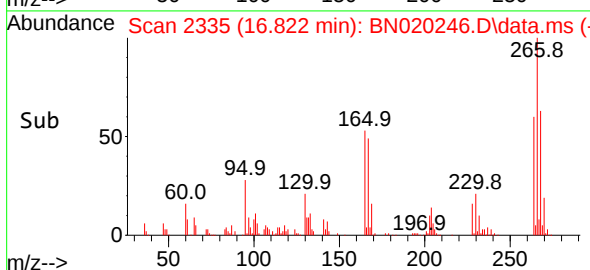



#72

Phenanthrene

Concen: 35.280 ng/ul

RT: 17.210 min Scan# 2401

Delta R.T. 0.012 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:178 Resp: 1834857

Ion Ratio Lower Upper

178 100

179 14.8 12.2 18.4

176 18.8 15.2 22.8

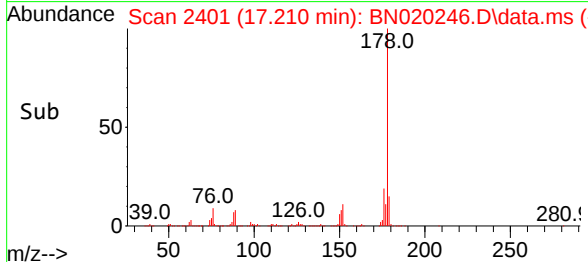

#74

Anthracene

Concen: 35.545 ng/ul

RT: 17.298 min Scan# 2416

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion:178 Resp: 1858851


Ion Ratio Lower Upper

178 100

179 15.7 13.0 19.4

176 18.5 15.5 23.3


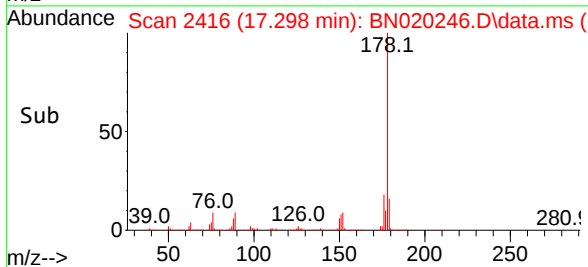

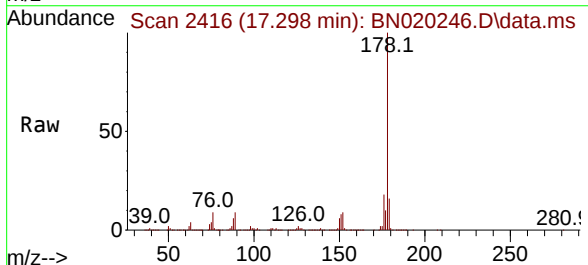




#75
1,2,3,4-Tetrachlorobenzene
Concen: 34.705 ng/uL
RT: 13.228 min Scan# 1723
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:216 Resp: 458000
Ion Ratio Lower Upper
216 100
214 77.2 63.2 94.8
218 47.8 37.9 56.9



#76
Pentachlorobenzene
Concen: 36.104 ng/uL
RT: 14.745 min Scan# 1982
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:250 Resp: 421103
Ion Ratio Lower Upper
250 100
248 64.6 53.0 79.4
252 64.8 53.4 80.2


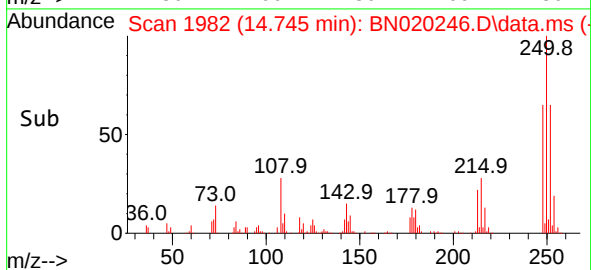

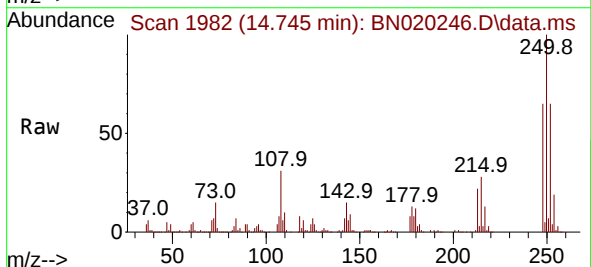




#77
 Carbazole
 Concen: 36.834 ng/ul
 RT: 17.569 min Scan# 2462
 Delta R.T. 0.006 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13




Instrument :
 BNA_N
 ClientSampleId :
 SLCS516


Tgt Ion:167 Resp: 1752427
 Ion Ratio Lower Upper
 167 100
 166 22.1 16.1 24.1
 139 13.9 10.2 15.2



#78
 Di-n-butylphthalate
 Concen: 37.226 ng/ul
 RT: 18.139 min Scan# 2559
 Delta R.T. 0.006 min
 Lab File: BN020246.D
 Acq: 17 Jun 2022 19:13

Tgt Ion:149 Resp: 2196094
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.1 10.7
 104 5.4 4.1 6.1


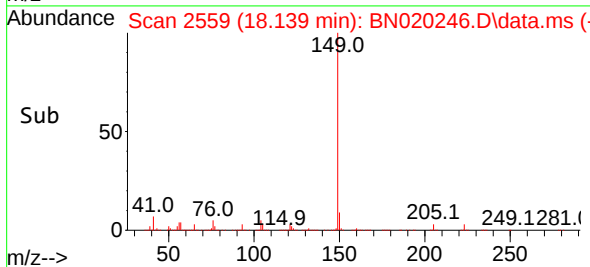

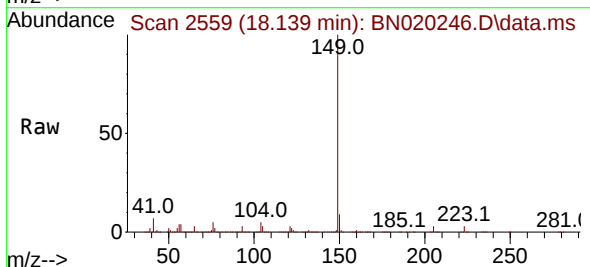




#80
Fluoranthene
Concen: 39.335 ng/u1
RT: 19.228 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:202 Resp: 2108666
Ion Ratio Lower Upper
202 100
101 12.2 8.9 13.3
100 9.2 6.7 10.1

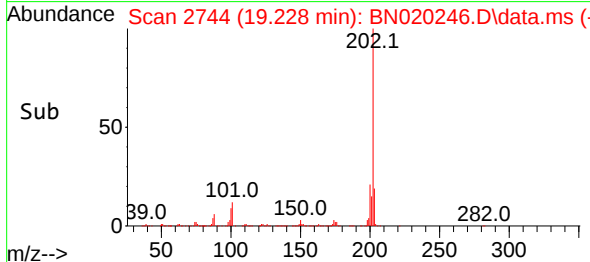

#82
Pyrene
Concen: 38.129 ng/u1
RT: 19.592 min Scan# 2806
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:202 Resp: 2097006
Ion Ratio Lower Upper
202 100
101 13.5 9.7 14.5
100 11.0 8.0 12.0

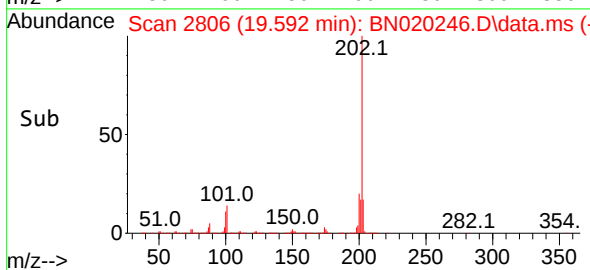



#83

Butylbenzylphthalate

Concen: 41.743 ng/ul

RT: 20.492 min Scan# 2959

Delta R.T. -0.000 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:149 Resp: 1033190

Ion Ratio Lower Upper

149 100

91 72.8 58.8 88.2

206 18.7 18.1 27.1

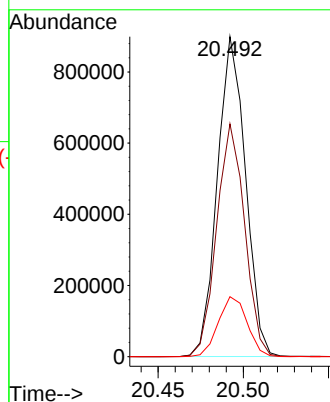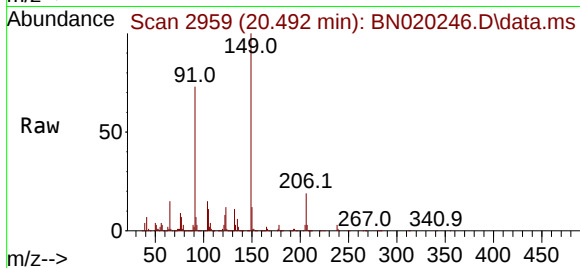

#84

3,3'-Dichlorobenzidine

Concen: 36.116 ng/ul

RT: 21.275 min Scan# 3092

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion:252 Resp: 564767


Ion Ratio Lower Upper

252 100

254 61.6 50.8 76.2

126 12.6 8.2 12.4#

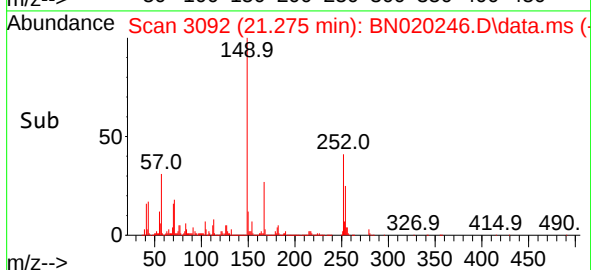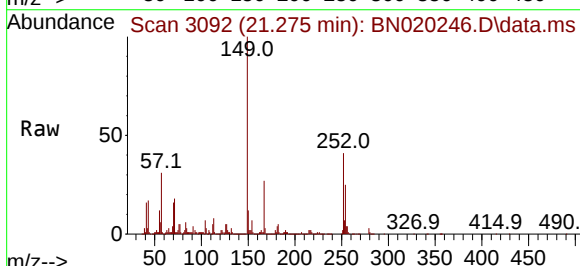



#85

Benzo(a)anthracene

Concen: 35.521 ng/ul

RT: 21.339 min Scan# 3102

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:228 Resp: 1836473

Ion Ratio Lower Upper

228 100

229 18.3 16.3 24.5

226 25.2 23.2 34.8



#86

Bis(2-ethylhexyl)phthalate

Concen: 41.572 ng/ul

RT: 21.280 min Scan# 3093

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13




Tgt Ion:149 Resp: 1451817


Ion Ratio Lower Upper

149 100

167 28.5 22.5 33.7

279 3.7 3.5 5.3

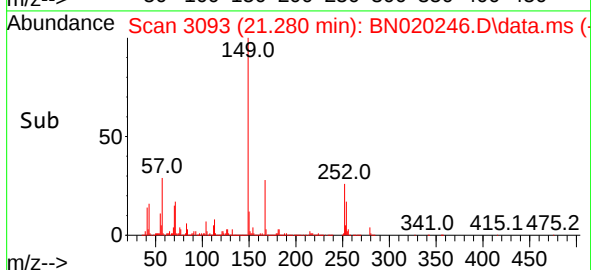



#87

Chrysene

Concen: 35.200 ng/ul

RT: 21.392 min Scan# 3111

Delta R.T. 0.006 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:228 Resp: 1780433

Ion Ratio Lower Upper

228 100

226 30.1 24.2 36.2

229 20.1 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 48.473 ng/ul




RT: 22.174 min Scan# 3245


Delta R.T. -0.000 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Tgt Ion:149 Resp: 2608402


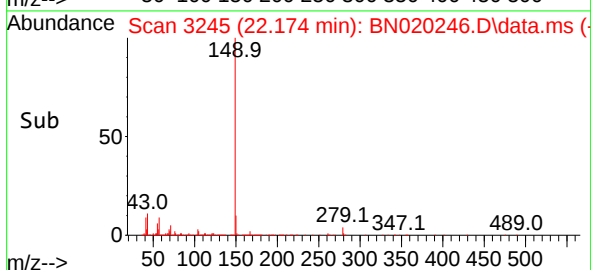






#90
Benzo(b)fluoranthene
Concen: 40.100 ng/ul
RT: 22.969 min Scan# 3379
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:252 Resp: 1663926
Ion Ratio Lower Upper
252 100
253 20.7 16.5 24.7
125 11.6 7.8 11.8



#91
Benzo(k)fluoranthene
Concen: 39.669 ng/ul
RT: 23.016 min Scan# 3388
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:252 Resp: 1566967
Ion Ratio Lower Upper
252 100
253 20.9 18.2 27.4
125 11.9 8.2 12.4


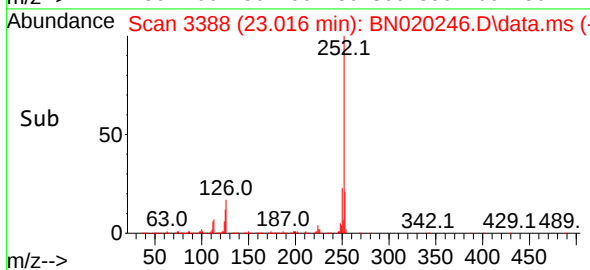






#93
Benzo(a)pyrene
Concen: 38.687 ng/ul
RT: 23.569 min Scan# 3481
Delta R.T. 0.006 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13




Instrument :
BNA_N
ClientSampleId :
SLCS516


Tgt Ion:252 Resp: 1553914
Ion Ratio Lower Upper
252 100
253 19.9 18.7 28.1
125 13.7 9.2 13.8

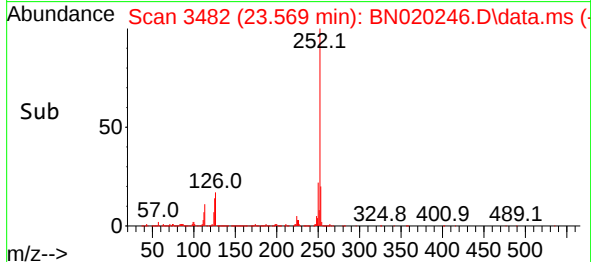

#94
Indeno(1,2,3-cd)pyrene
Concen: 38.006 ng/ul
RT: 26.045 min Scan# 3903
Delta R.T. 0.012 min
Lab File: BN020246.D
Acq: 17 Jun 2022 19:13

Tgt Ion:276 Resp: 1570606
Ion Ratio Lower Upper
276 100
138 28.9 19.5 29.3
277 22.9 21.4 32.0

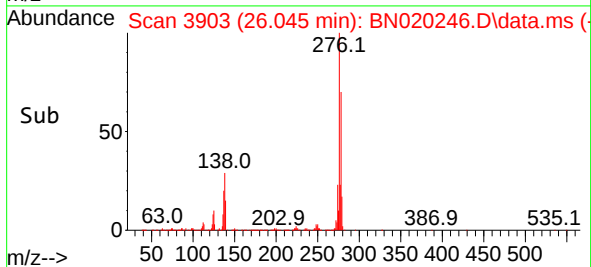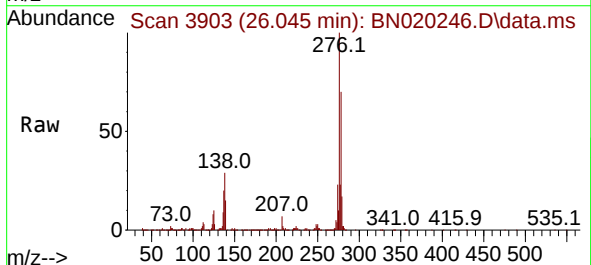



#95

Dibenzo(a,h)anthracene

Concen: 37.418 ng/ul

RT: 26.062 min Scan# 3905

Delta R.T. 0.012 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Instrument :

BNA_N

ClientSampleId :

SLCS516





Tgt Ion:278 Resp: 1320752

Ion Ratio Lower Upper

278 100

139 21.4 13.8 20.8#

279 23.5 18.3 27.5

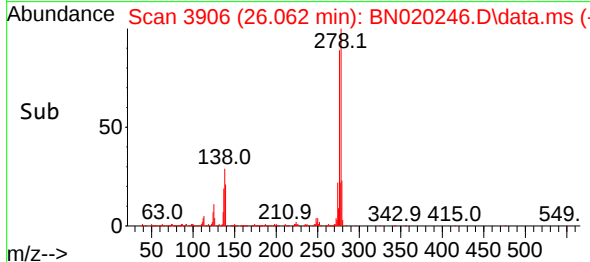

#96

Benzo(g,h,i)perylene

Concen: 38.453 ng/ul

RT: 26.780 min Scan# 4028

Delta R.T. 0.012 min

Lab File: BN020246.D

Acq: 17 Jun 2022 19:13

Tgt Ion:276 Resp: 1341934

Ion Ratio Lower Upper

276 100

138 25.8 17.0 25.6#

277 22.9 17.8 26.6

