




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020241.D
Acq On : 17 Jun 2022 16:10
Operator : CG/JU
Sample : N3313-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7N3

Manual IntegrationsAPPROVED

Quant Time: Jun 17 22:57:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 22:53:31 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :mohammad ahmed 06/22/2022

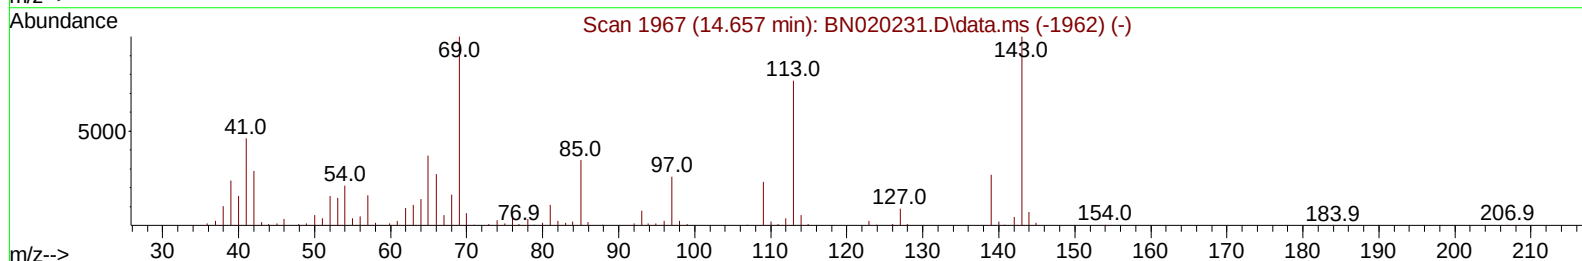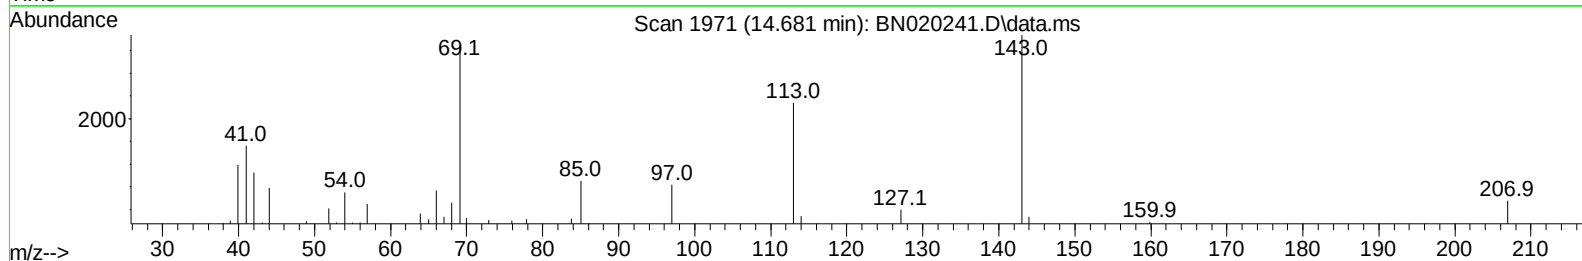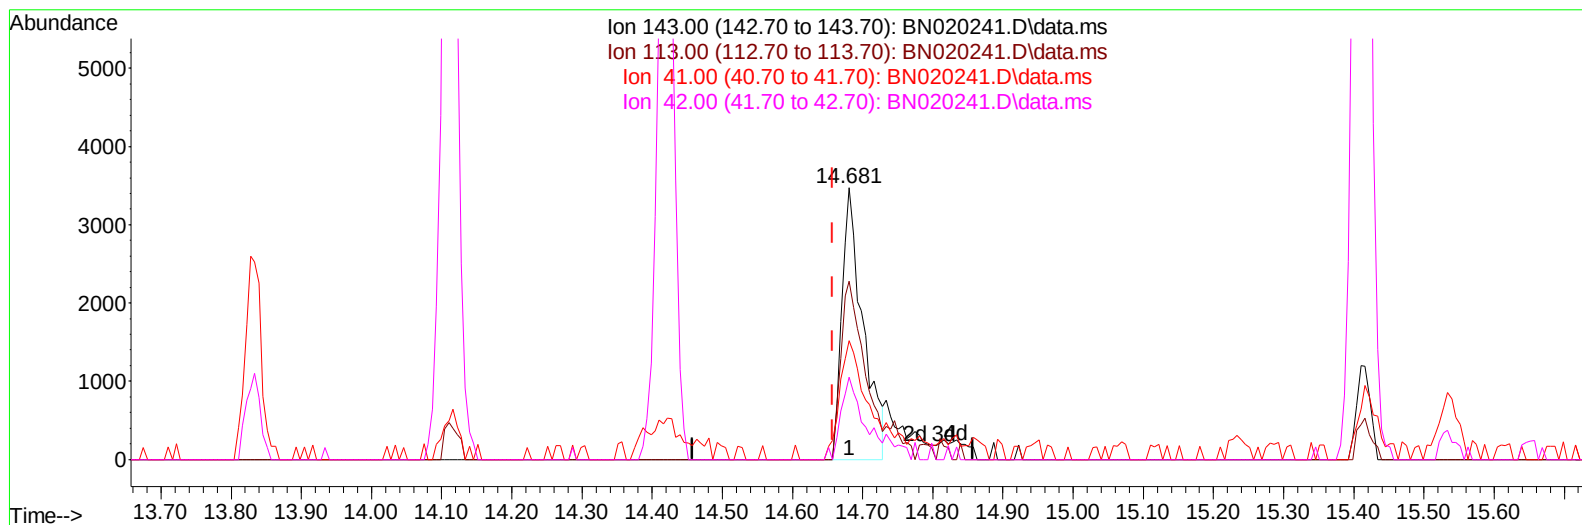

TIC: BN020241.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (+ 0.023) 1.15 ng/ul

response 7204

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	65.76
41.00	39.70	43.83
42.00	27.00	30.32




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020241.D
Acq On : 17 Jun 2022 16:10
Operator : CG/JU
Sample : N3313-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7N3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 17 22:57:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 22:53:31 2022
Response via : Initial Calibration

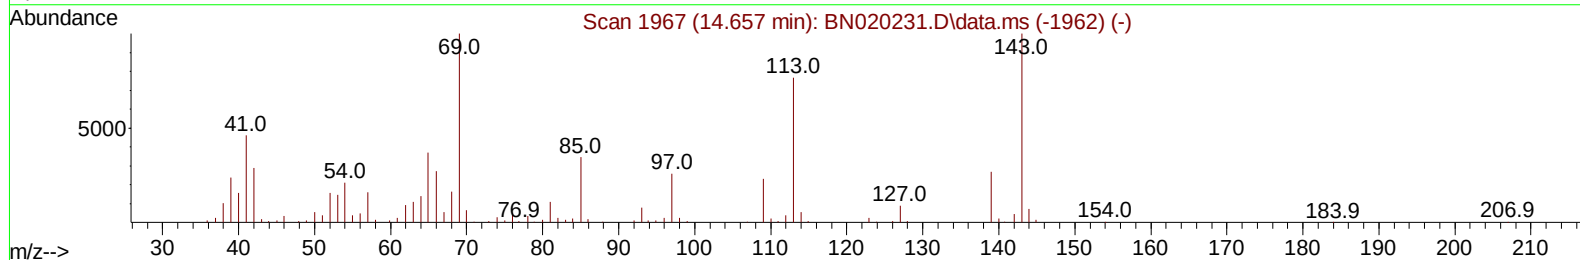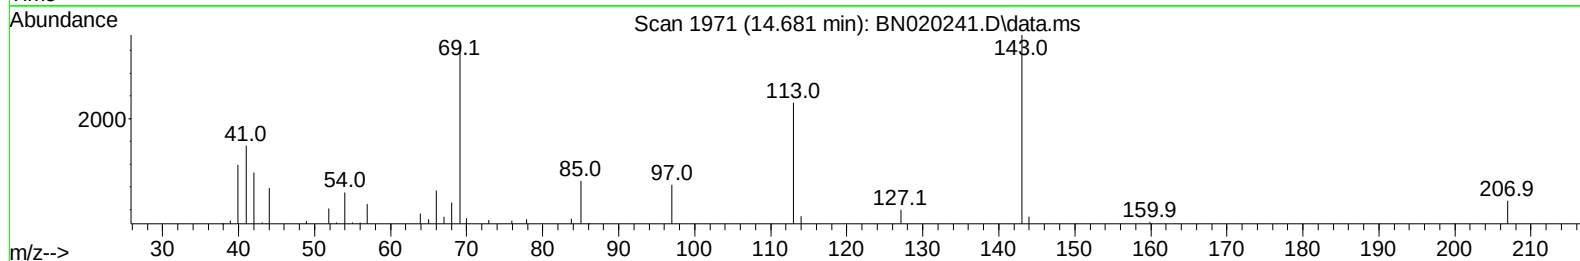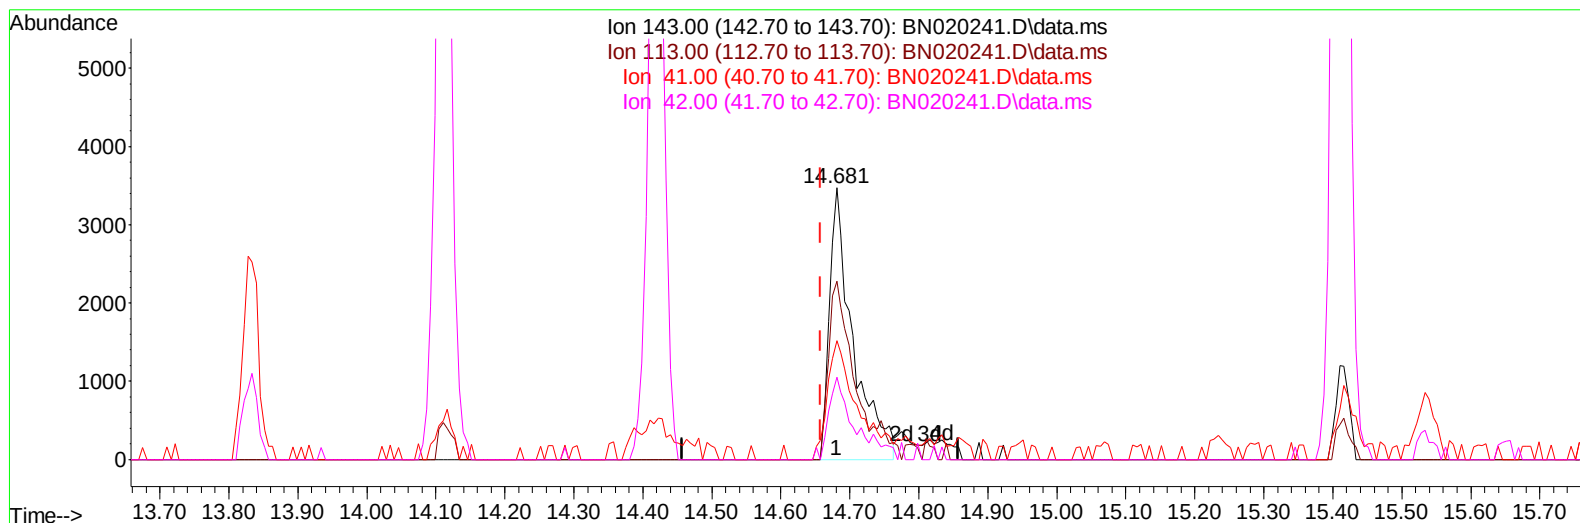

TIC: BN020241.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (+ 0.023) 1.31 ng/ul m

response 8197

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	65.76
41.00	39.70	43.83
42.00	27.00	30.32

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020241.D
 Acq On : 17 Jun 2022 16:10
 Operator : CG/JU
 Sample : N3313-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7N3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 17 22:57:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 22:53:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	119335	20.000	ng/ul	0.00
20) Naphthalene-d8	10.581	136	610212	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.422	164	427919	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	912182	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	821241	20.000	ng/ul	0.00
88) Perylene-d12	23.669	264	695761	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	13643	4.952	ng/uL	0.00
4) Pyridine-d5	3.670	84	75207	9.987	ng/ul	0.00
7) Phenol-d5	6.987	99	71937	7.285	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	214397	34.751	ng/ul	0.00
11) 2-Chlorophenol-d4	7.334	132	223271	27.828	ng/ul	0.00
15) 4-Methylphenol-d8	8.516	113	157634	18.451	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	150962	32.518	ng/ul	0.00
24) 2-Nitrophenol-d4	9.663	143	124622	25.295	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	274149	31.874	ng/ul	0.00
31) 4-Chloroaniline-d4	10.716	131	418717	30.062	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1072558	34.447	ng/ul	0.00
49) Acenaphthylene-d8	14.110	160	1237850	34.282	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	8197m	1.314	ng/ul	0.02
60) Fluorene-d10	15.410	176	925473	35.920	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.540	200	11512	2.179	ng/ul	0.00
73) Anthracene-d10	17.257	188	1476739	37.095	ng/ul	0.00
81) Pyrene-d10	19.557	212	1619604	36.378	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.521	264	1249526	36.705	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020241.D
Acq On : 17 Jun 2022 16:10
Operator : CG/JU
Sample : N3313-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7N3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :mohammad ahmed 06/22/2022

Quant Time: Jun 17 22:57:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 22:53:31 2022
Response via : Initial Calibration

