

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020242.D
 Acq On : 17 Jun 2022 16:46
 Operator : CG/JU
 Sample : N3313-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L1

Quant Time: Jun 17 22:57:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 22:53:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	101628	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	513022	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.422	164	347606	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.163	188	734446	20.000	ng/u1	0.00
79) Chrysene-d12	21.351	240	667493	20.000	ng/u1	# 0.00
88) Perylene-d12	23.663	264	555088	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	16571	7.062	ng/uL	0.00
4) Pyridine-d5	3.664	84	97108	15.142	ng/u1	0.00
7) Phenol-d5	6.987	99	76213	9.063	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	246029	46.826	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	247088	36.162	ng/u1	0.00
15) 4-Methylphenol-d8	8.516	113	152274	20.929	ng/u1	0.00
21) Nitrobenzene-d5	8.940	128	173286	44.399	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	181715	43.870	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	299921	41.477	ng/u1	0.00
31) 4-Chloroaniline-d4	10.716	131	155101	13.245	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	1155461	45.684	ng/u1	0.00
49) Acenaphthylene-d8	14.110	160	1297305	44.229	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	26710	5.270	ng/u1	0.01
60) Fluorene-d10	15.410	176	1006501	48.090	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.534	200	171300	40.265	ng/u1	0.00
73) Anthracene-d10	17.263	188	1460390	45.562	ng/u1	0.00
81) Pyrene-d10	19.557	212	1762081	48.695	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	1252877	46.131	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.287	88	3173	1.281	ng/uL	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020242.D
Acq On : 17 Jun 2022 16:46
Operator : CG/JU
Sample : N3313-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L1


Quant Time: Jun 17 22:57:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 22:53:31 2022
Response via : Initial Calibration

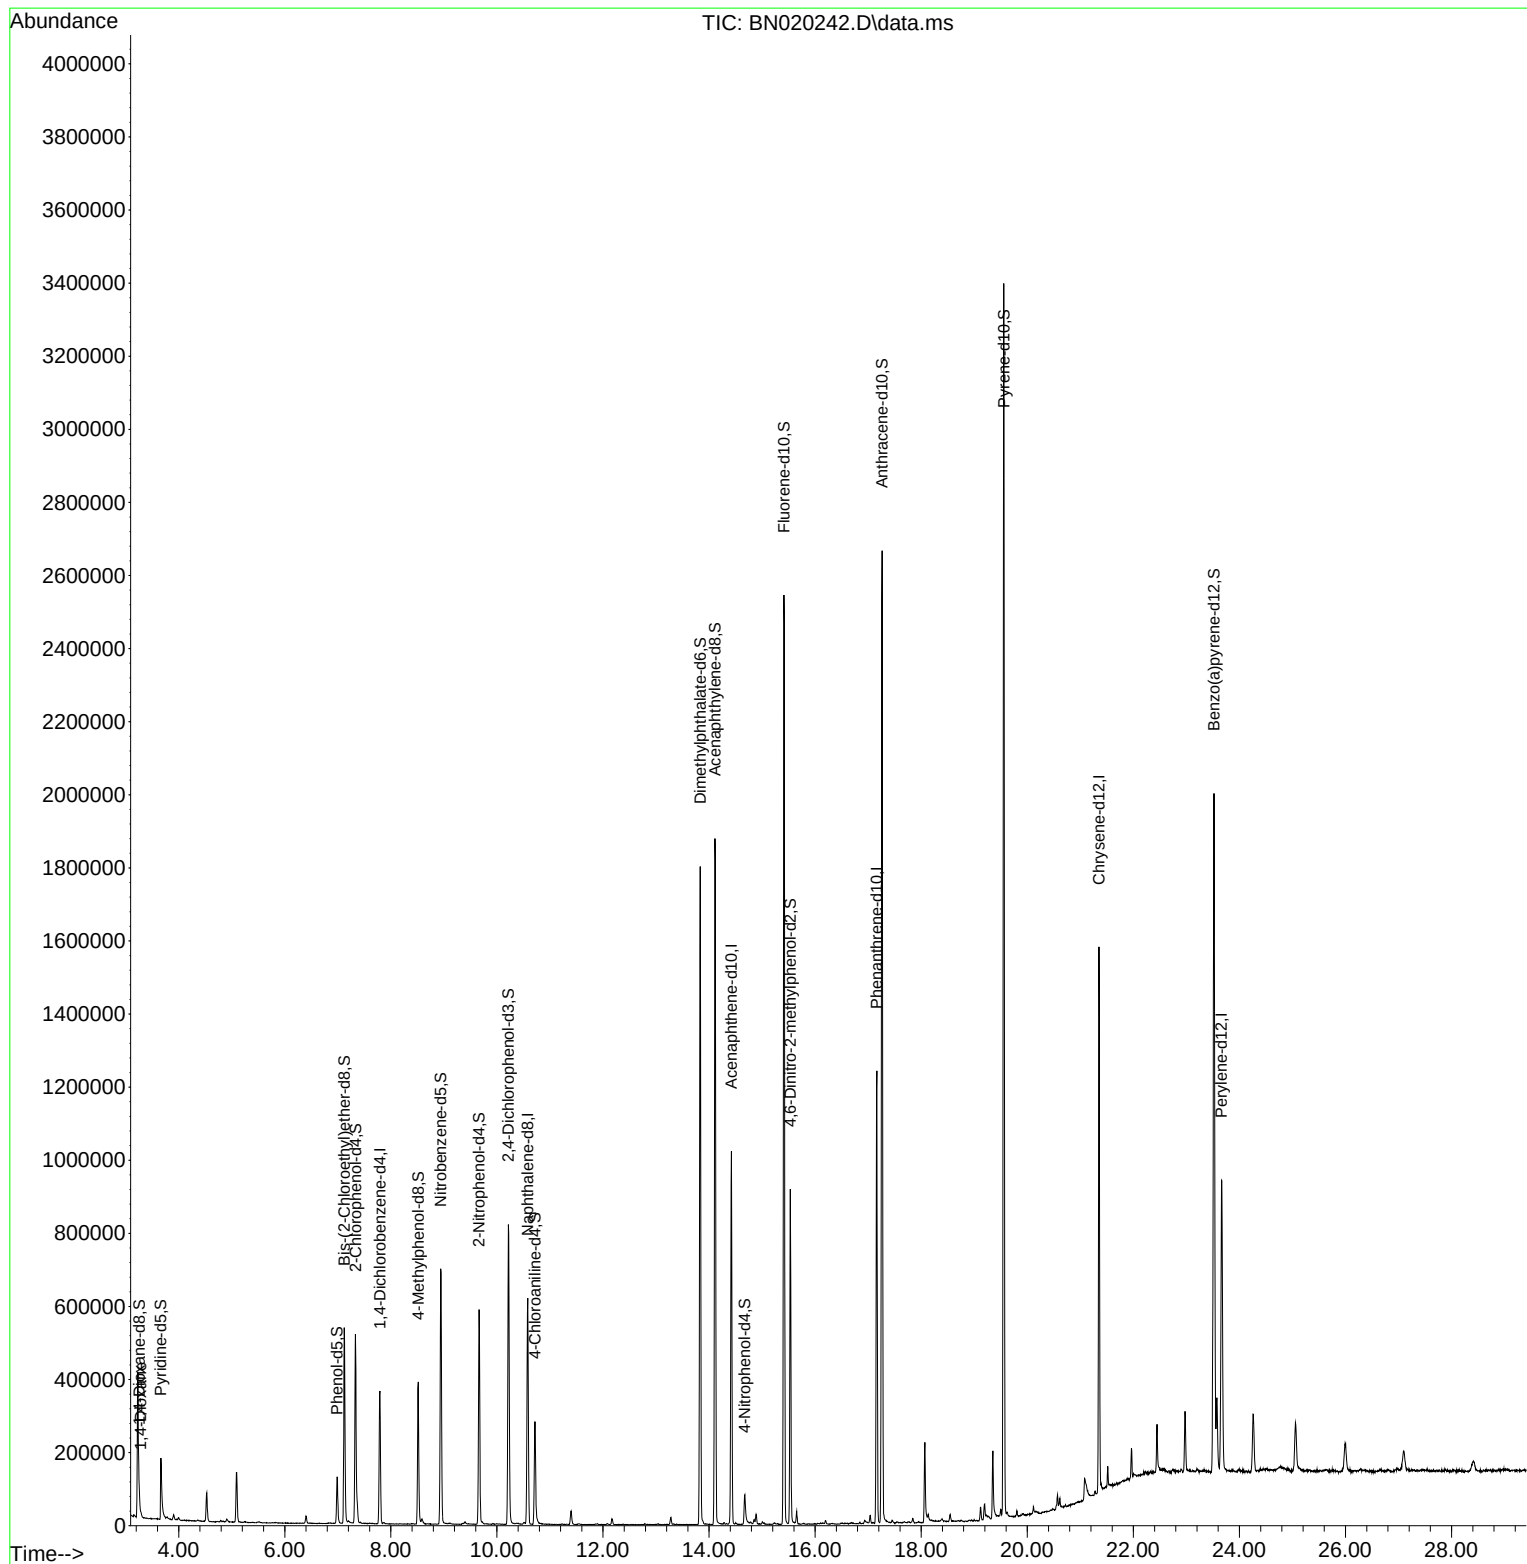

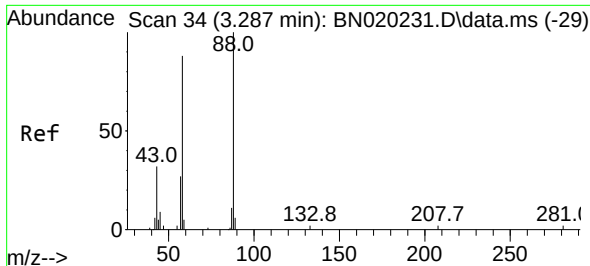

#2
 1,4-Dioxane
 Concen: 1.281 ng/uL
 RT: 3.287 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: BN020242.D
 Acq: 17 Jun 2022 16:46

Instrument :
 BNA_N
 ClientSampleId :
 YB7L1

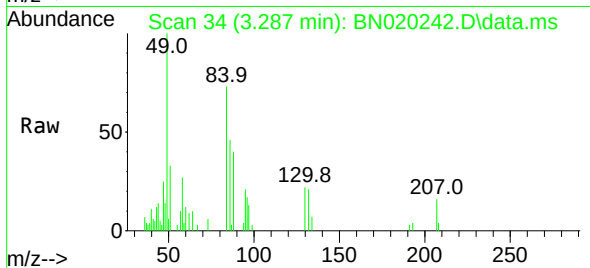

Tgt Ion:	88	Resp:	3173
Ion	Ratio	Lower	Upper
88	100		
43	29.8	22.4	33.6
58	68.0	61.0	91.4

