

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020251.D
 Acq On : 17 Jun 2022 22:53
 Operator : CG/JU
 Sample : N3313-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L5

Quant Time: Jun 18 00:24:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 22:53:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	121436	20.000	ng/u1	0.00
20) Naphthalene-d8	10.575	136	633559	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.422	164	430875	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.163	188	887501	20.000	ng/u1	0.00
79) Chrysene-d12	21.345	240	800850	20.000	ng/u1	0.00
88) Perylene-d12	23.657	264	668348	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	456493	162.816	ng/uL	-0.02
4) Pyridine-d5	3.664	84	93795	12.240	ng/u1	0.00
7) Phenol-d5	6.987	99	79874	7.949	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	248226	39.538	ng/u1	0.00
11) 2-Chlorophenol-d4	7.334	132	249837	30.600	ng/u1	0.00
15) 4-Methylphenol-d8	8.511	113	177526	20.420	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	172498	35.788	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	186334	36.427	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.216	165	317697	35.576	ng/u1	0.00
31) 4-Chloroaniline-d4	10.716	131	421029	29.115	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	1237562	39.474	ng/u1	0.00
49) Acenaphthylene-d8	14.110	160	1428264	39.284	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	30278	4.820	ng/u1	0.01
60) Fluorene-d10	15.410	176	1062162	40.942	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.534	200	191572	37.264	ng/u1	0.00
73) Anthracene-d10	17.257	188	1623611	41.918	ng/u1	0.00
81) Pyrene-d10	19.557	212	1826228	42.064	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.510	264	1403257	42.912	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.287	88	471562	159.320	ng/uL 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020251.D
Acq On : 17 Jun 2022 22:53
Operator : CG/JU
Sample : N3313-07
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L5

Quant Time: Jun 18 00:24:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 22:53:31 2022
Response via : Initial Calibration

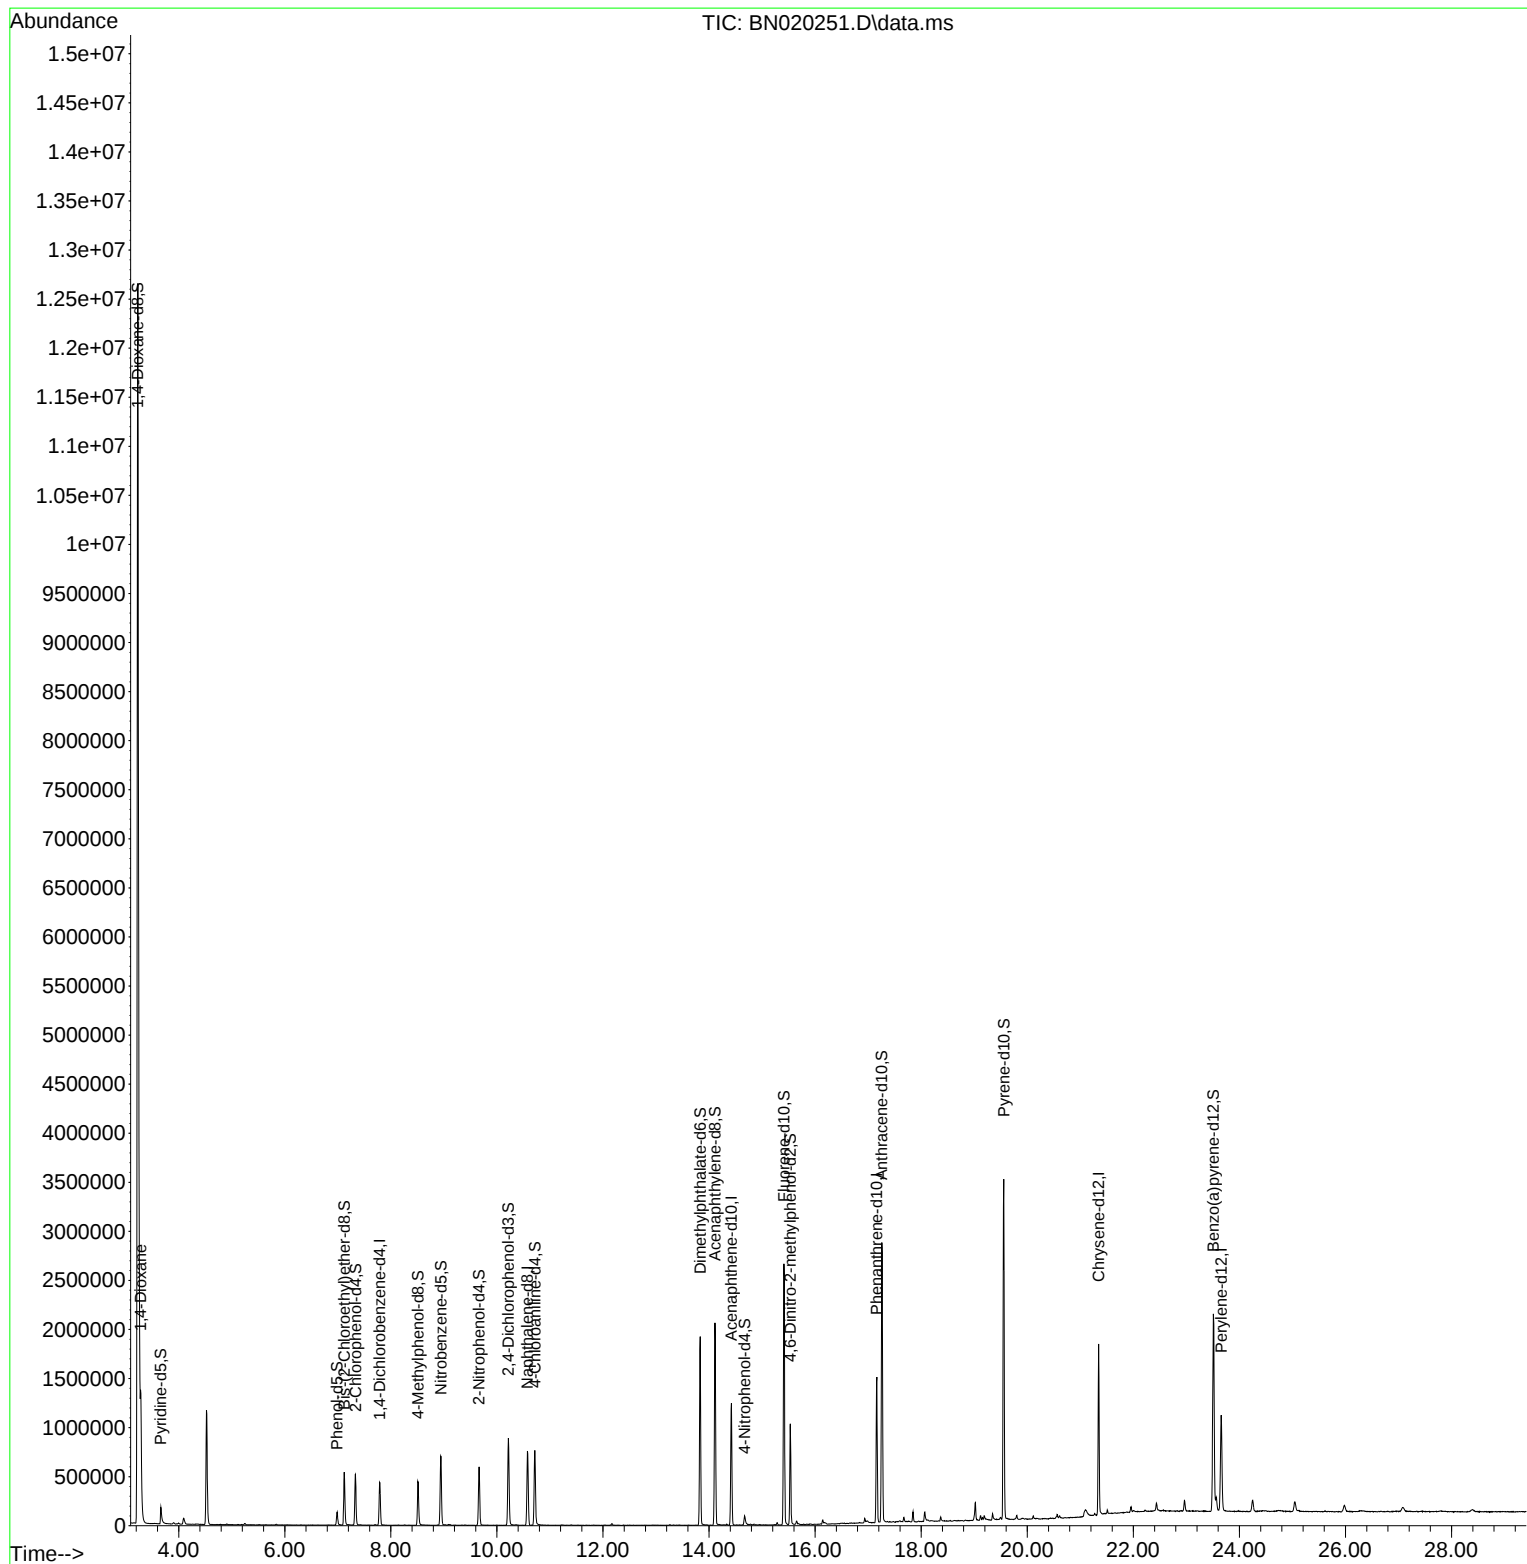

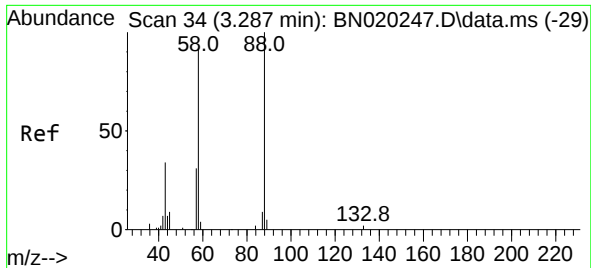

#2
 1,4-Dioxane
 Concen: 159.320 ng/uL
 RT: 3.287 min Scan# 34
 Delta R.T. 0.000 min
 Lab File: BN020251.D
 Acq: 17 Jun 2022 22:53

Instrument :
 BNA_N
 ClientSampleId :
 YB7L5

Tgt Ion: 88 Resp: 471562

Ion	Ratio	Lower	Upper
88	100		
43	31.4	22.4	33.6
58	83.4	61.0	91.4

