

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020232.D
 Acq On : 17 Jun 2022 10:41
 Operator : CG/JU
 Sample : PB145580BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK580

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	41	rVB	37683	64425	1.37%	0.131%
2	3.664	94	98	119	rBV	480752	869160	18.43%	1.766%
3	3.999	151	155	163	rVB3	9255	17235	0.37%	0.035%
4	6.981	656	662	679	rBV	682227	1187884	25.19%	2.413%
5	7.122	679	686	701	rVB	525778	871471	18.48%	1.770%
6	7.334	713	722	736	rBV	699055	1190739	25.25%	2.419%
7	7.793	792	800	807	rBV	500591	841988	17.86%	1.711%
8	8.510	916	922	939	rBV	955594	1642450	34.83%	3.337%
9	8.940	988	995	1010	rBV	690901	1190233	25.24%	2.418%
10	9.663	1110	1118	1133	rBV	614110	1029723	21.84%	2.092%
11	10.216	1205	1212	1232	rBV	937353	1669856	35.41%	3.392%
12	10.581	1266	1274	1285	rBV	845392	1479573	31.38%	3.006%
13	10.716	1288	1297	1318	rBV	987783	1784932	37.85%	3.626%
14	12.175	1538	1545	1552	rBV	13739	24660	0.52%	0.050%
15	13.834	1820	1827	1840	rBV	1835368	2622143	55.61%	5.327%
16	14.110	1867	1874	1887	rBV	2061101	3055408	64.80%	6.207%
17	14.422	1918	1927	1938	rBV	1415428	2190247	46.45%	4.450%
18	14.657	1961	1967	1986	rBV	635184	1246395	26.43%	2.532%
19	14.839	1996	1998	2005	rVB6	3200	5316	0.11%	0.011%
20	15.410	2088	2095	2106	rBV	2630359	3836400	81.36%	7.794%
21	15.534	2109	2116	2126	rVV	947972	1382534	29.32%	2.809%
22	15.651	2131	2136	2144	rVB2	31513	48876	1.04%	0.099%
23	16.192	2223	2228	2234	rVB5	9217	14420	0.31%	0.029%
24	16.945	2351	2356	2362	rBV6	5406	12434	0.26%	0.025%
25	17.163	2386	2393	2402	rBV	1767733	2651038	56.22%	5.386%
26	17.257	2402	2409	2425	rVV	2800542	4251453	90.16%	8.637%
27	19.122	2721	2726	2730	rBV	33880	46919	1.00%	0.095%
28	19.192	2733	2738	2744	rBV2	33271	45239	0.96%	0.092%
29	19.498	2787	2790	2793	rBV2	8006	7423	0.16%	0.015%
30	19.557	2793	2800	2812	rBV	3277731	4715414	100.00%	9.580%
31	20.569	2969	2972	2977	rVB3	23857	28405	0.60%	0.058%
32	21.351	3099	3105	3113	rBV	2019813	2674109	56.71%	5.433%
33	22.974	3377	3381	3388	rVB2	52354	81612	1.73%	0.166%
34	23.515	3465	3473	3480	rBV	1933307	3849196	81.63%	7.820%
35	23.663	3491	3498	3513	rVB2	1107716	2245583	47.62%	4.562%
36	24.257	3595	3599	3606	rVB2	78822	152646	3.24%	0.310%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020232.D
Acq On : 17 Jun 2022 10:41
Operator : CG/JU
Sample : PB145580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	25.051	3730	3734	3745	rVB2	84439	195998	4.16%	0.398%
----	--------	------	------	------	------	-------	--------	-------	--------




Sum of corrected areas: 49223537

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020232.D
Acq On : 17 Jun 2022 10:41
Operator : CG/JU
Sample : PB145580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

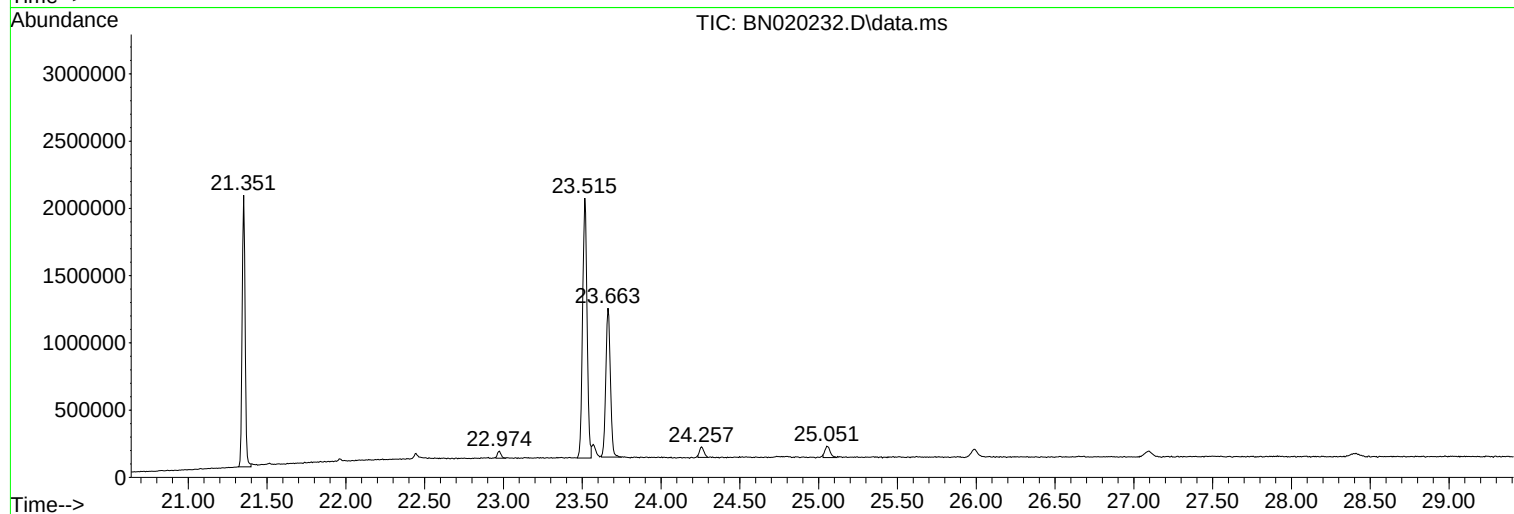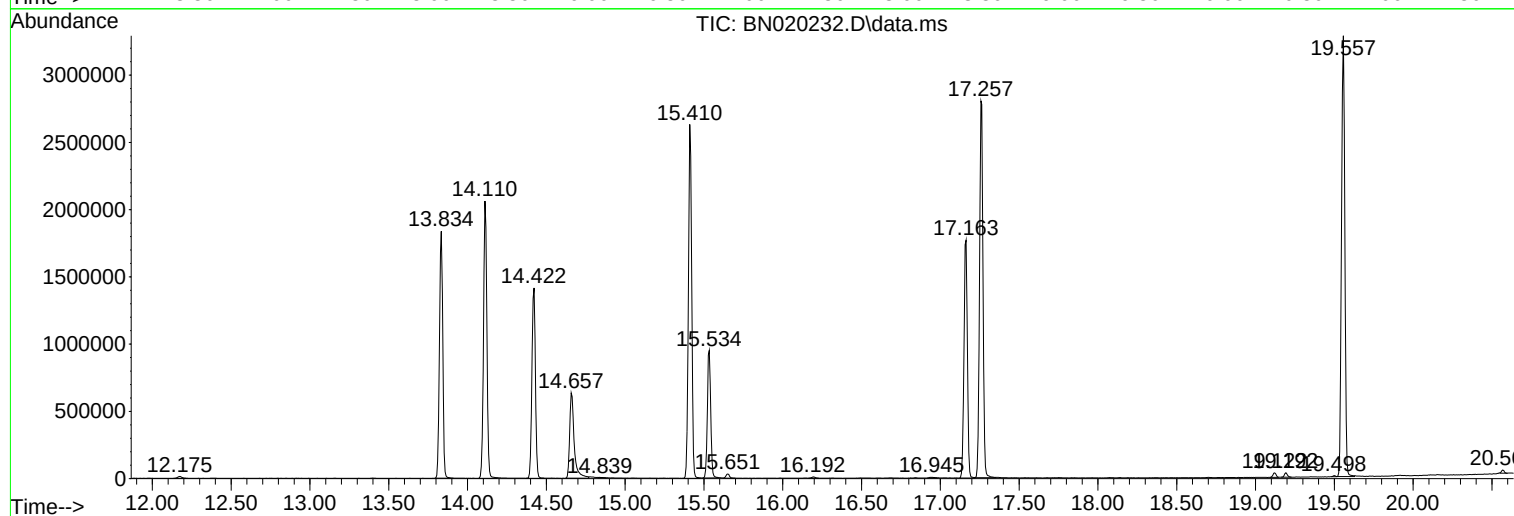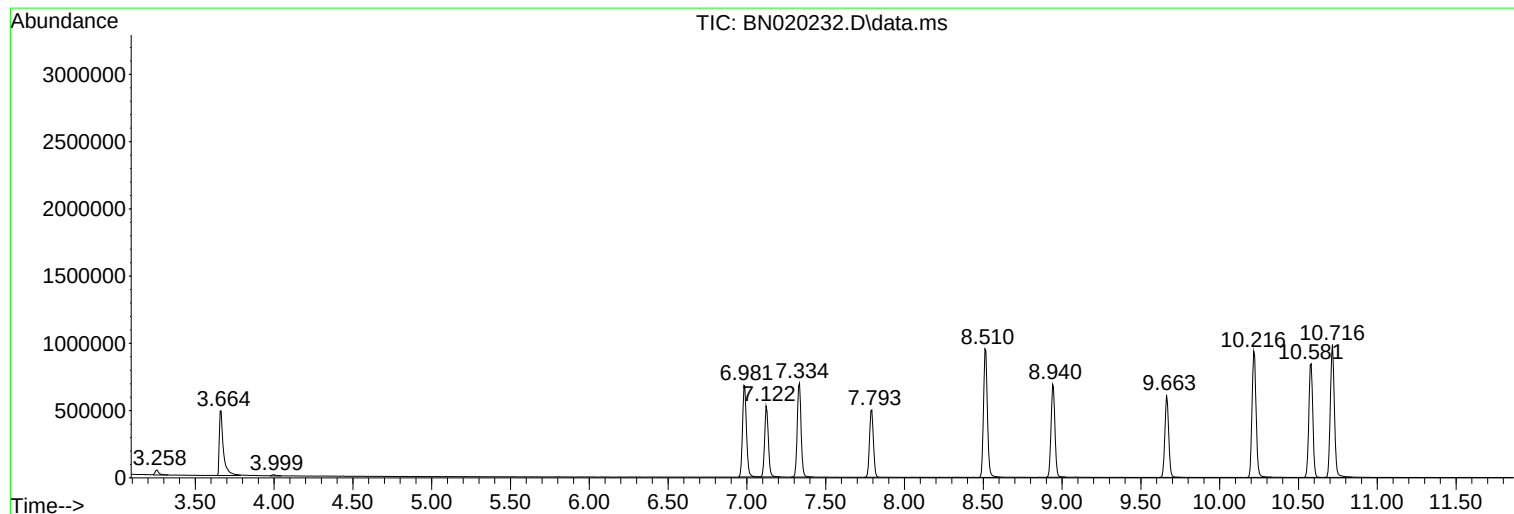

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020232.D
Acq On : 17 Jun 2022 10:41
Operator : CG/JU
Sample : PB145580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020232.D
Acq On : 17 Jun 2022 10:41
Operator : CG/JU
Sample : PB145580BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK580

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc