

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020235.D
 Acq On : 17 Jun 2022 12:30
 Operator : CG/JU
 Sample : N3313-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rVB	26447	41125	0.86%	0.096%
2	3.664	95	98	120	rBV	138341	258712	5.42%	0.604%
3	3.905	134	139	145	rVB2	12146	20806	0.44%	0.049%
4	3.999	152	155	166	rVB2	8641	15164	0.32%	0.035%
5	4.793	285	290	295	rBV6	2927	5189	0.11%	0.012%
6	4.916	306	311	313	rBV4	4242	6676	0.14%	0.016%
7	6.987	654	663	674	rBV	113791	199634	4.18%	0.466%
8	7.122	680	686	703	rBV	462109	772558	16.19%	1.805%
9	7.334	715	722	735	rBV	479847	793770	16.63%	1.855%
10	7.793	793	800	811	rBV	466289	782940	16.40%	1.829%
11	8.516	916	923	939	rBV	399518	681456	14.28%	1.592%
12	8.940	988	995	1009	rBV	606818	1063572	22.28%	2.485%
13	9.399	1069	1073	1077	rBV4	3307	5219	0.11%	0.012%
14	9.663	1108	1118	1129	rBV	513317	917392	19.22%	2.144%
15	10.216	1205	1212	1228	rBV	756536	1357391	28.44%	3.172%
16	10.581	1266	1274	1284	rBV	786764	1352860	28.34%	3.161%
17	10.716	1289	1297	1316	rBV	708150	1335030	27.97%	3.119%
18	11.887	1492	1496	1502	rVB2	3582	6017	0.13%	0.014%
19	12.169	1539	1544	1554	rVB	13986	24121	0.51%	0.056%
20	13.392	1749	1752	1756	rVB2	4849	5585	0.12%	0.013%
21	13.834	1820	1827	1840	rBV	1721857	2414579	50.59%	5.642%
22	14.110	1867	1874	1889	rBV	1815449	2800747	58.68%	6.544%
23	14.422	1915	1927	1936	rBV	1311080	2070004	43.37%	4.837%
24	14.675	1964	1970	1986	rBV	63893	148469	3.11%	0.347%
25	14.845	1995	1999	2005	rVB4	15287	23922	0.50%	0.056%
26	15.228	2057	2064	2070	rBV7	3378	6982	0.15%	0.016%
27	15.410	2088	2095	2105	rBV	2464264	3708413	77.69%	8.665%
28	15.534	2110	2116	2132	rVV	947708	1313535	27.52%	3.069%
29	15.651	2132	2136	2143	rVB2	30116	47857	1.00%	0.112%
30	16.192	2223	2228	2239	rBV2	40282	83275	1.74%	0.195%
31	16.839	2334	2338	2342	rBV4	3906	6067	0.13%	0.014%
32	16.939	2350	2355	2359	rBV7	6100	12702	0.27%	0.030%
33	17.098	2377	2382	2386	rVB6	3972	6732	0.14%	0.016%
34	17.163	2386	2393	2402	rBV	1574609	2403450	50.35%	5.616%
35	17.263	2402	2410	2424	rBV	2873375	4277213	89.61%	9.994%
36	17.398	2429	2433	2440	rVB	12947	21358	0.45%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020235.D
 Acq On : 17 Jun 2022 12:30
 Operator : CG/JU
 Sample : N3313-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7N1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	18.786	2664	2669	2674	rBV2	5670	9368	0.20%	0.022%
38	19.122	2721	2726	2731	rVB	36389	49510	1.04%	0.116%
39	19.192	2733	2738	2744	rVV	33739	46538	0.97%	0.109%
40	19.498	2787	2790	2793	rBV2	12289	13541	0.28%	0.032%
41	19.557	2793	2800	2808	rBV2	3398689	4773197	100.00%	11.153%
42	20.569	2966	2972	2977	rBV	134982	169863	3.56%	0.397%
43	21.274	3089	3092	3099	rBV5	22475	26189	0.55%	0.061%
44	21.351	3099	3105	3122	rBV	1772113	2493258	52.23%	5.826%
45	22.439	3288	3290	3295	rVB	45171	53053	1.11%	0.124%
46	22.974	3377	3381	3388	rVB2	70973	109088	2.29%	0.255%
47	23.515	3465	3473	3480	rBV	1935956	3831345	80.27%	8.952%
48	23.662	3491	3498	3512	rVB2	1010959	2044099	42.82%	4.776%
49	24.257	3595	3599	3607	rVB2	97572	188853	3.96%	0.441%




Sum of corrected areas: 42798424

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020235.D
Acq On : 17 Jun 2022 12:30
Operator : CG/JU
Sample : N3313-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

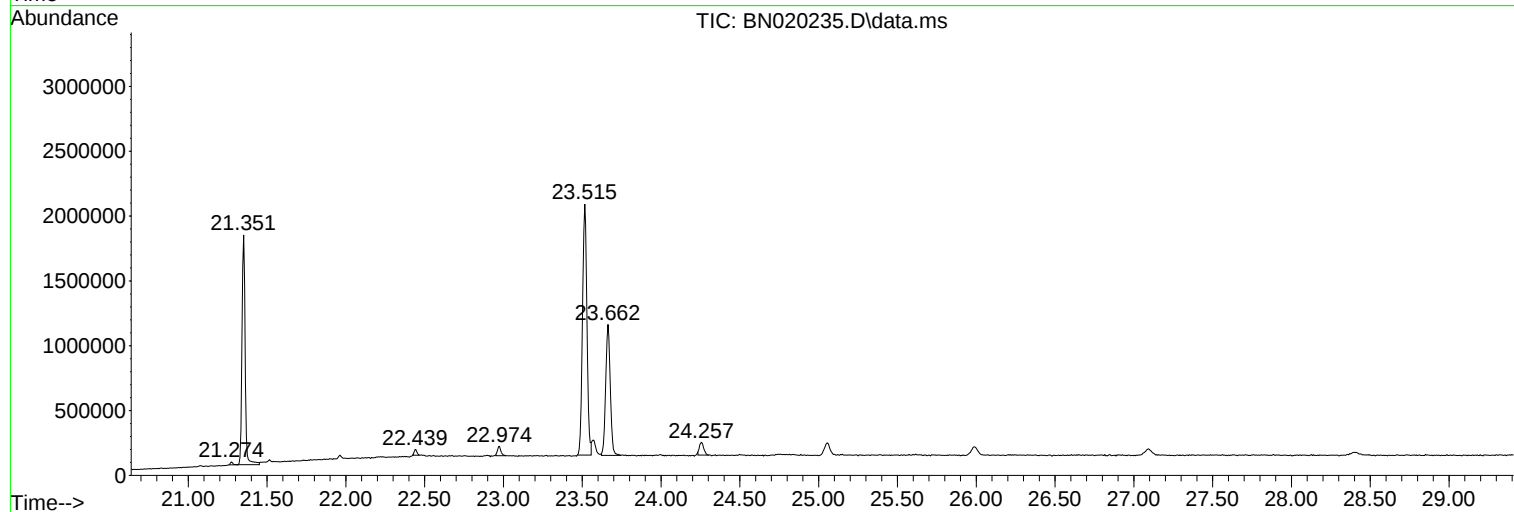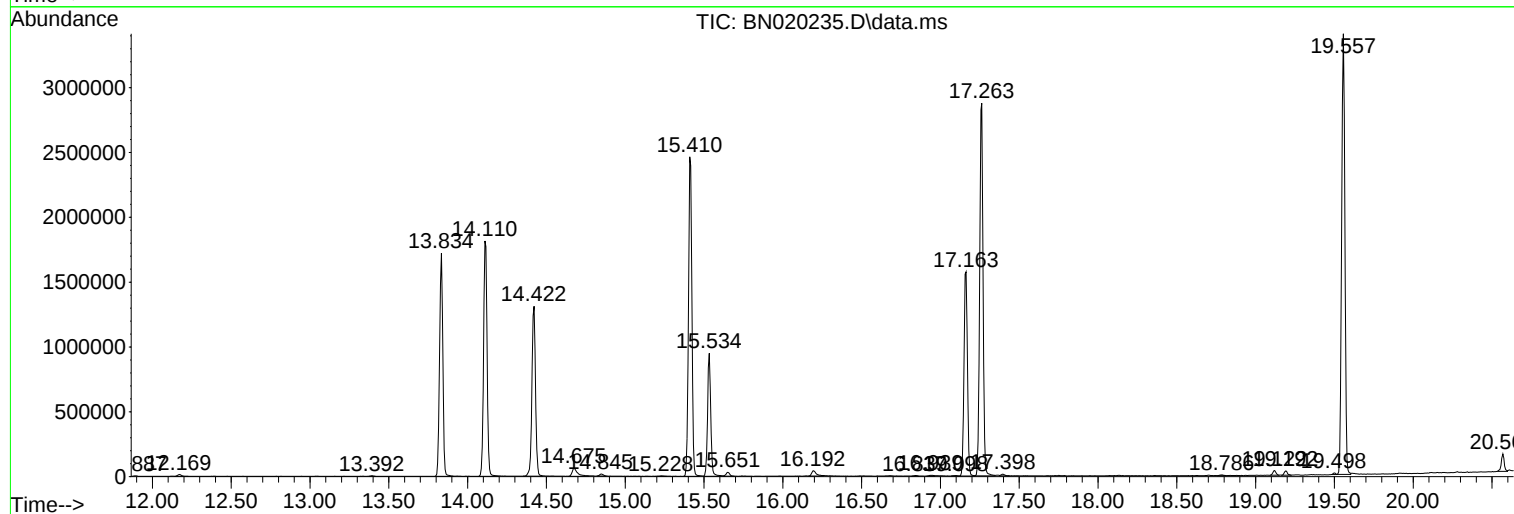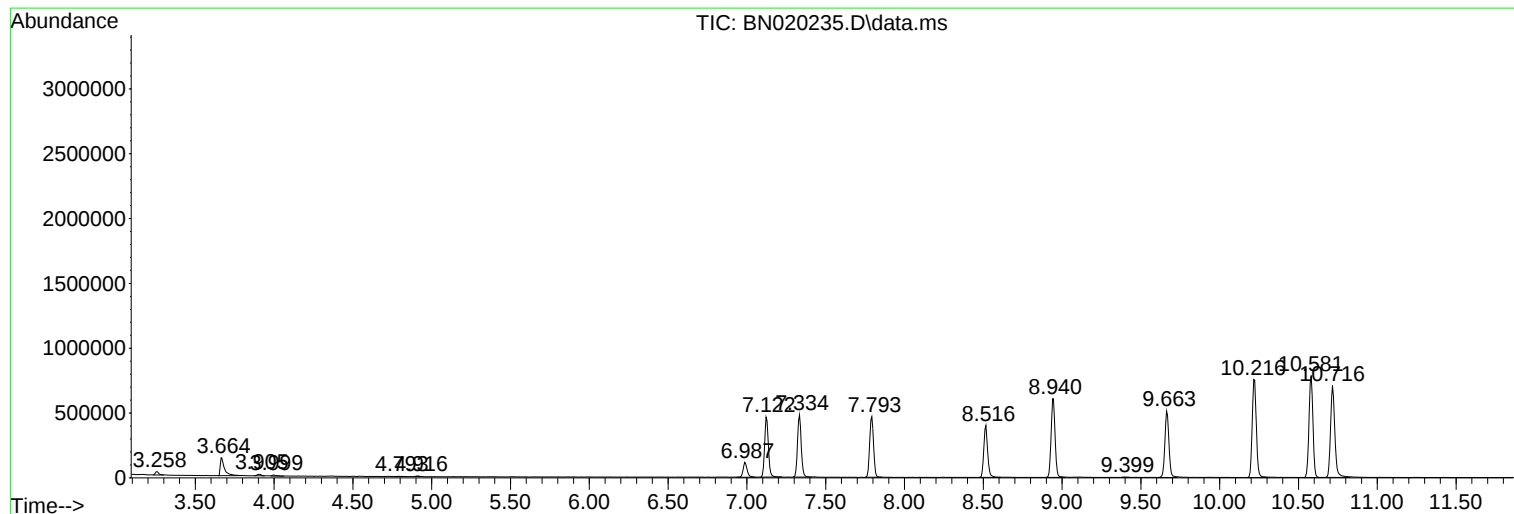

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020235.D
Acq On : 17 Jun 2022 12:30
Operator : CG/JU
Sample : N3313-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020235.D
Acq On : 17 Jun 2022 12:30
Operator : CG/JU
Sample : N3313-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7N1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------