

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020240.D
 Acq On : 17 Jun 2022 15:33
 Operator : CG/JU
 Sample : N3292-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	25	29	39	rVB	15906	26550	1.11%	0.095%
2	3.675	98	100	112	rBV	28957	58366	2.43%	0.209%
3	3.775	113	117	125	rVB3	9241	16797	0.70%	0.060%
4	3.904	134	139	145	rBV2	19808	33603	1.40%	0.120%
5	3.993	152	154	161	rVB	7615	10471	0.44%	0.037%
6	4.369	215	218	223	rVB5	4346	5235	0.22%	0.019%
7	4.546	244	248	257	rVB2	12566	20696	0.86%	0.074%
8	4.904	304	309	320	rBV	32155	57080	2.38%	0.204%
9	5.522	408	414	417	rBV2	4433	7149	0.30%	0.026%
10	6.987	657	663	675	rVB	284485	494468	20.59%	1.768%
11	7.122	680	686	695	rBV	225269	376930	15.70%	1.347%
12	7.204	696	700	707	rVB	5522	11893	0.50%	0.043%
13	7.334	715	722	733	rBV	300030	505276	21.04%	1.806%
14	7.428	734	738	746	rVB4	7775	12599	0.52%	0.045%
15	7.793	793	800	809	rBV	438964	732014	30.48%	2.617%
16	8.516	916	923	934	rVV	358994	615239	25.62%	2.199%
17	8.610	934	939	947	rVB	19645	36275	1.51%	0.130%
18	8.940	988	995	1006	rVV	293097	507054	21.11%	1.813%
19	9.028	1006	1010	1017	rVB2	14450	22794	0.95%	0.081%
20	9.663	1110	1118	1127	rBV	246391	426415	17.76%	1.524%
21	10.028	1173	1180	1186	rVB7	6005	13045	0.54%	0.047%
22	10.222	1205	1213	1226	rBV	381932	682609	28.43%	2.440%
23	10.581	1266	1274	1282	rBV	732520	1277006	53.18%	4.565%
24	10.716	1286	1297	1313	rBV	353430	678640	28.26%	2.426%
25	11.045	1348	1353	1357	rBV4	10209	16867	0.70%	0.060%
26	11.516	1430	1433	1438	rVB6	3122	5569	0.23%	0.020%
27	11.622	1444	1451	1462	rVB6	8861	20232	0.84%	0.072%
28	11.781	1474	1478	1484	rVB4	2763	5663	0.24%	0.020%
29	11.875	1487	1494	1499	rBV10	3013	7239	0.30%	0.026%
30	12.016	1514	1518	1525	rVB	27976	45581	1.90%	0.163%
31	12.169	1537	1544	1549	rBV4	7853	17197	0.72%	0.061%
32	12.239	1552	1556	1561	rVB5	3768	6623	0.28%	0.024%
33	12.704	1630	1635	1642	rVB7	5274	12282	0.51%	0.044%
34	12.951	1674	1677	1678	rVV3	4547	5336	0.22%	0.019%
35	12.975	1678	1681	1686	rVV3	11633	17340	0.72%	0.062%
36	13.028	1686	1690	1696	rVB7	3638	6159	0.26%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020240.D
 Acq On : 17 Jun 2022 15:33
 Operator : CG/JU
 Sample : N3292-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	13.263	1722	1730	1736	rBV	33357	57619	2.40%	0.206%
38	13.351	1742	1745	1750	rVB3	7245	10820	0.45%	0.039%
39	13.751	1810	1813	1816	rVV5	5043	5723	0.24%	0.020%
40	13.833	1820	1827	1835	rVV	810547	1163747	48.46%	4.160%

41	13.922	1838	1842	1845	rVV2	15460	23649	0.98%	0.085%
42	13.957	1847	1848	1854	rVB5	7658	8614	0.36%	0.031%
43	14.045	1859	1863	1867	rVB4	6997	10400	0.43%	0.037%
44	14.110	1867	1874	1885	rBV	860297	1316878	54.84%	4.707%
45	14.333	1907	1912	1918	rBV	39928	54387	2.26%	0.194%

46	14.422	1920	1927	1934	rBV	1204956	1865307	77.68%	6.668%
47	14.669	1963	1969	1984	rBV	154985	334869	13.94%	1.197%
48	14.845	1993	1999	2005	rBV4	35929	58819	2.45%	0.210%
49	14.957	2013	2018	2022	rVB7	8477	14440	0.60%	0.052%
50	15.127	2043	2047	2051	rBV4	6335	8857	0.37%	0.032%

51	15.227	2058	2064	2069	rBV8	4510	8446	0.35%	0.030%
52	15.286	2069	2074	2078	rVB	31088	39405	1.64%	0.141%
53	15.410	2088	2095	2103	rBV	1200184	1775153	73.92%	6.345%
54	15.533	2109	2116	2123	rBV	236141	351577	14.64%	1.257%
55	15.651	2132	2136	2139	rBV	14023	21853	0.91%	0.078%

56	15.686	2139	2142	2151	rVB2	22516	38750	1.61%	0.139%
57	15.780	2153	2158	2162	rBV7	4457	5993	0.25%	0.021%
58	15.839	2165	2168	2174	rBV7	4810	9305	0.39%	0.033%
59	15.904	2174	2179	2185	rVB7	11847	20057	0.84%	0.072%
60	16.145	2216	2220	2222	rBV	37731	50203	2.09%	0.179%

61	16.169	2222	2224	2235	rVB4	44432	70815	2.95%	0.253%
62	16.292	2238	2245	2247	rBV6	3935	8152	0.34%	0.029%
63	16.492	2275	2279	2281	rBV4	5611	8346	0.35%	0.030%
64	16.710	2309	2316	2320	rBV9	12755	26334	1.10%	0.094%
65	16.939	2348	2355	2359	rBV2	33106	52517	2.19%	0.188%

66	16.986	2359	2363	2375	rVB3	27870	54947	2.29%	0.196%
67	17.163	2386	2393	2402	rBV	1503007	2237366	93.17%	7.998%
68	17.257	2403	2409	2421	rVV	1260947	1934462	80.55%	6.915%
69	17.357	2422	2426	2431	rVB3	43068	62158	2.59%	0.222%
70	17.457	2439	2443	2449	rBV7	10325	18331	0.76%	0.066%

71	17.674	2472	2480	2484	rBV	29687	45084	1.88%	0.161%
72	17.845	2502	2509	2514	rBV2	19893	30690	1.28%	0.110%
73	17.886	2514	2516	2520	rVB5	5871	6934	0.29%	0.025%
74	18.063	2542	2546	2554	rVV	58205	97433	4.06%	0.348%
75	18.133	2556	2558	2562	rVB	9438	12010	0.50%	0.043%

76	18.221	2570	2573	2579	rVB7	5812	9522	0.40%	0.034%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020240.D
 Acq On : 17 Jun 2022 15:33
 Operator : CG/JU
 Sample : N3292-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4P4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

77	18.268	2579	2581	2588	rVB8	4988	8521	0.35%	0.030%
78	18.368	2594	2598	2602	rBV	22500	33347	1.39%	0.119%
79	18.763	2662	2665	2670	rBV6	3280	5246	0.22%	0.019%
80	18.833	2674	2677	2678	rBV3	7795	6947	0.29%	0.025%
81	18.957	2694	2698	2703	rBV7	6949	13991	0.58%	0.050%
82	19.004	2703	2706	2710	rVB	24207	29478	1.23%	0.105%
83	19.121	2721	2726	2730	rBV4	23186	36848	1.53%	0.132%
84	19.163	2730	2733	2735	rVV4	10546	14900	0.62%	0.053%
85	19.192	2735	2738	2742	rVV	17525	28859	1.20%	0.103%
86	19.262	2746	2750	2754	rVB6	7346	9121	0.38%	0.033%
87	19.351	2761	2765	2774	rBV5	26663	42677	1.78%	0.153%
88	19.504	2788	2791	2794	rVB3	12583	13088	0.55%	0.047%
89	19.557	2794	2800	2808	rBV	1580652	2232710	92.97%	7.981%
90	20.121	2892	2896	2899	rBV	28366	32963	1.37%	0.118%
91	20.574	2970	2973	2976	rVB	33273	35133	1.46%	0.126%
92	20.615	2977	2980	2983	rVB	27634	30839	1.28%	0.110%
93	21.080	3056	3059	3070	rBV4	66000	185555	7.73%	0.663%
94	21.357	3100	3106	3119	rBV	1773290	2401425	100.00%	8.584%
95	21.521	3131	3134	3137	rVB	31932	34503	1.44%	0.123%
96	21.968	3207	3210	3214	rBV2	37887	45521	1.90%	0.163%
97	22.980	3379	3382	3388	rVB	68600	95074	3.96%	0.340%
98	23.521	3467	3474	3481	rBV2	825506	1731377	72.10%	6.189%
99	23.668	3492	3499	3513	rVB2	969019	2029355	84.51%	7.254%
100	24.262	3596	3600	3607	rVB2	78389	153604	6.40%	0.549%




Sum of corrected areas: 27975346

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020240.D
Acq On : 17 Jun 2022 15:33
Operator : CG/JU
Sample : N3292-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

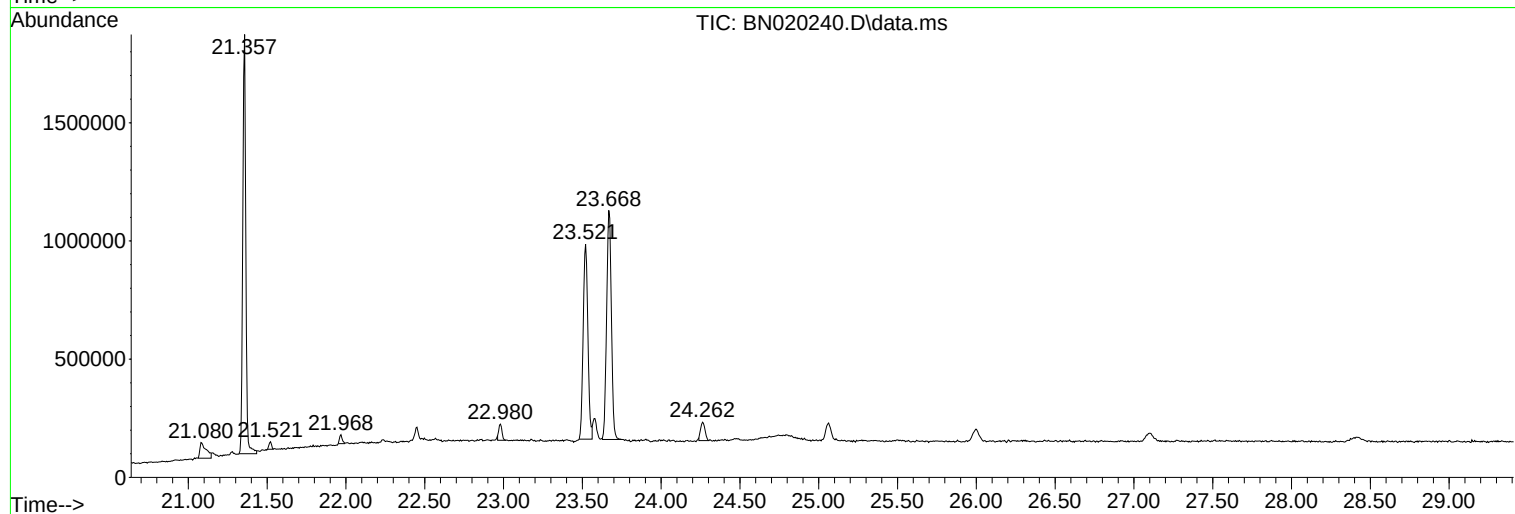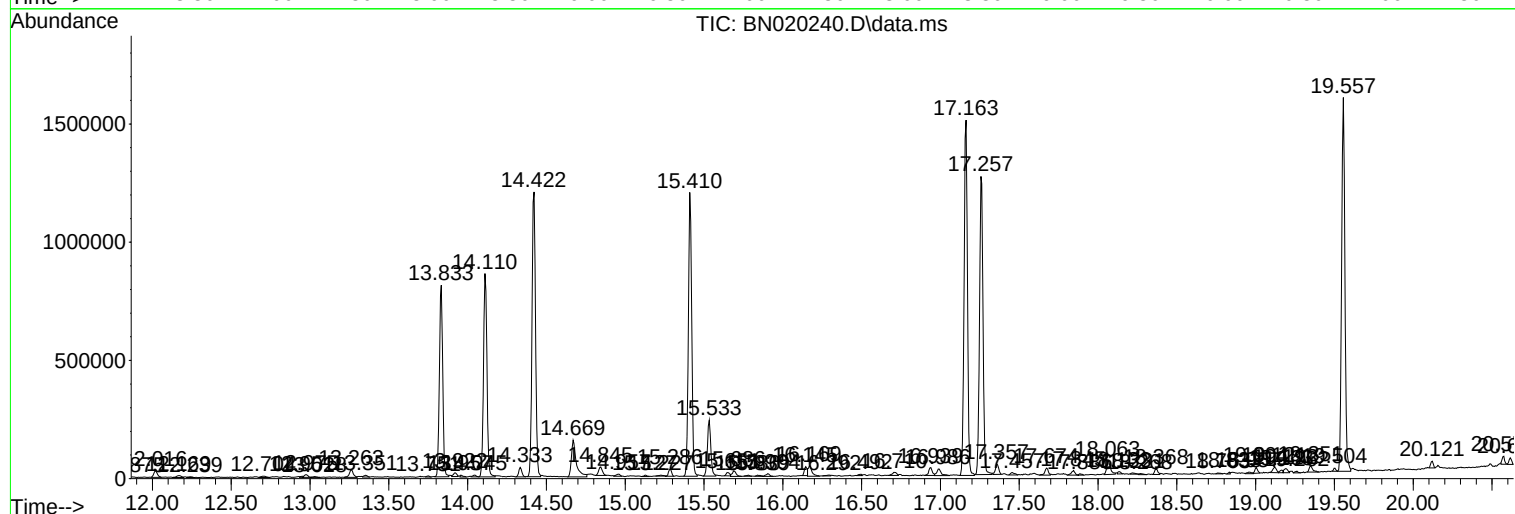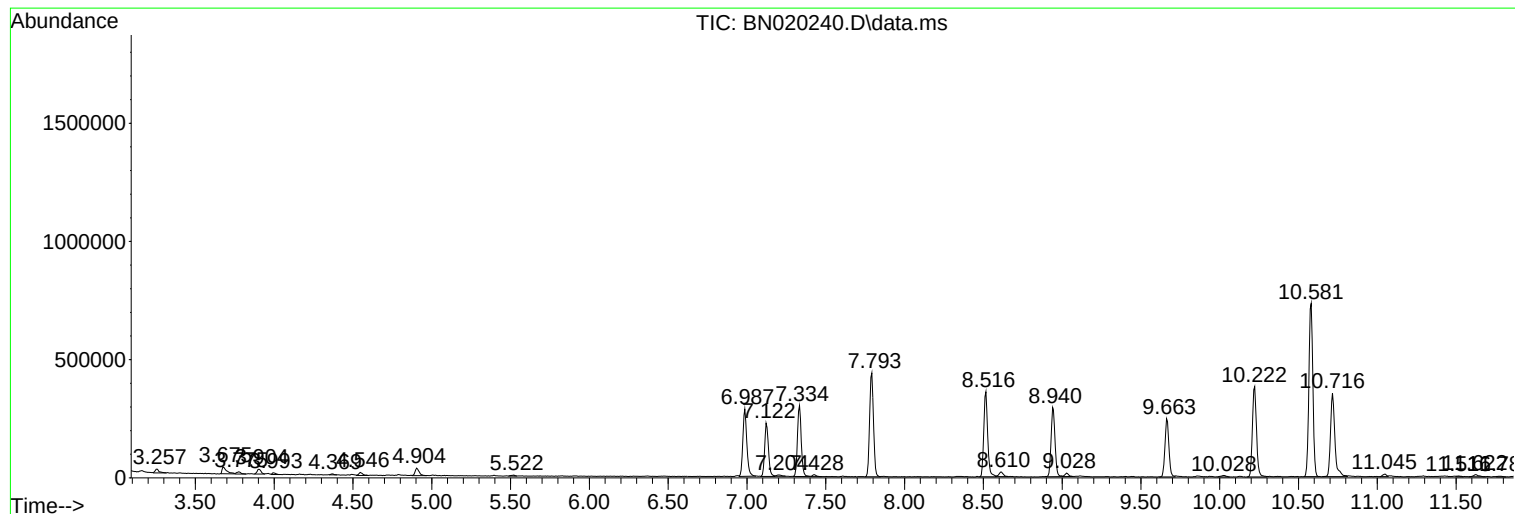

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020240.D
Acq On : 17 Jun 2022 15:33
Operator : CG/JU
Sample : N3292-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020240.D
Acq On : 17 Jun 2022 15:33
Operator : CG/JU
Sample : N3292-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4P4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------