

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020244.D
 Acq On : 17 Jun 2022 18:00
 Operator : CG/JU
 Sample : N3313-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	19	24	45	rVB	445532	797804	18.06%	1.904%
2	3.546	75	78	82	rBV3	5043	8127	0.18%	0.019%
3	3.670	95	99	117	rBV	85542	164393	3.72%	0.392%
4	3.905	135	139	146	rVB2	11457	21111	0.48%	0.050%
5	3.999	152	155	162	rVB2	7329	11812	0.27%	0.028%
6	4.522	239	244	253	rVB	108849	184872	4.19%	0.441%
7	4.905	305	309	318	rBV4	7080	13660	0.31%	0.033%
8	5.840	463	468	472	rBV5	2758	6240	0.14%	0.015%
9	6.987	657	663	676	rBV	118329	208591	4.72%	0.498%
10	7.122	680	686	696	rVV	478237	787736	17.84%	1.880%
11	7.199	696	699	707	rVB	6004	12512	0.28%	0.030%
12	7.334	715	722	734	rBV	482808	804235	18.21%	1.920%
13	7.793	793	800	807	rBV	399915	654259	14.81%	1.562%
14	7.869	809	813	821	rVB6	5243	10260	0.23%	0.024%
15	8.516	916	923	936	rBV	394401	687958	15.58%	1.642%
16	8.940	987	995	1009	rBV	635138	1094631	24.79%	2.613%
17	9.087	1015	1020	1024	rBV5	7818	13904	0.31%	0.033%
18	9.399	1069	1073	1077	rVB2	5293	7436	0.17%	0.018%
19	9.663	1111	1118	1130	rBV	534045	897992	20.33%	2.143%
20	10.216	1205	1212	1228	rBV	773862	1358792	30.77%	3.243%
21	10.581	1266	1274	1285	rBV	657344	1152276	26.09%	2.750%
22	10.716	1288	1297	1312	rBV	656539	1192626	27.00%	2.847%
23	11.240	1380	1386	1387	rBV5	2695	4629	0.10%	0.011%
24	12.169	1539	1544	1553	rVB2	14082	25195	0.57%	0.060%
25	12.793	1642	1650	1654	rBV6	2701	6290	0.14%	0.015%
26	13.263	1726	1730	1736	rVB3	5602	8469	0.19%	0.020%
27	13.834	1820	1827	1842	rBV	1652251	2358761	53.41%	5.630%
28	14.110	1867	1874	1889	rBV	1786319	2780256	62.95%	6.636%
29	14.422	1920	1927	1940	rBV	1107275	1698228	38.45%	4.054%
30	14.675	1960	1970	1978	rBV	74330	149310	3.38%	0.356%
31	14.851	1995	2000	2005	rVB7	8381	13872	0.31%	0.033%
32	15.234	2060	2065	2070	rBV3	6364	10525	0.24%	0.025%
33	15.287	2070	2074	2077	rVB4	3223	4967	0.11%	0.012%
34	15.410	2089	2095	2110	rBV	2393037	3556871	80.54%	8.490%
35	15.534	2110	2116	2127	rVV	859215	1220769	27.64%	2.914%
36	15.651	2130	2136	2147	rVB2	30061	50127	1.14%	0.120%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020244.D
 Acq On : 17 Jun 2022 18:00
 Operator : CG/JU
 Sample : N3313-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	15.922	2178	2182	2187	rVB5	2976	5164	0.12%	0.012%
38	16.145	2216	2220	2225	rBV3	3699	6738	0.15%	0.016%
39	16.198	2225	2229	2233	rVB3	9098	13304	0.30%	0.032%
40	16.845	2334	2339	2343	rVB4	4145	4940	0.11%	0.012%
41	16.939	2351	2355	2356	rBV3	7219	9046	0.20%	0.022%
42	16.969	2356	2360	2367	rVB	13639	23778	0.54%	0.057%
43	17.098	2377	2382	2386	rVB5	3142	5268	0.12%	0.013%
44	17.163	2386	2393	2402	rBV	1392650	2041394	46.22%	4.873%
45	17.263	2403	2410	2423	rBV	2584959	3905251	88.43%	9.322%
46	17.681	2475	2481	2482	rBV6	3123	4738	0.11%	0.011%
47	17.781	2496	2498	2503	rVB4	3395	5129	0.12%	0.012%
48	17.845	2503	2509	2519	rBV	97141	128553	2.91%	0.307%
49	18.069	2542	2547	2555	rBV	163865	244939	5.55%	0.585%
50	18.134	2555	2558	2563	rVB	10639	18567	0.42%	0.044%
51	19.022	2704	2709	2713	rVB	60470	69233	1.57%	0.165%
52	19.122	2721	2726	2730	rBV	37977	50575	1.15%	0.121%
53	19.192	2733	2738	2742	rBV	34553	53849	1.22%	0.129%
54	19.345	2760	2764	2776	rBV	74060	119604	2.71%	0.285%
55	19.498	2786	2790	2793	rBV5	19515	24118	0.55%	0.058%
56	19.557	2793	2800	2808	rVV	3110417	4416374	100.00%	10.542%
57	19.804	2838	2842	2845	rVB2	22777	25579	0.58%	0.061%
58	20.116	2892	2895	2898	rBV4	9210	10500	0.24%	0.025%
59	20.569	2966	2972	2977	rBV3	41327	65177	1.48%	0.156%
60	21.080	3054	3059	3074	rBV3	157913	539097	12.21%	1.287%
61	21.275	3088	3092	3099	rBV	373560	422324	9.56%	1.008%
62	21.351	3099	3105	3115	rBV	1589437	2130560	48.24%	5.086%
63	22.969	3377	3380	3387	rVB2	60259	96097	2.18%	0.229%
64	23.516	3465	3473	3480	rBV	1800537	3552803	80.45%	8.480%
65	23.663	3491	3498	3512	rVB2	874967	1754321	39.72%	4.188%
66	24.257	3595	3599	3606	rVB3	83176	167391	3.79%	0.400%




Sum of corrected areas: 41893907

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020244.D
Acq On : 17 Jun 2022 18:00
Operator : CG/JU
Sample : N3313-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

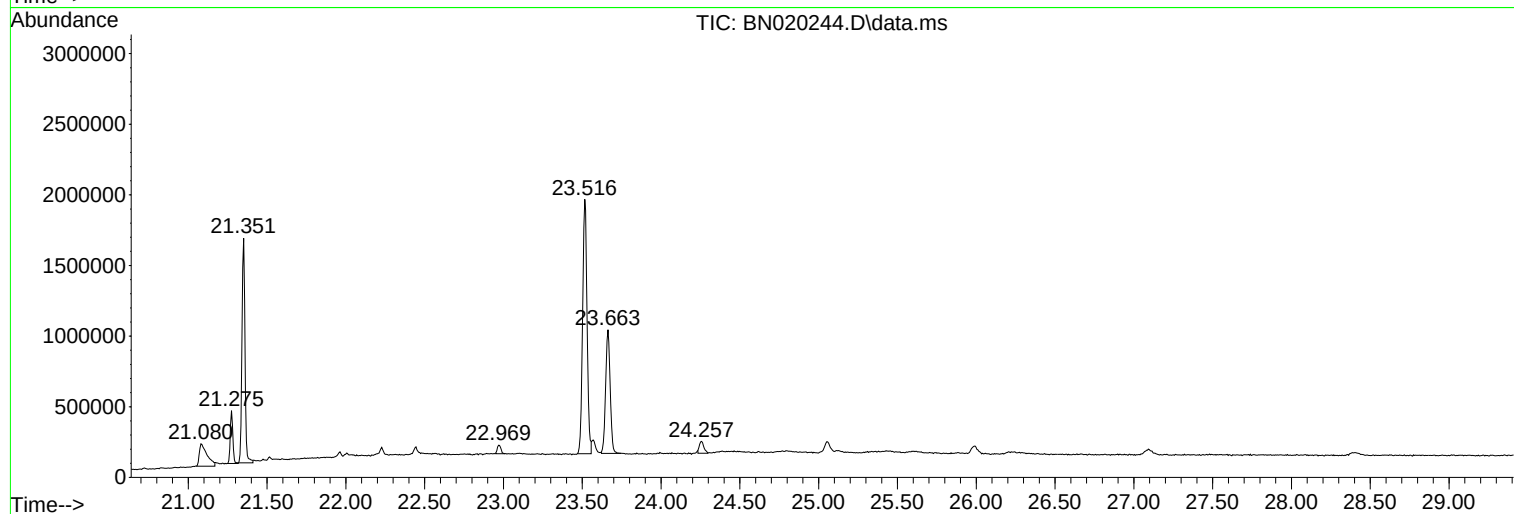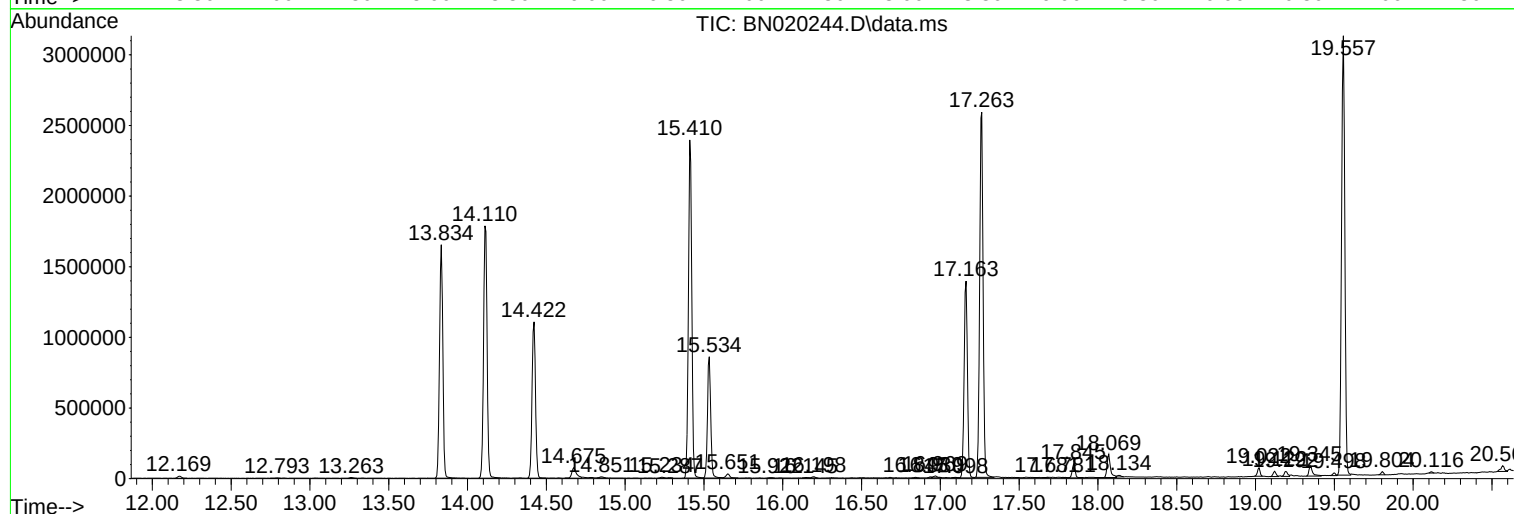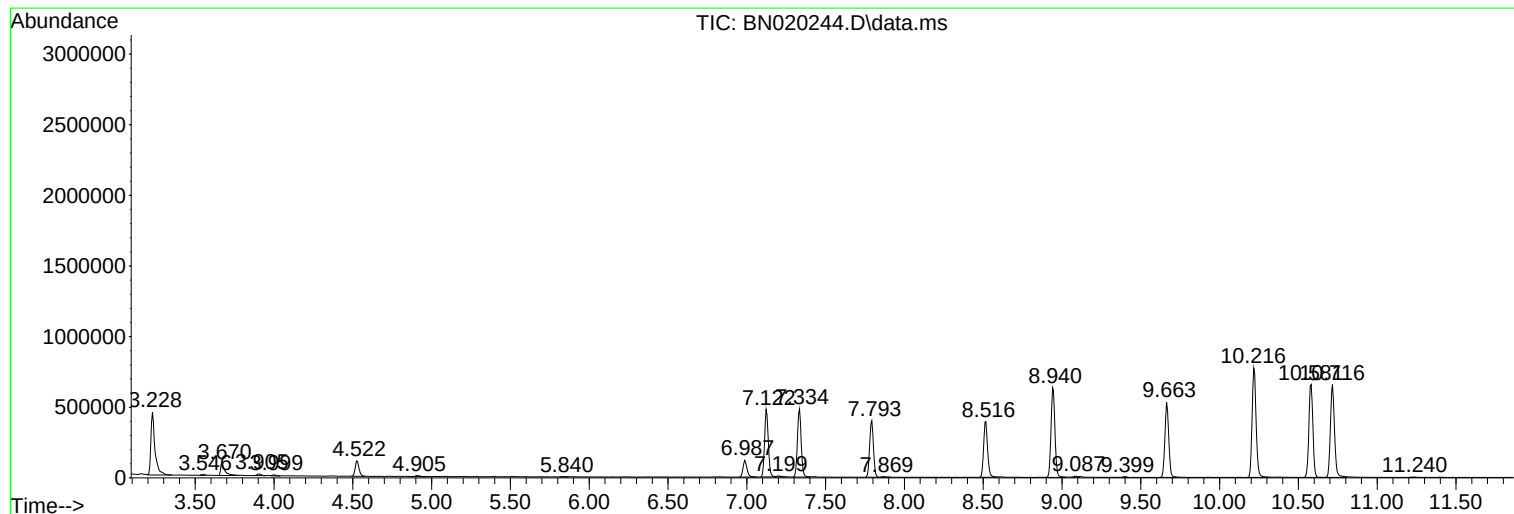

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020244.D
Acq On : 17 Jun 2022 18:00
Operator : CG/JU
Sample : N3313-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020244.D
Acq On : 17 Jun 2022 18:00
Operator : CG/JU
Sample : N3313-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc