

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
 Data File : BN020248.D
 Acq On : 17 Jun 2022 21:03
 Operator : CG/JU
 Sample : PB145571BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	35	rBV	35495	50222	1.12%	0.104%
2	3.658	93	97	115	rBV	492928	847284	18.87%	1.761%
3	3.993	152	154	162	rVB2	9590	14194	0.32%	0.029%
4	6.981	656	662	677	rBV	684298	1146149	25.52%	2.382%
5	7.122	680	686	702	rVB	510975	844244	18.80%	1.754%
6	7.334	714	722	734	rBV	665381	1147395	25.55%	2.384%
7	7.793	792	800	810	rBV	510749	864743	19.25%	1.797%
8	8.511	915	922	936	rBV	911248	1573870	35.04%	3.271%
9	8.940	986	995	1011	rBV	670872	1165189	25.94%	2.421%
10	9.663	1110	1118	1129	rBV	598714	1012527	22.54%	2.104%
11	10.216	1205	1212	1225	rBV	922791	1602323	35.68%	3.330%
12	10.581	1265	1274	1282	rBV	880131	1532125	34.11%	3.184%
13	10.716	1289	1297	1319	rBV	937726	1731486	38.55%	3.598%
14	12.169	1538	1544	1552	rBV	13370	25796	0.57%	0.054%
15	13.834	1820	1827	1841	rBV	1747673	2489803	55.44%	5.174%
16	14.110	1867	1874	1893	rBV	1888977	2915174	64.91%	6.058%
17	14.422	1920	1927	1937	rBV	1491777	2251404	50.13%	4.679%
18	14.657	1960	1967	1996	rBV	644871	1238504	27.58%	2.574%
19	14.846	1996	1999	2006	rVB6	3715	7016	0.16%	0.015%
20	15.410	2088	2095	2105	rBV	2424027	3656577	81.42%	7.599%
21	15.534	2109	2116	2131	rVV	960942	1361891	30.32%	2.830%
22	15.651	2131	2136	2143	rVB2	28753	45440	1.01%	0.094%
23	16.198	2223	2229	2234	rBV4	7574	11788	0.26%	0.024%
24	16.845	2334	2339	2342	rVB4	3695	5243	0.12%	0.011%
25	16.951	2350	2357	2360	rBV4	5445	11194	0.25%	0.023%
26	17.163	2386	2393	2402	rBV	1822905	2693617	59.98%	5.598%
27	17.263	2403	2410	2425	rVV2	2640892	4016432	89.43%	8.347%
28	18.075	2543	2548	2550	rBV5	5154	6563	0.15%	0.014%
29	19.122	2721	2726	2732	rVB	32795	44697	1.00%	0.093%
30	19.192	2732	2738	2743	rBV	32681	45571	1.01%	0.095%
31	19.498	2786	2790	2793	rBV3	11013	13508	0.30%	0.028%
32	19.557	2793	2800	2808	rBV	3245382	4491138	100.00%	9.333%
33	19.922	2854	2862	2867	rBV9	7149	20415	0.45%	0.042%
34	20.563	2965	2971	2977	rBV4	31998	53105	1.18%	0.110%
35	21.345	3099	3104	3116	rBV2	1979656	2723362	60.64%	5.659%
36	22.439	3286	3290	3297	rBV3	43932	70100	1.56%	0.146%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020248.D
Acq On : 17 Jun 2022 21:03
Operator : CG/JU
Sample : PB145571BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK571

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	22.969	3376	3380	3387	rVB2	67274	101060	2.25%	0.210%
38	23.510	3464	3472	3479	rBV	1799467	3617795	80.55%	7.518%
39	23.657	3490	3497	3508	rVB2	1093896	2252050	50.14%	4.680%
40	24.251	3593	3598	3607	rVB	93969	198713	4.42%	0.413%
41	25.045	3728	3733	3743	rVB	93899	221402	4.93%	0.460%




Sum of corrected areas: 48121109

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020248.D
Acq On : 17 Jun 2022 21:03
Operator : CG/JU
Sample : PB145571BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

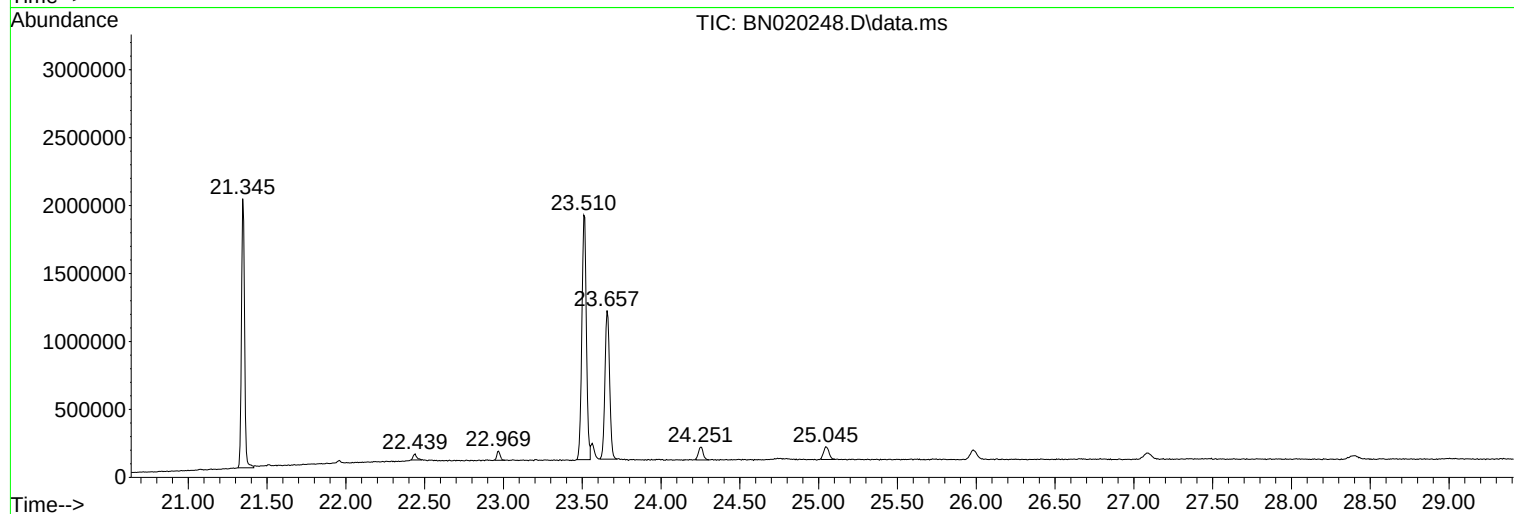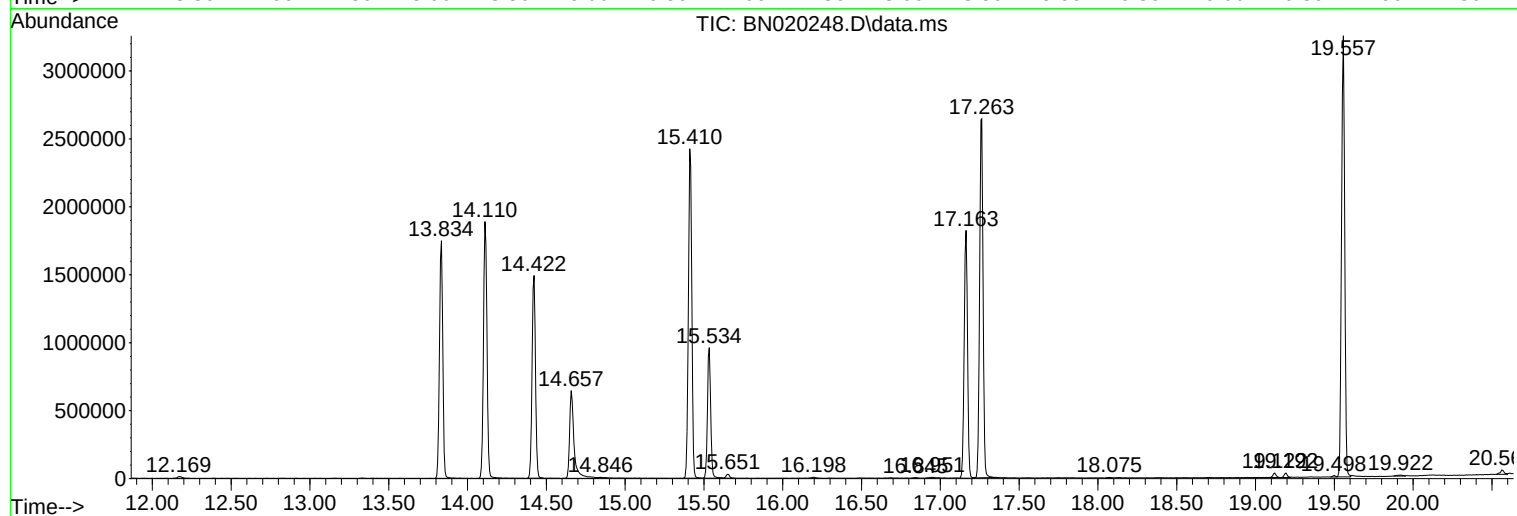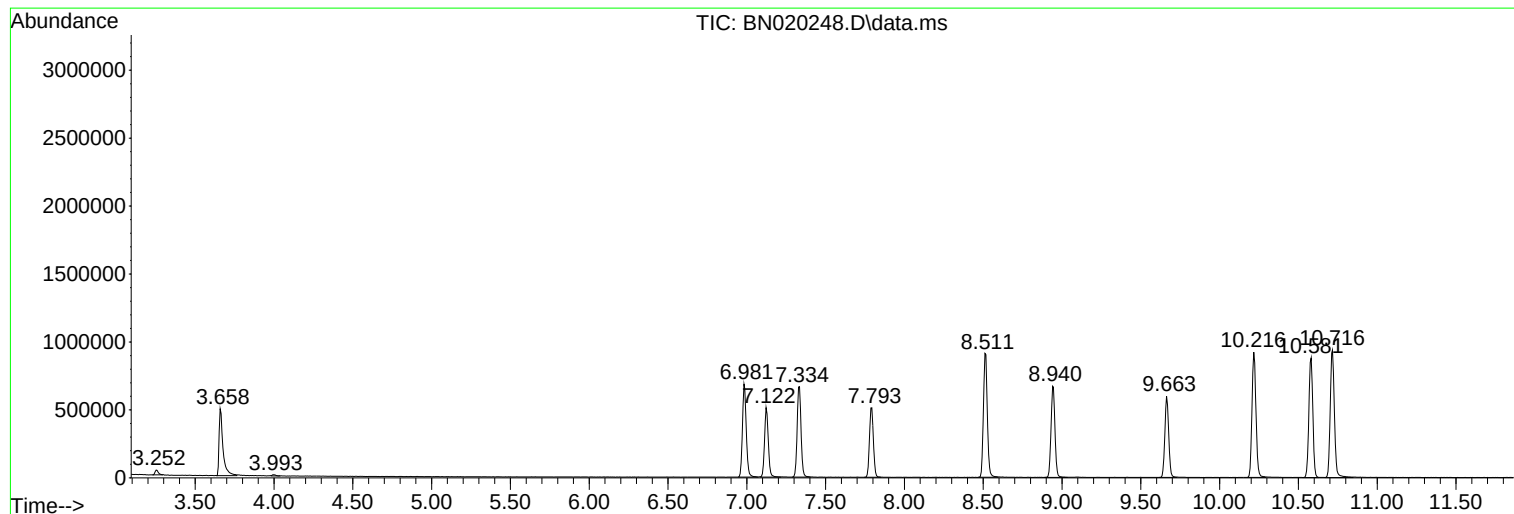

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020248.D
Acq On : 17 Jun 2022 21:03
Operator : CG/JU
Sample : PB145571BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061722\
Data File : BN020248.D
Acq On : 17 Jun 2022 21:03
Operator : CG/JU
Sample : PB145571BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------