

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020301.D
 Acq On : 21 Jun 2022 11:14
 Operator : CG/JU
 Sample : PB145581BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK581

Quant Time: Jun 22 00:07:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	1019	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	3576	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.419	164	2431	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.159	188	5824	0.400	ng/ul	0.00
17) Chrysene-d12	21.357	240	7124	0.400	ng/ul	0.00
23) Perylene-d12	23.663	264	10603	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	5291	4.547	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.179	152	1636	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.193	212	5254	0.357	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.409	166	618	0.054	ng/ul#	20
20) Pyrene	19.556	202	851	0.027	ng/ul#	1
26) Benzo(a)pyrene	23.514	252	2746	0.057	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020301.D
Acq On : 21 Jun 2022 11:14
Operator : CG/JU
Sample : PB145581BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK581

Quant Time: Jun 22 00:07:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




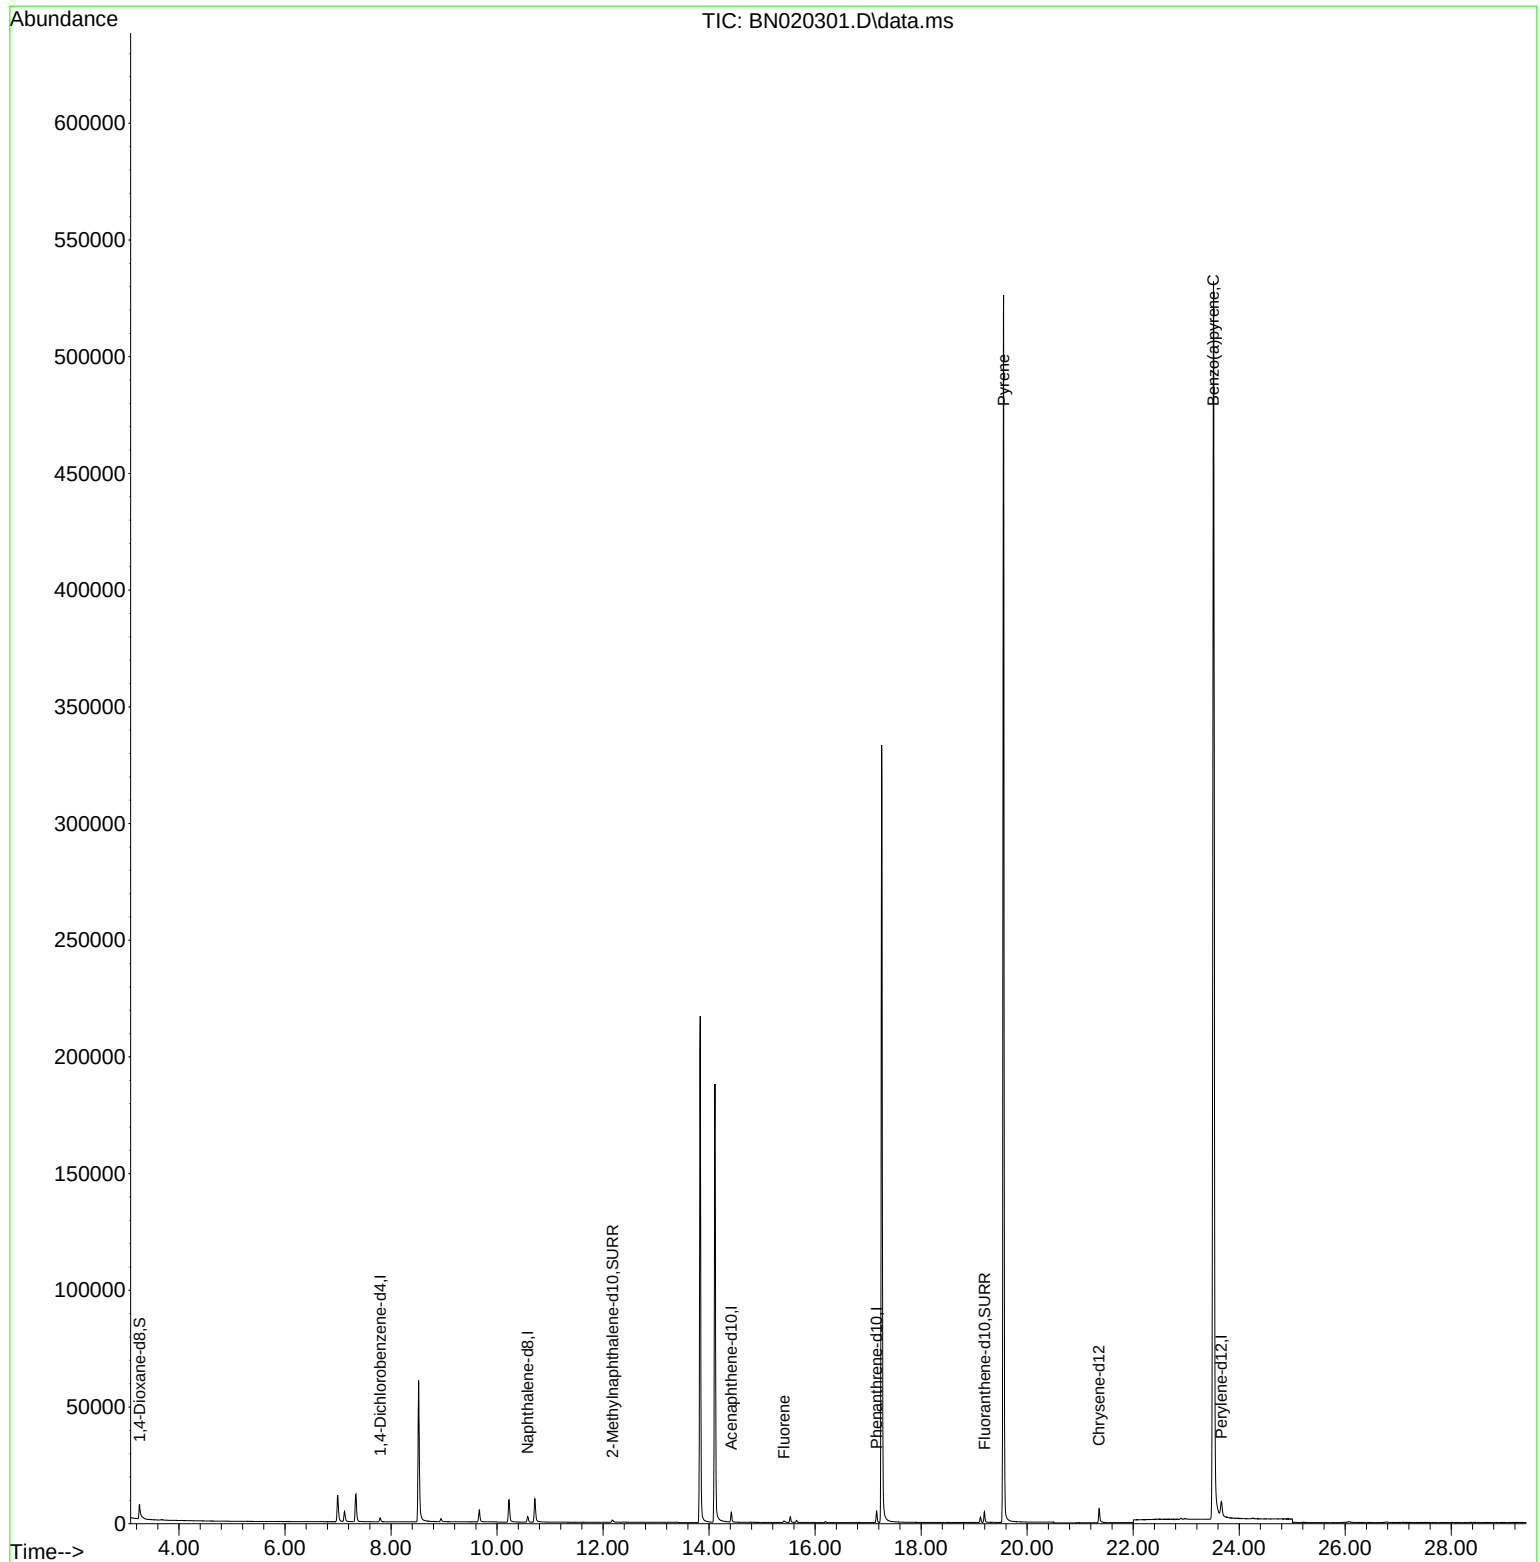


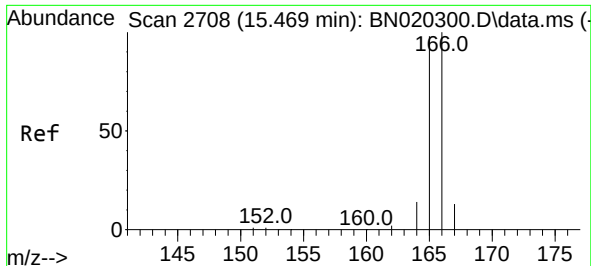

#12
Fluorene
Concen: 0.054 ng/ul
RT: 15.409 min Scan# 2695
Delta R.T. -0.064 min
Lab File: BN020301.D
Acq: 21 Jun 2022 11:14




Instrument :
BNA_N
ClientSampleId :
SBLK581


Tgt Ion:166 Resp: 618
Ion Ratio Lower Upper
166 100
165 16.1 78.2 117.4#
167 40.3 12.1 18.1#

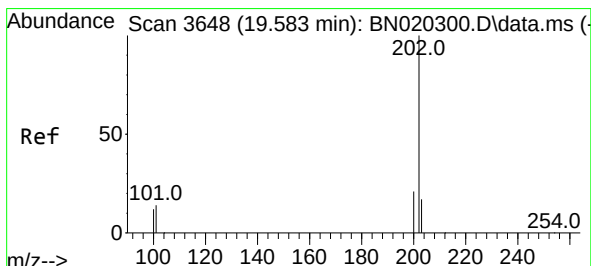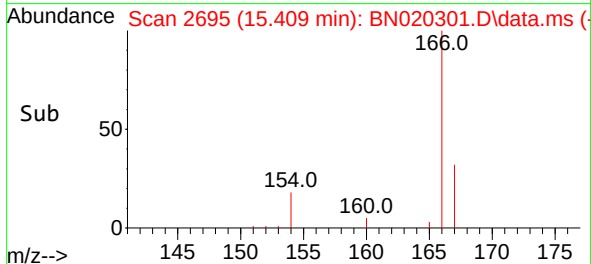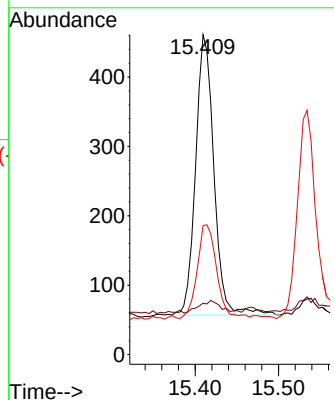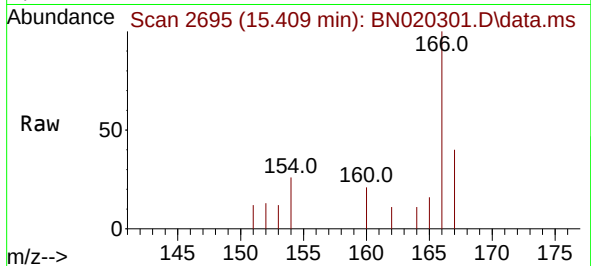

#20
Pyrene
Concen: 0.027 ng/ul
RT: 19.556 min Scan# 3642
Delta R.T. -0.027 min
Lab File: BN020301.D
Acq: 21 Jun 2022 11:14

Tgt Ion:202 Resp: 851
Ion Ratio Lower Upper
202 100
101 160.8 12.6 19.0#
100 1086.5 10.3 15.5#

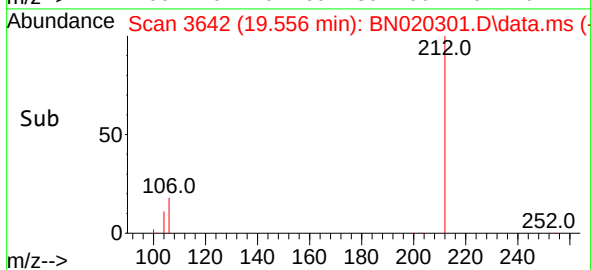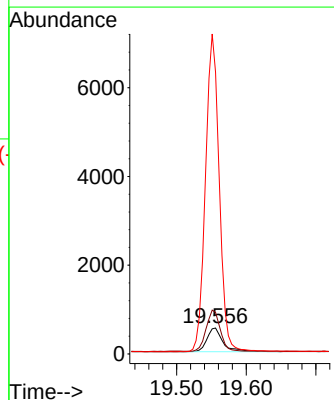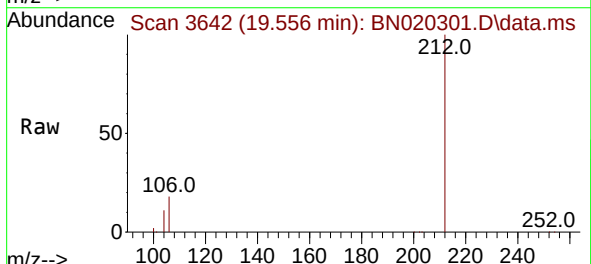

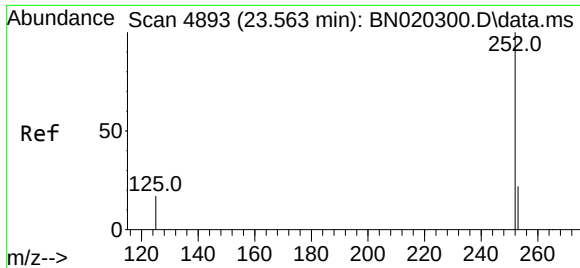

#26

Benzo(a)pyrene

Concen: 0.057 ng/ul

RT: 23.514 min Scan# 41

Delta R.T. -0.049 min

Lab File: BN020301.D


Acq: 21 Jun 2022 11:14

Instrument :

BNA_N

ClientSampleId :

SBLK581

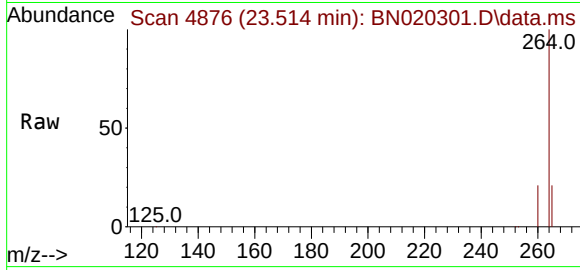

Tgt Ion:252 Resp: 2746

Ion Ratio Lower Upper

252 100

253 49.3 21.7 32.5#

125 38.2 18.6 28.0#

