

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020302.D
 Acq On : 21 Jun 2022 11:50
 Operator : CG/JU
 Sample : PB145572BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK572

Quant Time: Jun 22 00:08:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	674	0.400	ng/ul	0.00
4) Naphthalene-d8	10.577	136	2455	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.422	164	1824	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.161	188	4649	0.400	ng/ul	0.00
17) Chrysene-d12	21.356	240	5903	0.400	ng/ul	0.00
23) Perylene-d12	23.656	264	9524	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	5097	6.623	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.178	152	1558	0.384	ng/ul	0.00
18) Fluoranthene-d10	19.191	212	5745	0.471	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.412	166	604	0.070	ng/ul#	20
20) Pyrene	19.553	202	920	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.510	252	3089	0.072	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020302.D
Acq On : 21 Jun 2022 11:50
Operator : CG/JU
Sample : PB145572BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK572

Quant Time: Jun 22 00:08:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




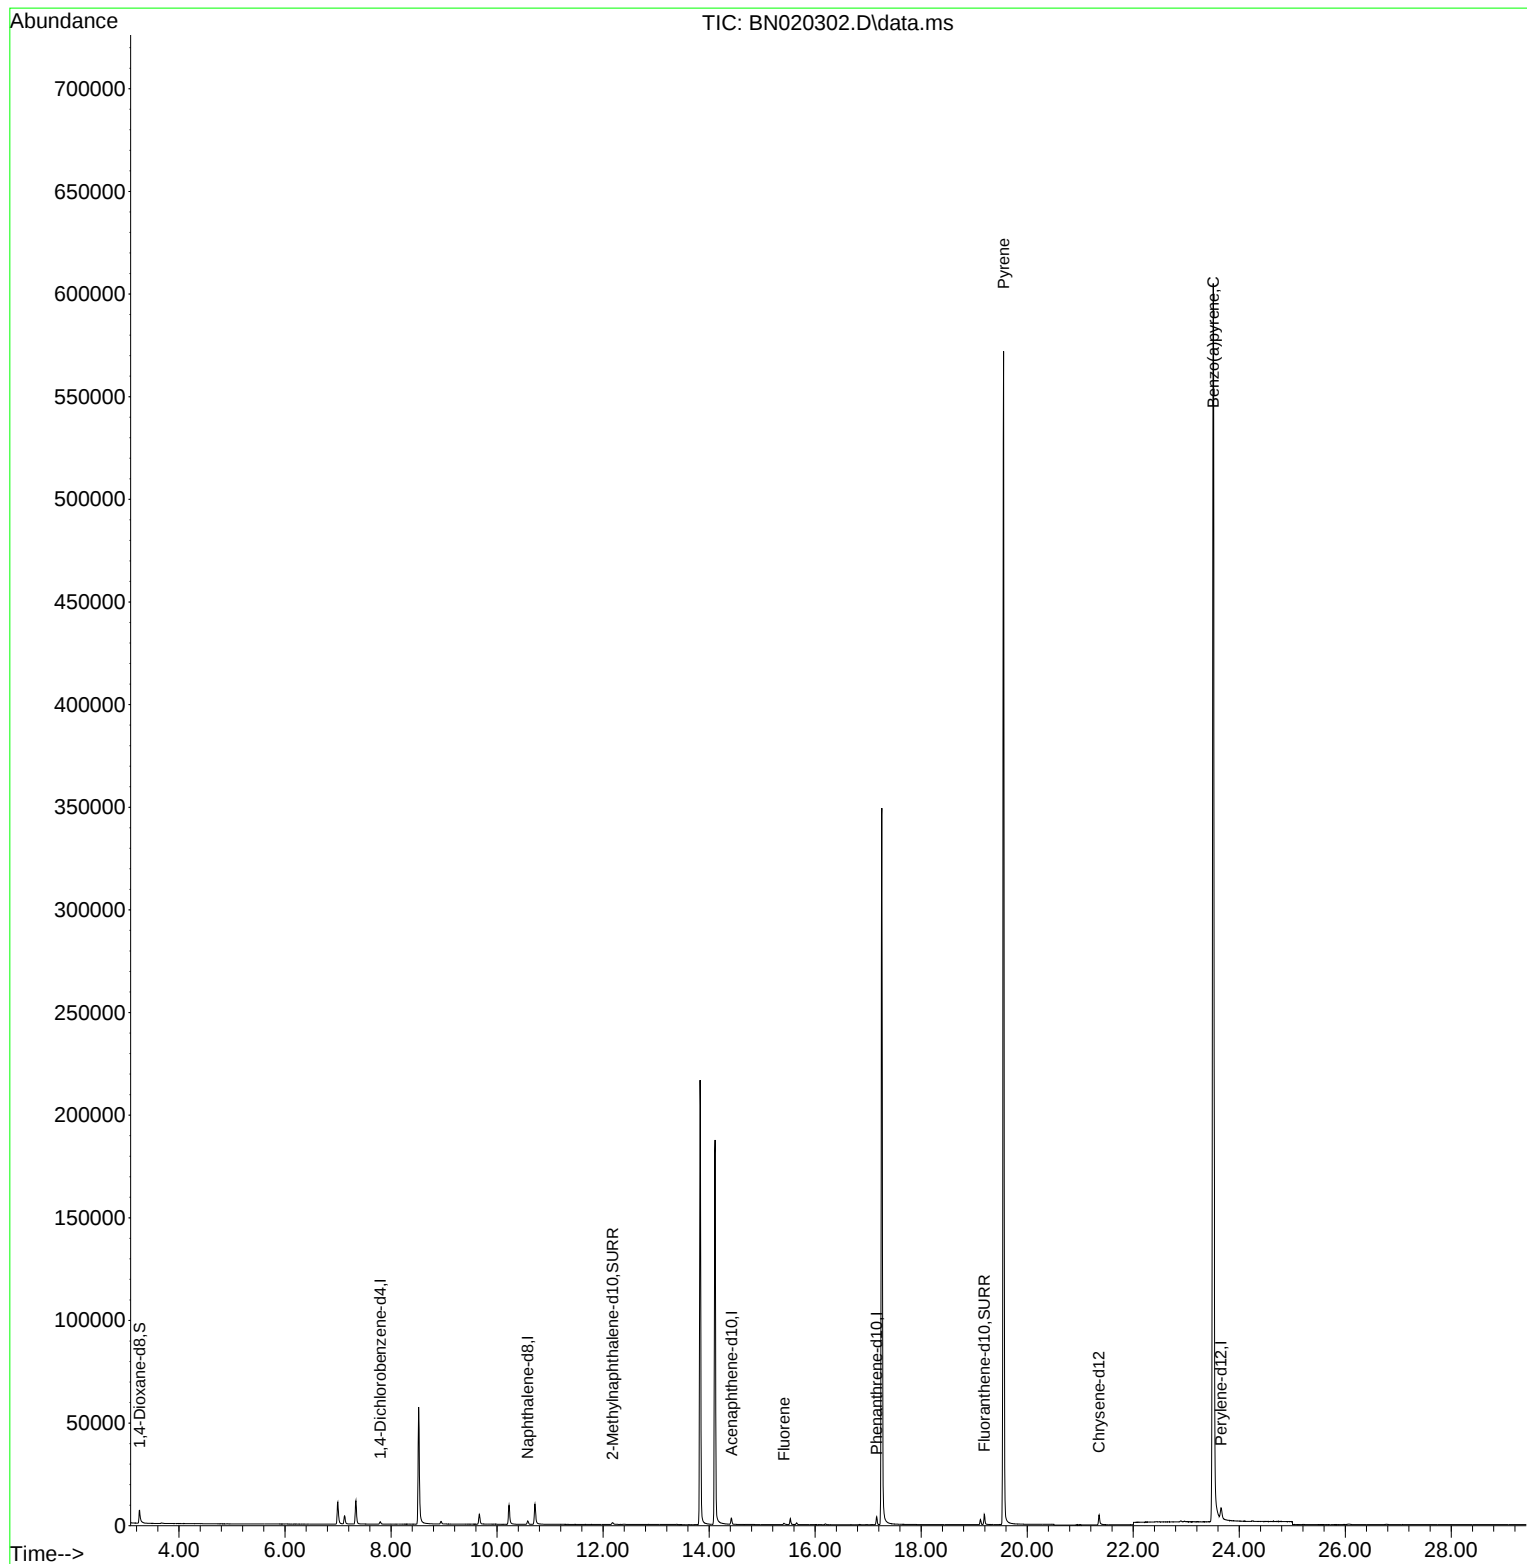


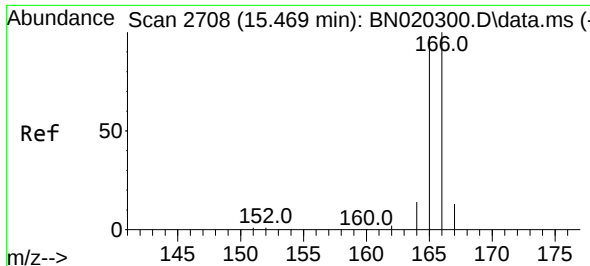

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.412 min Scan# 2696
Delta R.T. -0.062 min
Lab File: BN020302.D
Acq: 21 Jun 2022 11:50




Instrument :
BNA_N
ClientSampleId :
SBLK572


Tgt Ion:166 Resp: 604
Ion Ratio Lower Upper
166 100
165 17.2 78.2 117.4#
167 42.8 12.1 18.1#

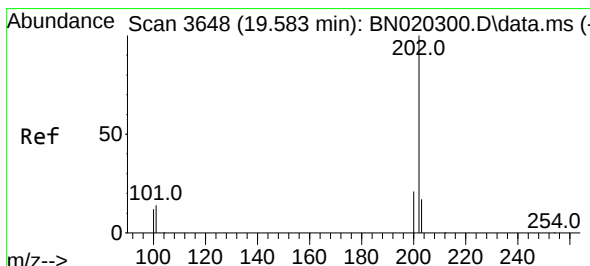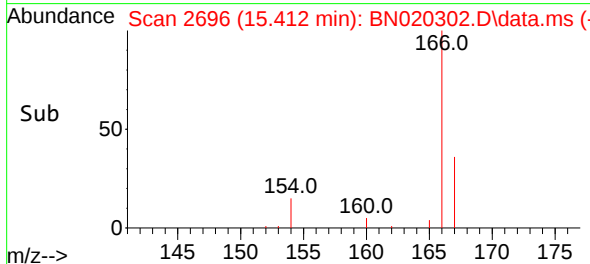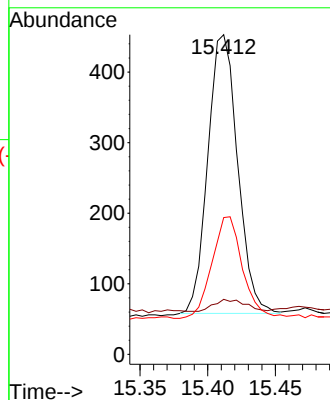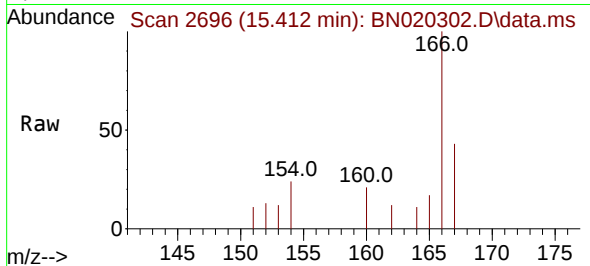

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.553 min Scan# 3642
Delta R.T. -0.030 min
Lab File: BN020302.D
Acq: 21 Jun 2022 11:50

Tgt Ion:202 Resp: 920
Ion Ratio Lower Upper
202 100
101 165.3 12.6 19.0#
100 1180.1 10.3 15.5#

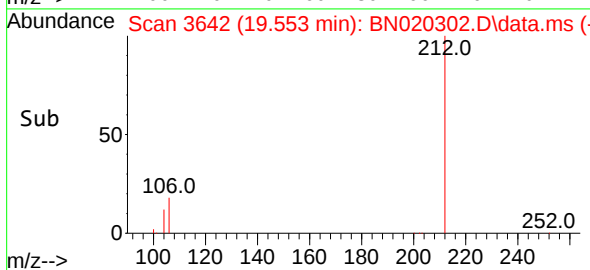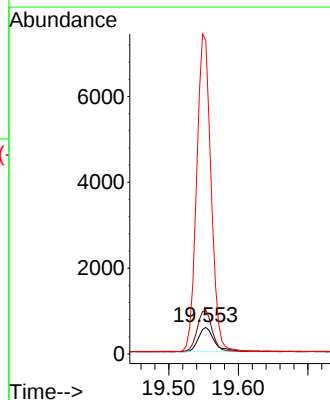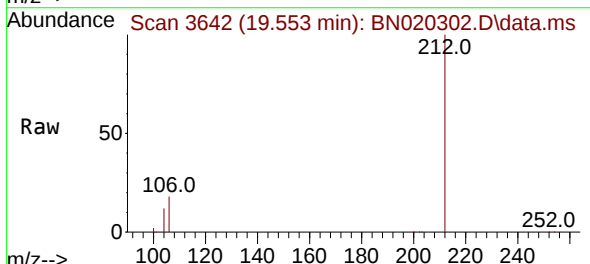

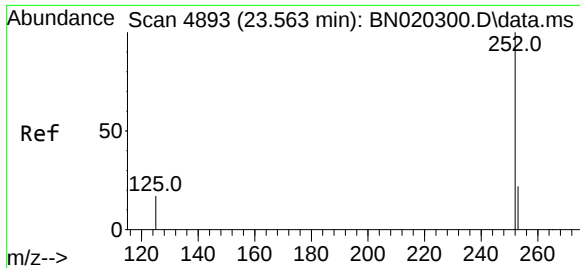

#26

Benzo(a)pyrene

Concen: 0.072 ng/ul

RT: 23.510 min Scan# 4875

Delta R.T. -0.053 min

Lab File: BN020302.D


Acq: 21 Jun 2022 11:50

Instrument :

BNA_N

ClientSampleId :

SBLK572

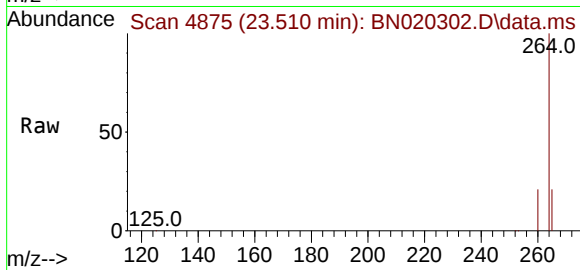

Tgt Ion:252 Resp: 3089

Ion Ratio Lower Upper

252 100

253 47.0 21.7 32.5#

125 38.5 18.6 28.0#

