

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020304.D
 Acq On : 21 Jun 2022 13:02
 Operator : CG/JU
 Sample : N3313-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7N1

Quant Time: Jun 22 00:08:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	837	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	3184	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.419	164	2357	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.158	188	5897	0.400	ng/ul	0.00
17) Chrysene-d12	21.353	240	7337	0.400	ng/ul	0.00
23) Perylene-d12	23.659	264	10469	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	3997	4.182	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.174	152	1631	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	6574	0.434	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.273	88	51	0.055	ng/ul#	74
20) Pyrene	19.555	202	1191	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.510	252	3370	0.071	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020304.D
Acq On : 21 Jun 2022 13:02
Operator : CG/JU
Sample : N3313-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7N1

Quant Time: Jun 22 00:08:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




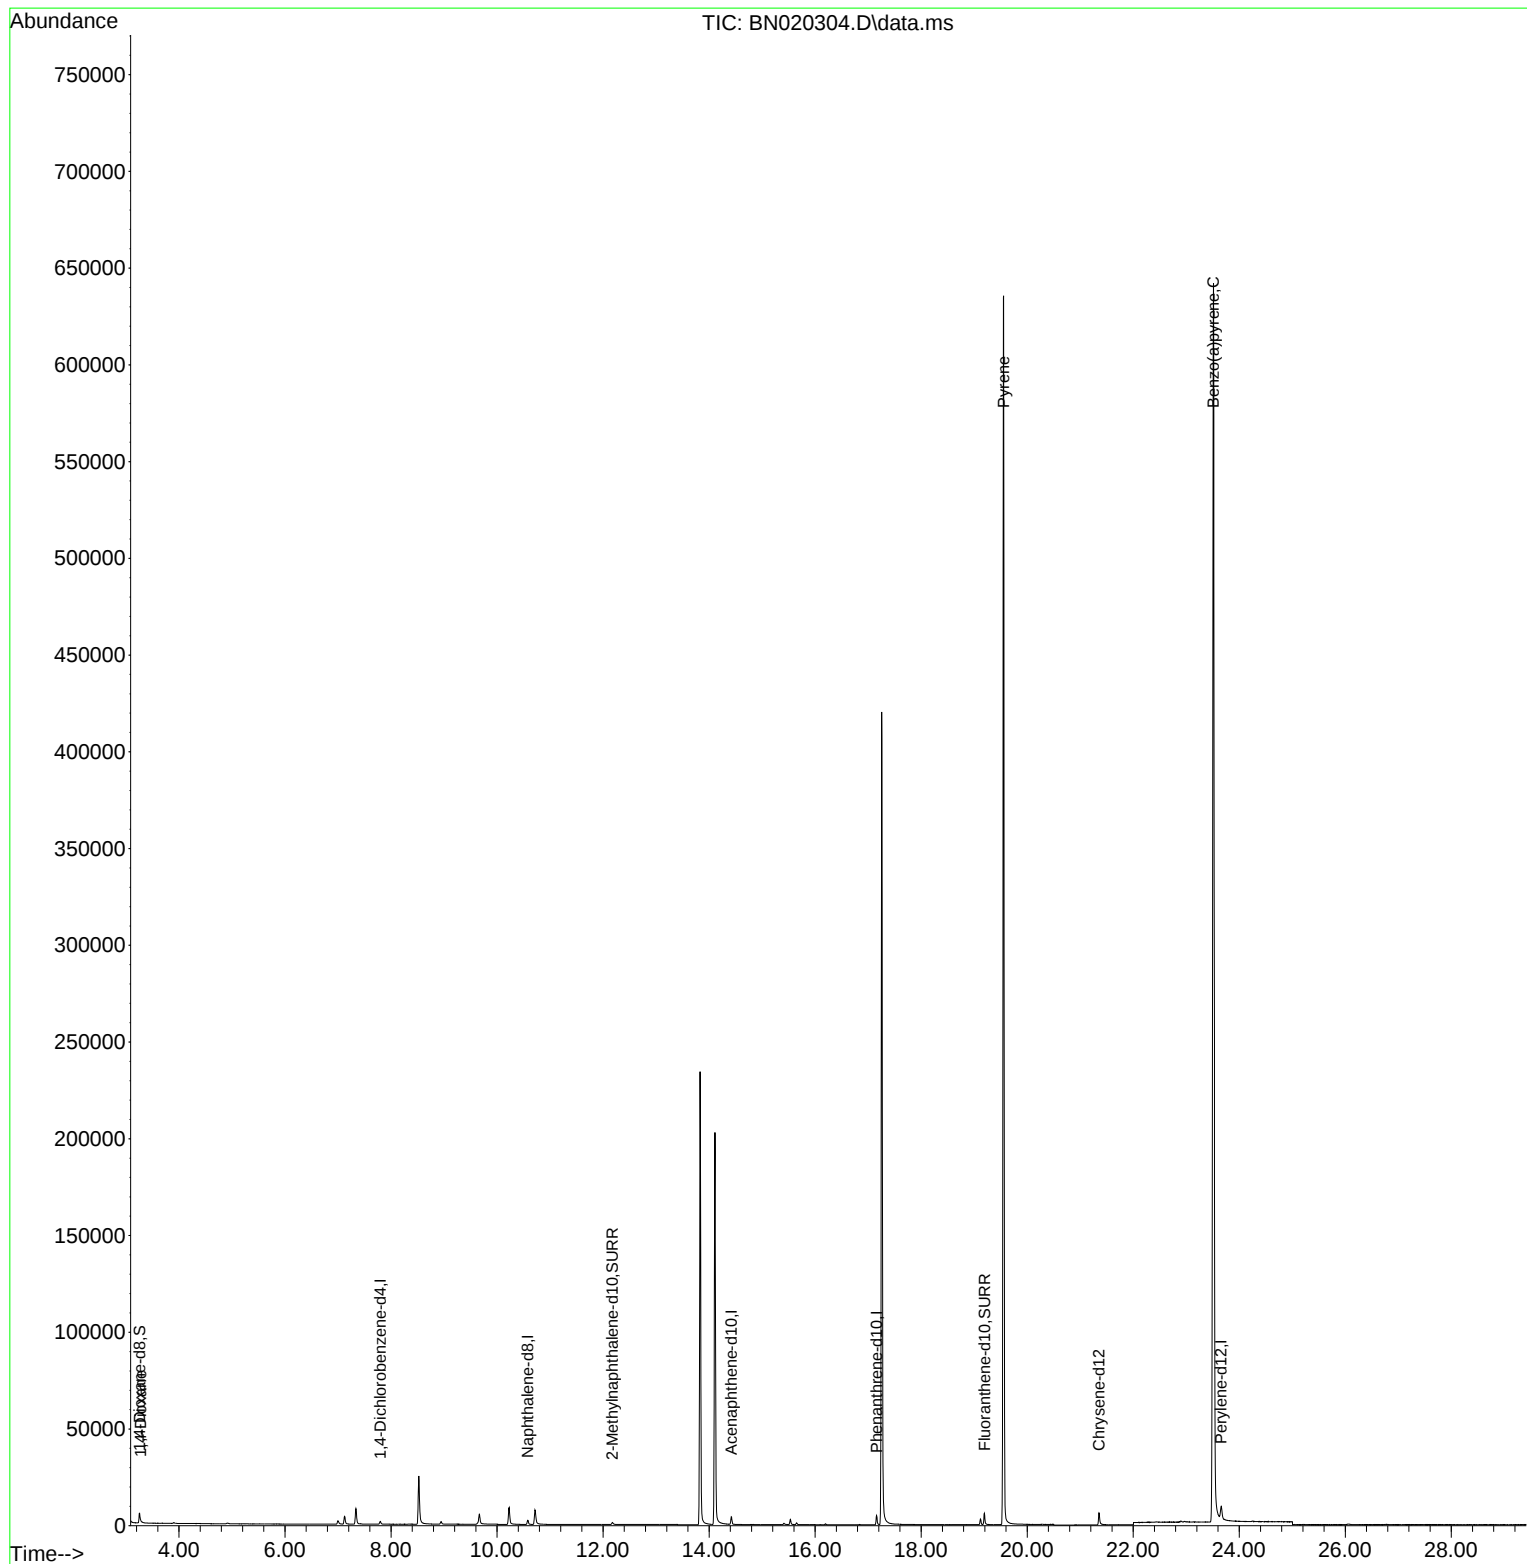


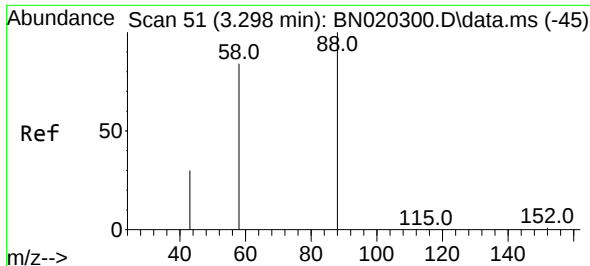

#2
 1,4-Dioxane
 Concen: 0.055 ng/ul
 RT: 3.273 min Scan# 41
 Delta R.T. -0.021 min
 Lab File: BN020304.D
 Acq: 21 Jun 2022 13:02




Instrument :
 BNA_N
 ClientSampleId :
 YB7N1


Tgt Ion: 88 Resp: 51
 Ion Ratio Lower Upper
 88 100
 43 61.3 31.6 47.4#
 58 22.1 23.8 35.6#

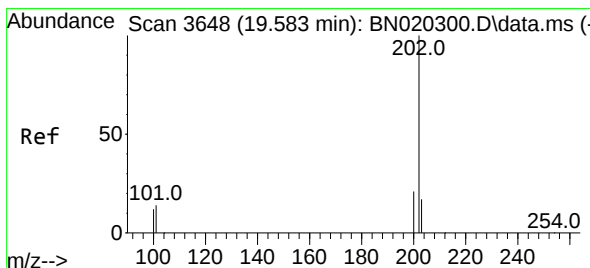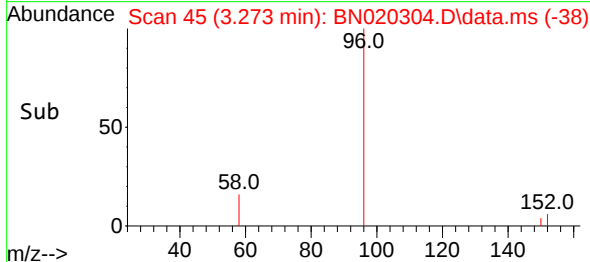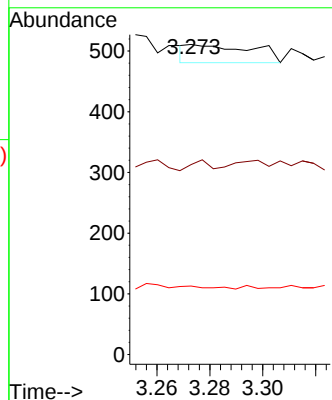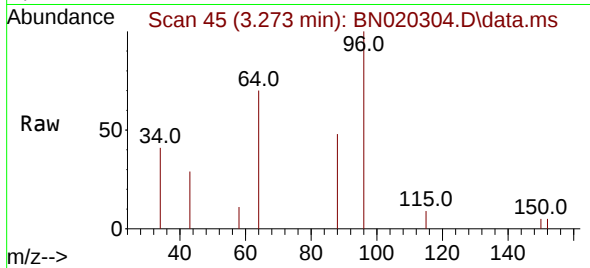

#20
 Pyrene
 Concen: 0.037 ng/ul
 RT: 19.555 min Scan# 3642
 Delta R.T. -0.028 min
 Lab File: BN020304.D
 Acq: 21 Jun 2022 13:02

Tgt Ion: 202 Resp: 1191
 Ion Ratio Lower Upper
 202 100
 101 159.7 12.6 19.0#
 100 1083.5 10.3 15.5#

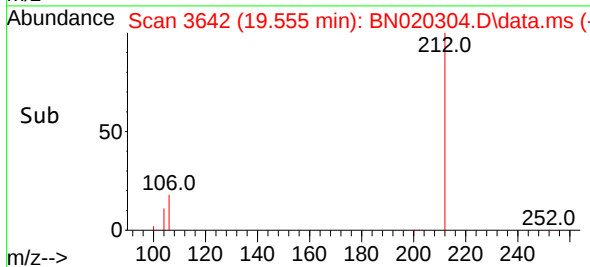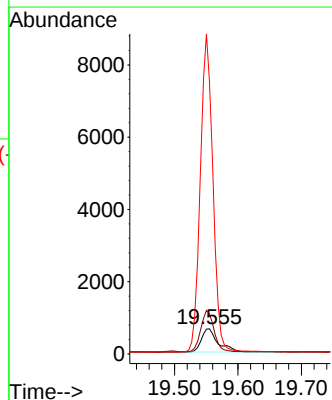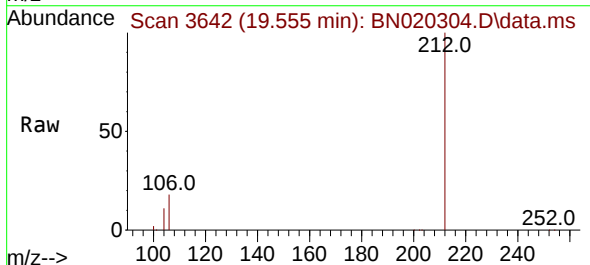

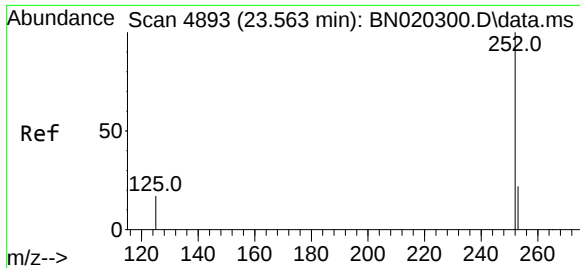

#26

Benzo(a)pyrene

Concen: 0.071 ng/ul

RT: 23.510 min Scan# 41

Delta R.T. -0.053 min

Lab File: BN020304.D


Acq: 21 Jun 2022 13:02

Instrument :

BNA_N

ClientSampleId :

YB7N1

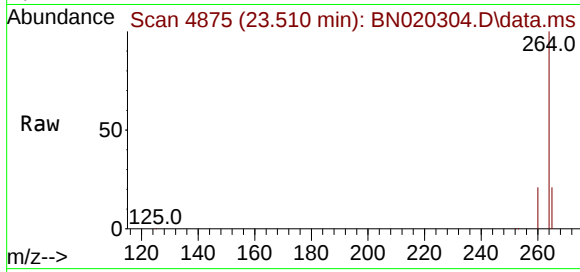

Tgt Ion:252 Resp: 3370

Ion Ratio Lower Upper

252 100

253 46.6 21.7 32.5#

125 37.4 18.6 28.0#

