

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020306.D
 Acq On : 21 Jun 2022 14:14
 Operator : CG/JU
 Sample : N3313-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L2

Quant Time: Jun 22 00:08:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	659	0.400	ng/ul	0.00
4) Naphthalene-d8	10.583	136	2389	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.422	164	1730	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.161	188	4522	0.400	ng/ul	0.00
17) Chrysene-d12	21.354	240	6531	0.400	ng/ul	0.00
23) Perylene-d12	23.660	264	10068	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	2898	3.851	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.178	152	1155	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.191	212	5298	0.393	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.290	88	932	1.287	ng/ul#	71
20) Pyrene	19.554	202	865	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.511	252	2901	0.064	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020306.D
Acq On : 21 Jun 2022 14:14
Operator : CG/JU
Sample : N3313-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L2

Quant Time: Jun 22 00:08:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




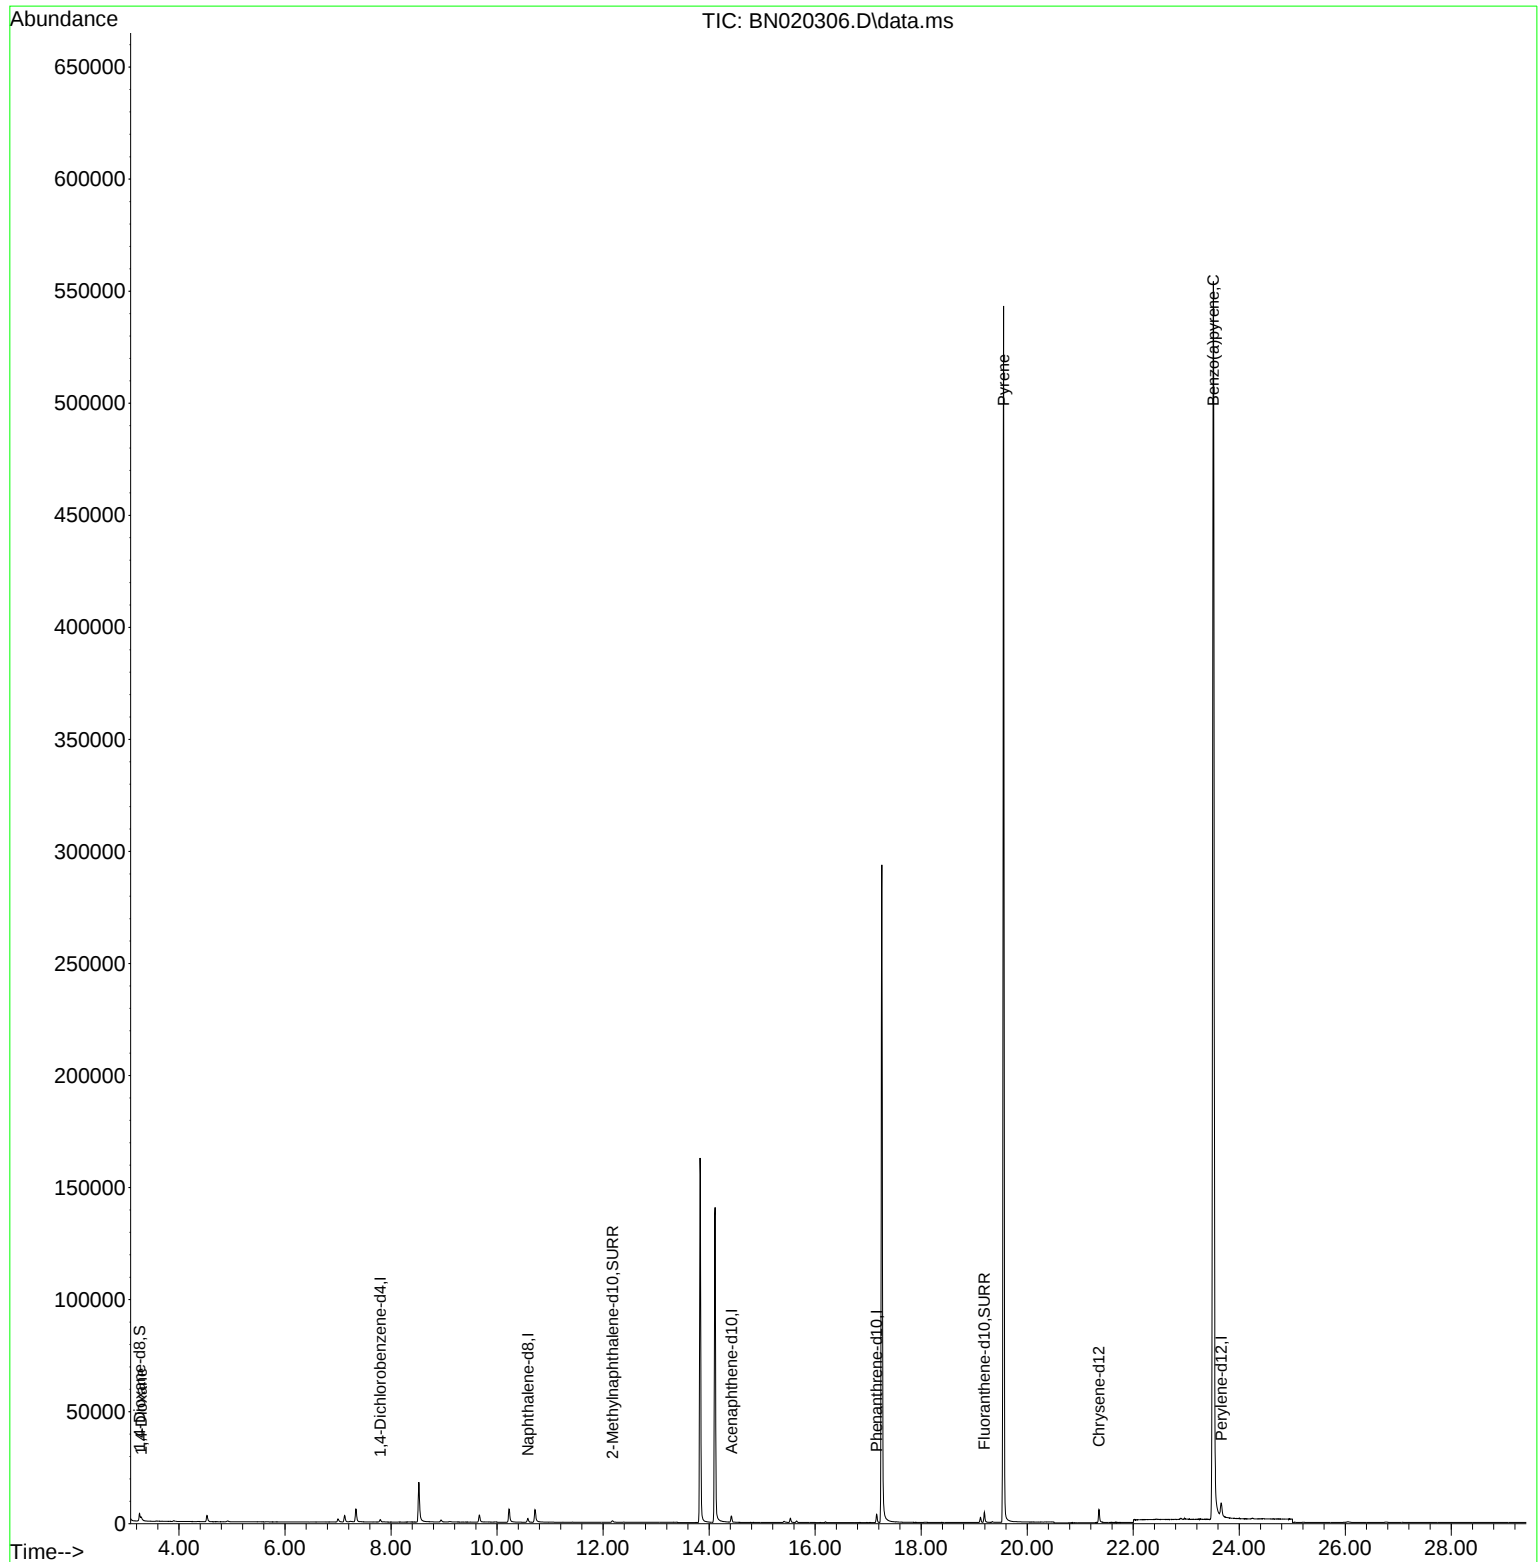


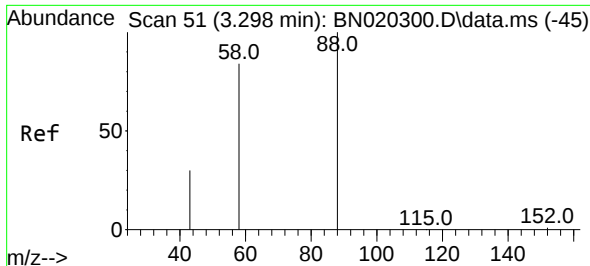

#2
 1,4-Dioxane
 Concen: 1.287 ng/ul
 RT: 3.290 min Scan# 49
 Delta R.T. -0.004 min
 Lab File: BN020306.D
 Acq: 21 Jun 2022 14:14




Instrument :
 BNA_N
 ClientSampleId :
 YB7L2


Tgt Ion: 88 Resp: 932
 Ion Ratio Lower Upper
 88 100
 43 45.5 31.6 47.4
 58 59.3 23.8 35.6#

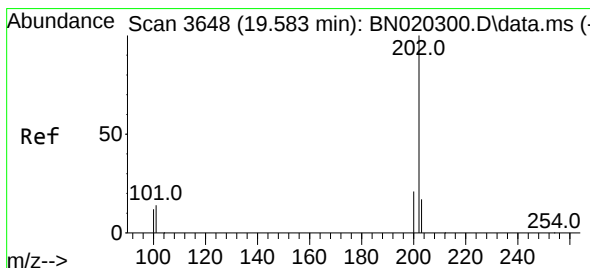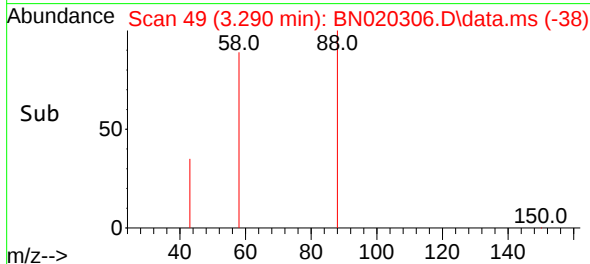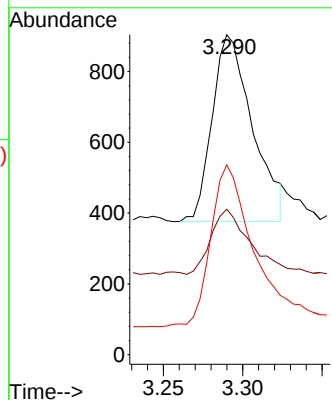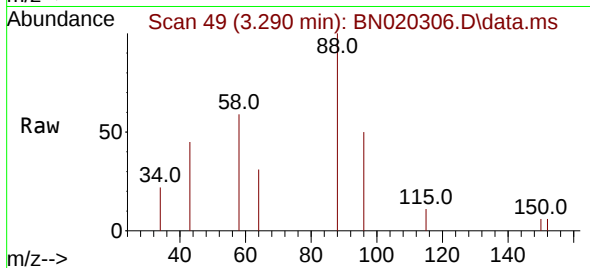

#20
 Pyrene
 Concen: 0.030 ng/ul
 RT: 19.554 min Scan# 3642
 Delta R.T. -0.029 min
 Lab File: BN020306.D
 Acq: 21 Jun 2022 14:14

Tgt Ion: 202 Resp: 865
 Ion Ratio Lower Upper
 202 100
 101 172.0 12.6 19.0#
 100 1190.4 10.3 15.5#

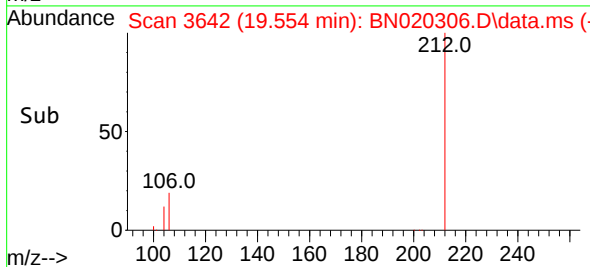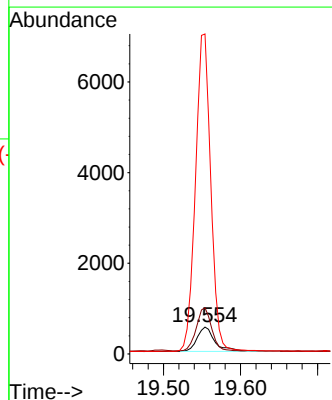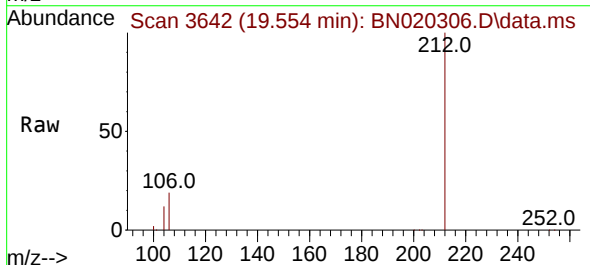

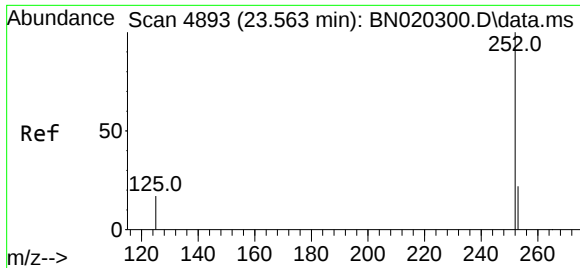

#26

Benzo(a)pyrene

Concen: 0.064 ng/ul

RT: 23.511 min Scan# 4875

Delta R.T. -0.052 min

Lab File: BN020306.D


Acq: 21 Jun 2022 14:14

Instrument :

BNA_N

ClientSampleId :

YB7L2

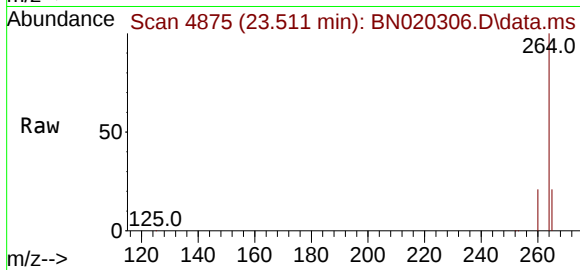

Tgt Ion:252 Resp: 2901

Ion Ratio Lower Upper

252 100

253 50.5 21.7 32.5#

125 40.9 18.6 28.0#

