

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020309.D
 Acq On : 21 Jun 2022 16:02
 Operator : CG/JU
 Sample : N3313-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L1

Quant Time: Jun 22 00:08:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	610	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136	2114	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.418	164	1580	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.162	188	4074	0.400	ng/ul	0.00
17) Chrysene-d12	21.353	240	6215	0.400	ng/ul	0.00
23) Perylene-d12	23.659	264	9896	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	4529	6.502	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152	1360	0.389	ng/ul	0.00
18) Fluoranthene-d10	19.192	212	5591	0.436	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.294	88	541	0.807	ng/ul#	86
14) Pentachlorophenol	16.833	266	22	0.028	ng/ul	91
20) Pyrene	19.555	202	950	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.510	252	3072	0.069	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020309.D
Acq On : 21 Jun 2022 16:02
Operator : CG/JU
Sample : N3313-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L1

Quant Time: Jun 22 00:08:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




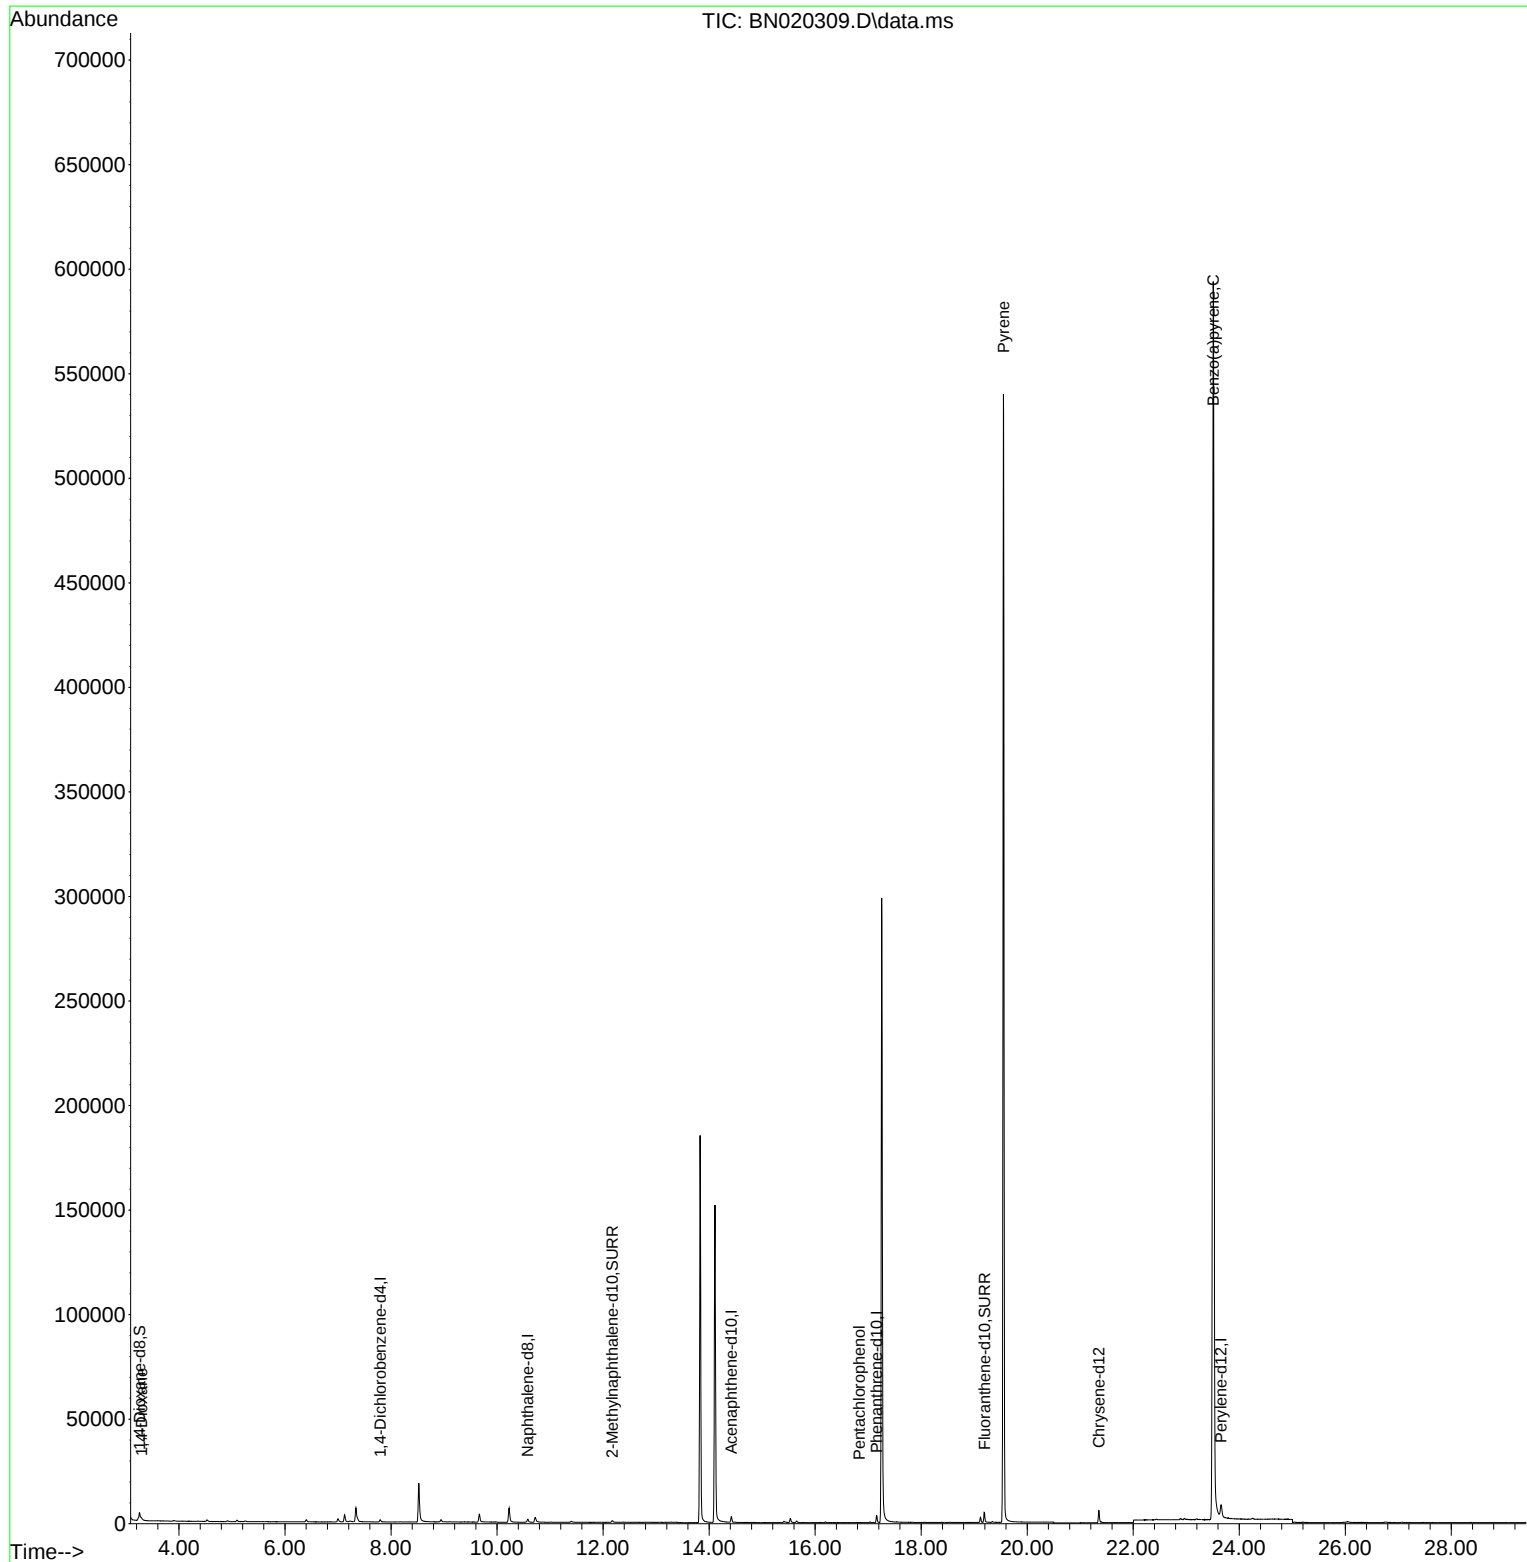


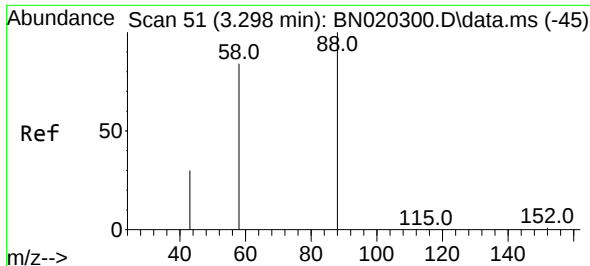

#2
1,4-Dioxane
Concen: 0.807 ng/ul
RT: 3.294 min Scan# 51
Delta R.T. -0.000 min
Lab File: BN020309.D
Acq: 21 Jun 2022 16:02




Instrument :
BNA_N
ClientSampleId :
YB7L1


Tgt Ion: 88 Resp: 541
Ion Ratio Lower Upper
88 100
43 45.3 31.6 47.4
58 41.0 23.8 35.6#

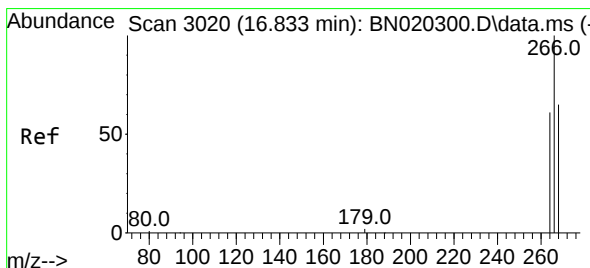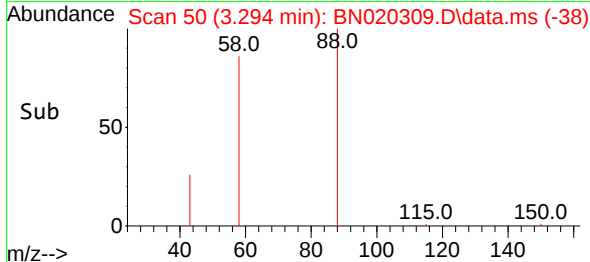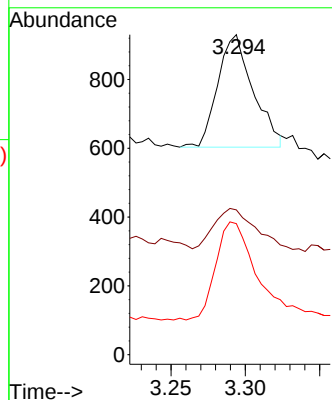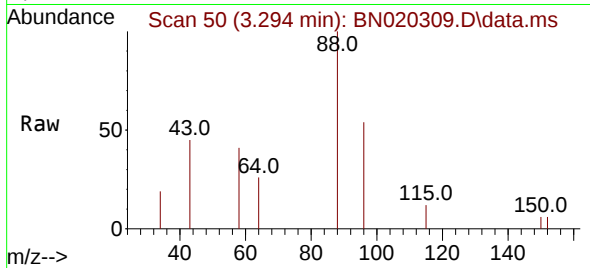

#14
Pentachlorophenol
Concen: 0.028 ng/ul
RT: 16.833 min Scan# 3020
Delta R.T. -0.004 min
Lab File: BN020309.D
Acq: 21 Jun 2022 16:02

Tgt Ion: 266 Resp: 22
Ion Ratio Lower Upper
266 100
264 63.6 49.8 74.8
268 77.3 51.8 77.6


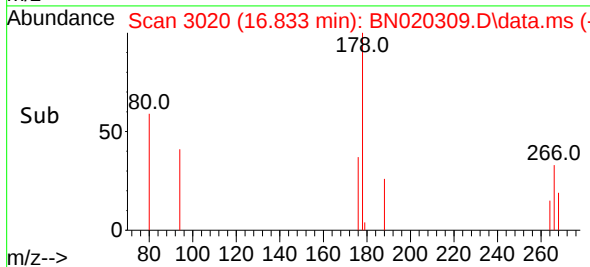
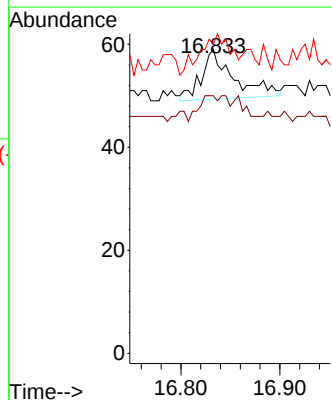
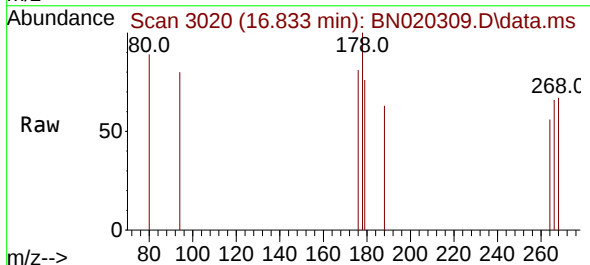


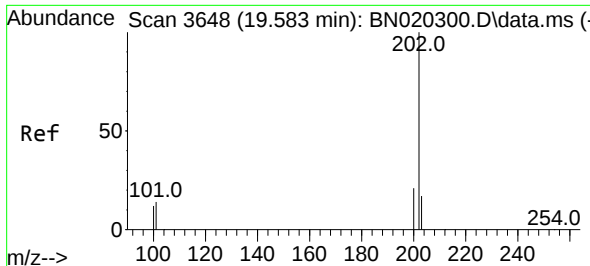

#20
Pyrene
Concen: 0.035 ng/u1
RT: 19.555 min Scan# 3642
Delta R.T. -0.028 min
Lab File: BN020309.D
Acq: 21 Jun 2022 16:02

Instrument :
BNA_N
ClientSampleId :
YB7L1

Tgt Ion:202 Resp: 950
Ion Ratio Lower Upper
202 100
101 157.4 12.6 19.0#
100 1062.4 10.3 15.5#

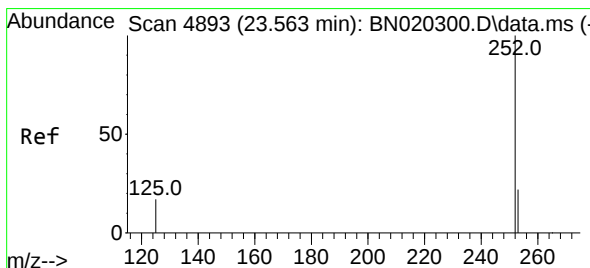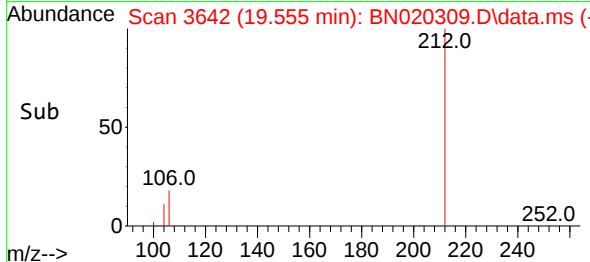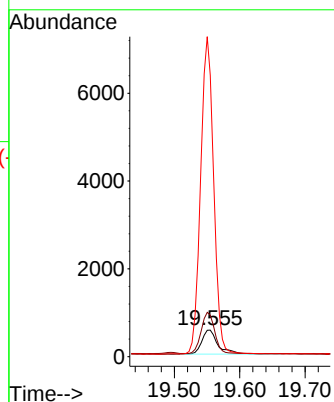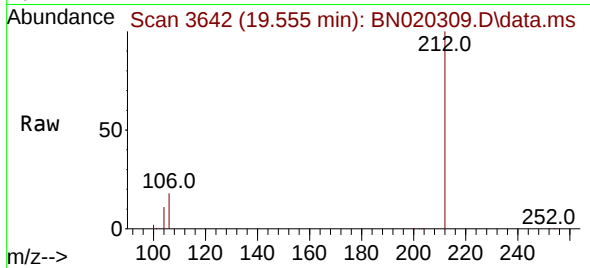

#26
Benzo(a)pyrene
Concen: 0.069 ng/u1
RT: 23.510 min Scan# 4875
Delta R.T. -0.053 min
Lab File: BN020309.D
Acq: 21 Jun 2022 16:02

Tgt Ion:252 Resp: 3072
Ion Ratio Lower Upper
252 100
253 47.5 21.7 32.5#
125 39.4 18.6 28.0#

