

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020311.D
 Acq On : 21 Jun 2022 17:15
 Operator : CG/JU
 Sample : N3313-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L4

Quant Time: Jun 22 00:08:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	751	0.400	ng/ul	0.00
4) Naphthalene-d8	10.583	136	2776	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.417	164	2042	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.161	188	5041	0.400	ng/ul	0.00
17) Chrysene-d12	21.351	240	7143	0.400	ng/ul	0.00
23) Perylene-d12	23.660	264	10088	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	5464	6.372	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.172	152	1674	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.191	212	6510	0.442	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.290	88	897	1.087	ng/ul#	66
20) Pyrene	19.554	202	1146	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.511	252	3364	0.074	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020311.D
Acq On : 21 Jun 2022 17:15
Operator : CG/JU
Sample : N3313-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L4

Quant Time: Jun 22 00:08:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration




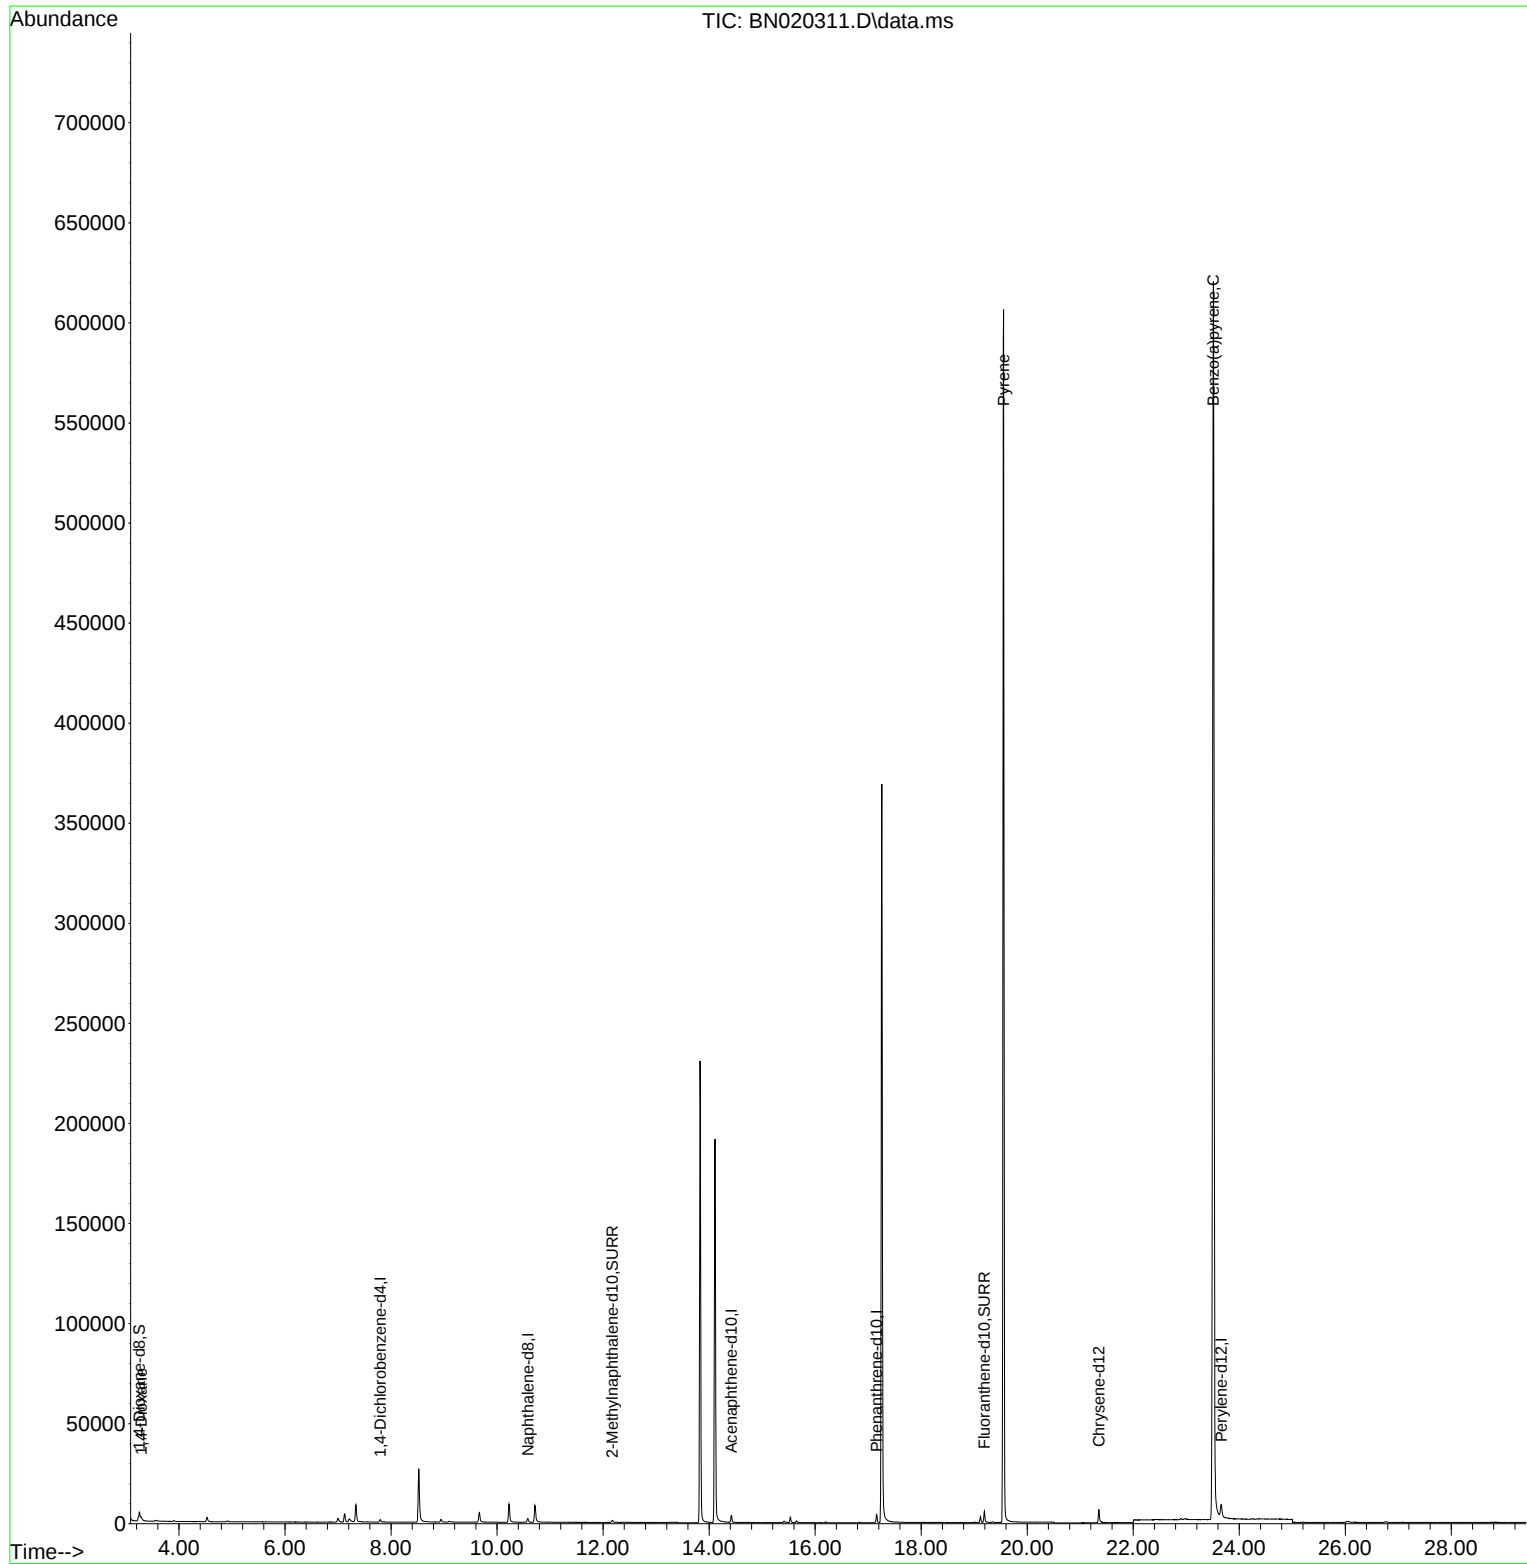


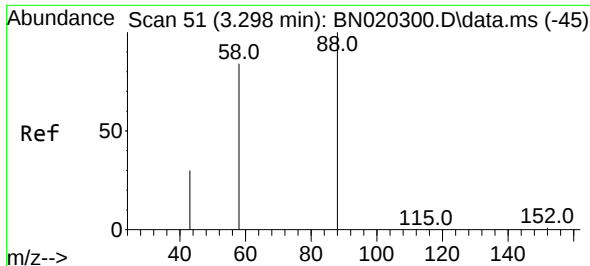

#2
 1,4-Dioxane
 Concen: 1.087 ng/ul
 RT: 3.290 min Scan# 49
 Delta R.T. -0.004 min
 Lab File: BN020311.D
 Acq: 21 Jun 2022 17:15




Instrument :
 BNA_N
 ClientSampleId :
 YB7L4


Tgt Ion: 88 Resp: 897
 Ion Ratio Lower Upper
 88 100
 43 52.6 31.6 47.4#
 58 57.2 23.8 35.6#

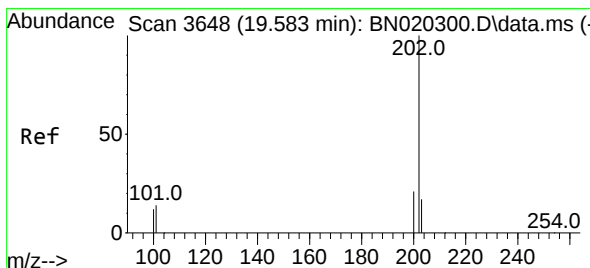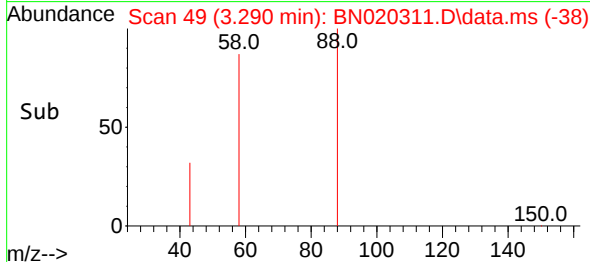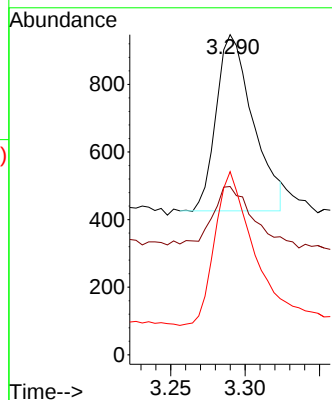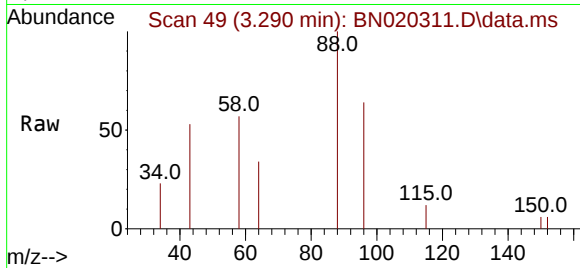

#20
 Pyrene
 Concen: 0.037 ng/ul
 RT: 19.554 min Scan# 3642
 Delta R.T. -0.029 min
 Lab File: BN020311.D
 Acq: 21 Jun 2022 17:15

Tgt Ion: 202 Resp: 1146
 Ion Ratio Lower Upper
 202 100
 101 161.7 12.6 19.0#
 100 1120.2 10.3 15.5#

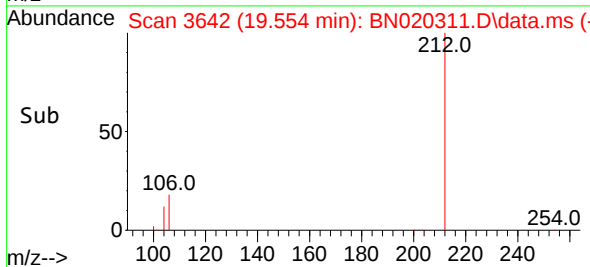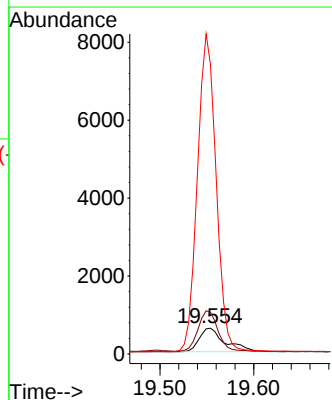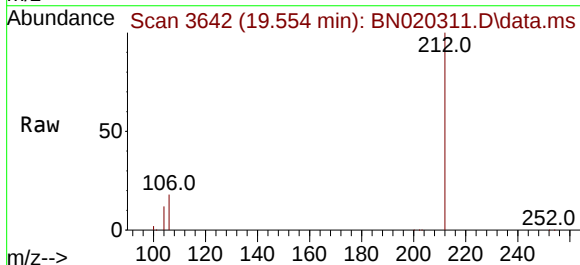

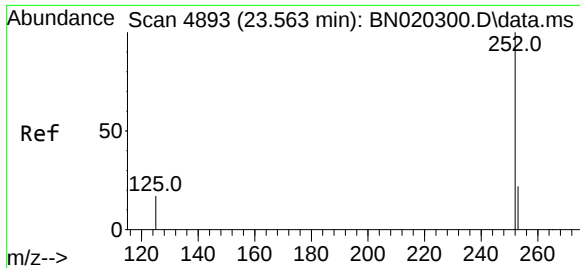

#26

Benzo(a)pyrene

Concen: 0.074 ng/ul

RT: 23.511 min Scan# 41

Delta R.T. -0.052 min

Lab File: BN020311.D


Acq: 21 Jun 2022 17:15

Instrument :

BNA_N

ClientSampleId :

YB7L4

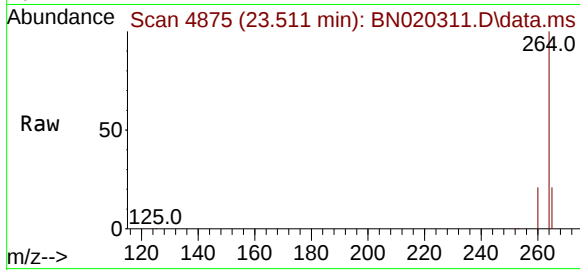

Tgt Ion:252 Resp: 3364

Ion Ratio Lower Upper

252 100

253 48.4 21.7 32.5#

125 42.5 18.6 28.0#

