




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020309.D
 Acq On : 21 Jun 2022 16:02
 Operator : CG/JU
 Sample : N3313-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:36:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

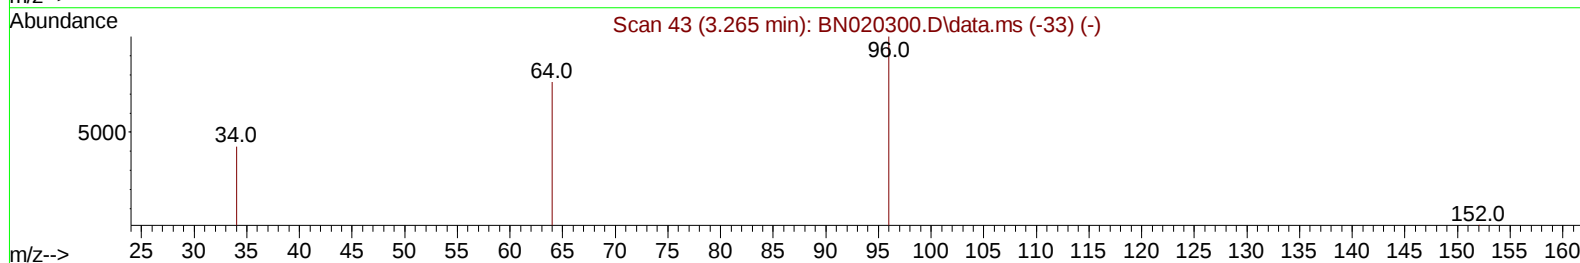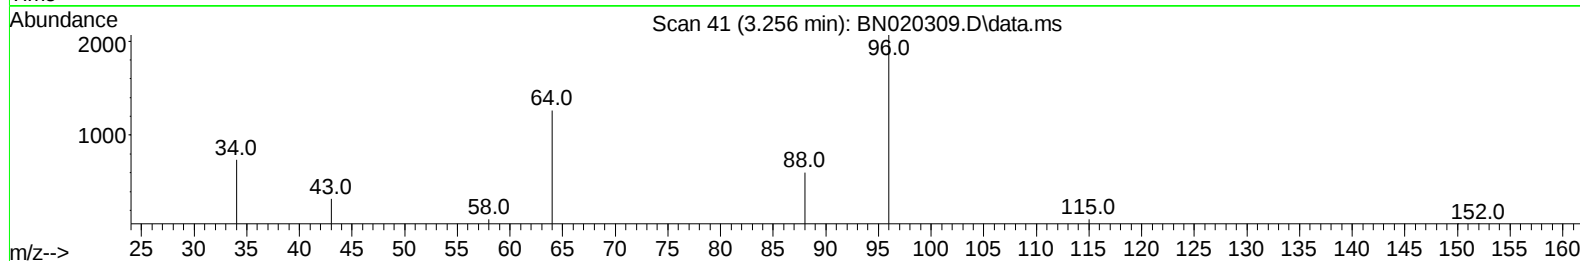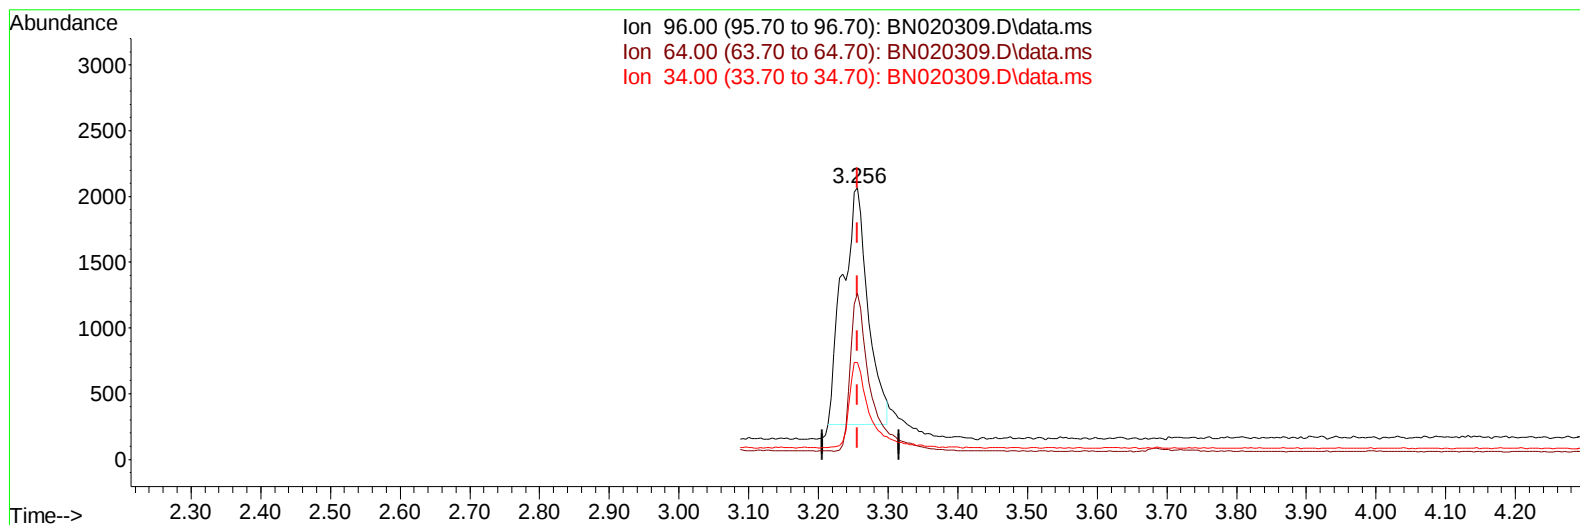

TIC: BN020309.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.256min (-0.000) 6.50 ng/u1

response 4529

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	58.80	61.21
34.00	45.10	35.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020309.D
 Acq On : 21 Jun 2022 16:02
 Operator : CG/JU
 Sample : N3313-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:36:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

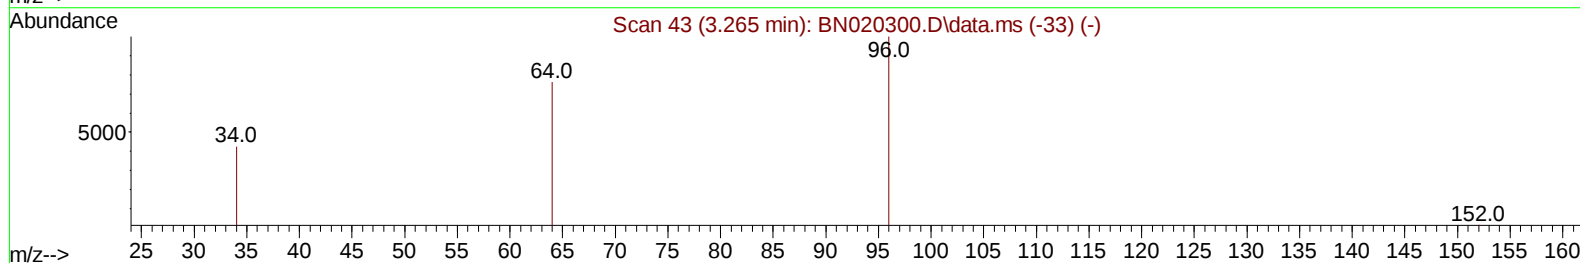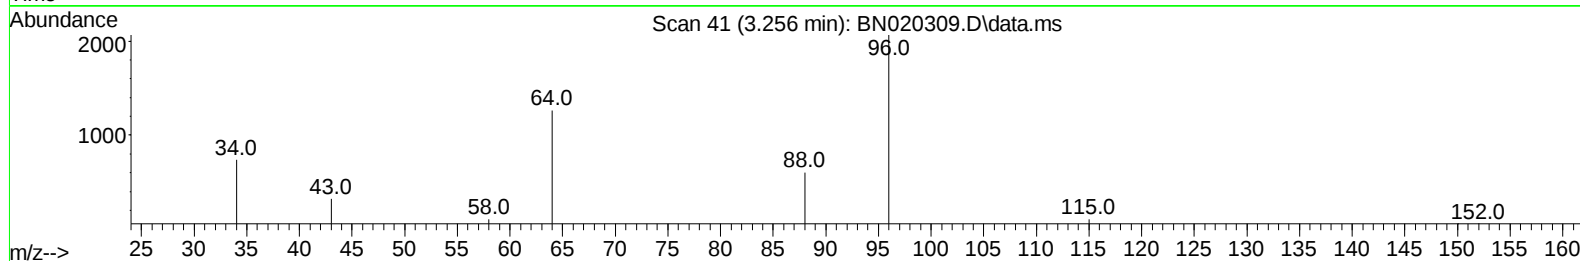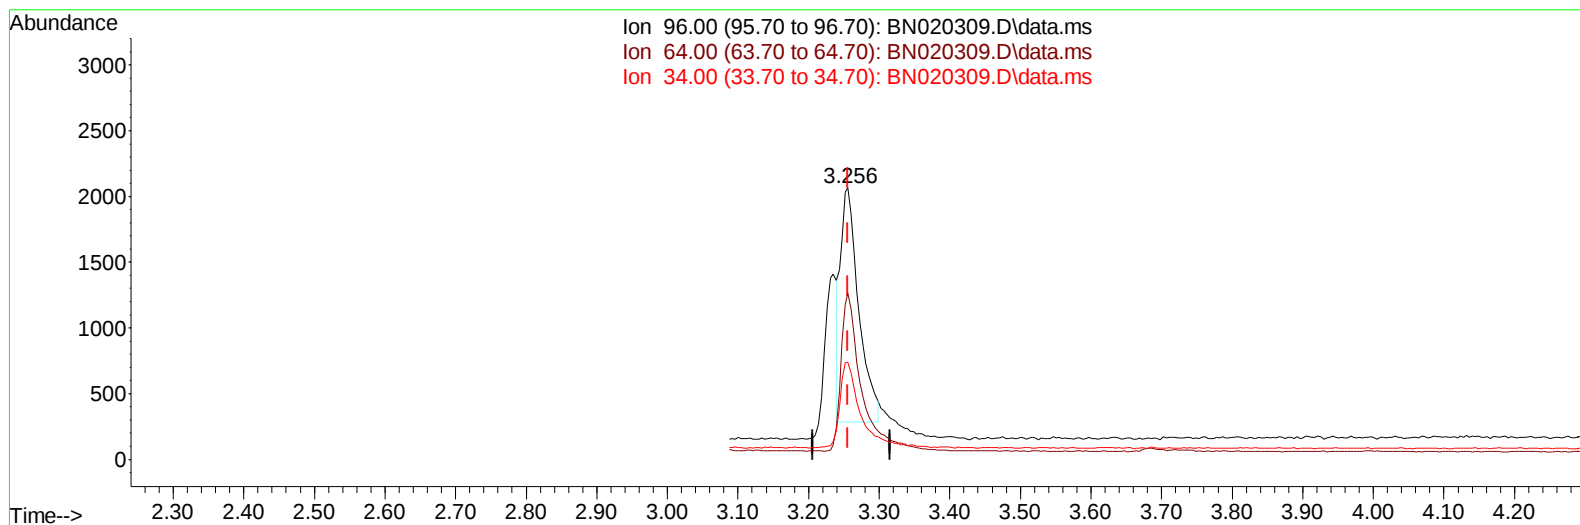

TIC: BN020309.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.256min (-0.000) 4.60 ng/ul m

response 3205

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	58.80	61.21
34.00	45.10	35.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020309.D
 Acq On : 21 Jun 2022 16:02
 Operator : CG/JU
 Sample : N3313-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 00:36:49 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.796	152		610	0.400	ng/ul	0.00
4) Naphthalene-d8	10.579	136		2114	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.418	164		1580	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.162	188		4074	0.400	ng/ul	0.00
17) Chrysene-d12	21.353	240		6215	0.400	ng/ul	0.00
23) Perylene-d12	23.659	264		9896	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.256	96		3205m	4.601	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.173	152		1360	0.389	ng/ul	0.00
18) Fluoranthene-d10	19.192	212		5591	0.436	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.294	88		541	0.807	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020309.D
Acq On : 21 Jun 2022 16:02
Operator : CG/JU
Sample : N3313-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L1

Manual IntegrationsAPPROVED

Quant Time: Jun 22 00:36:49 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022

