

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020306.D
 Acq On : 21 Jun 2022 14:14
 Operator : CG/JU
 Sample : N3313-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 00:08:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	659	0.400	ng/u1	0.00
4) Naphthalene-d8	10.583	136	2389	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.422	164	1730	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.161	188	4522	0.400	ng/u1	0.00
17) Chrysene-d12	21.354	240	6531	0.400	ng/u1	0.00
23) Perylene-d12	23.660	264	10068	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.256	96	2898	3.851	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.178	152	1155	0.292	ng/u1	0.00
18) Fluoranthene-d10	19.191	212	5298	0.393	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.290	88	985m	1.360	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020306.D
Acq On : 21 Jun 2022 14:14
Operator : CG/JU
Sample : N3313-02
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
YB7L2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 00:08:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration

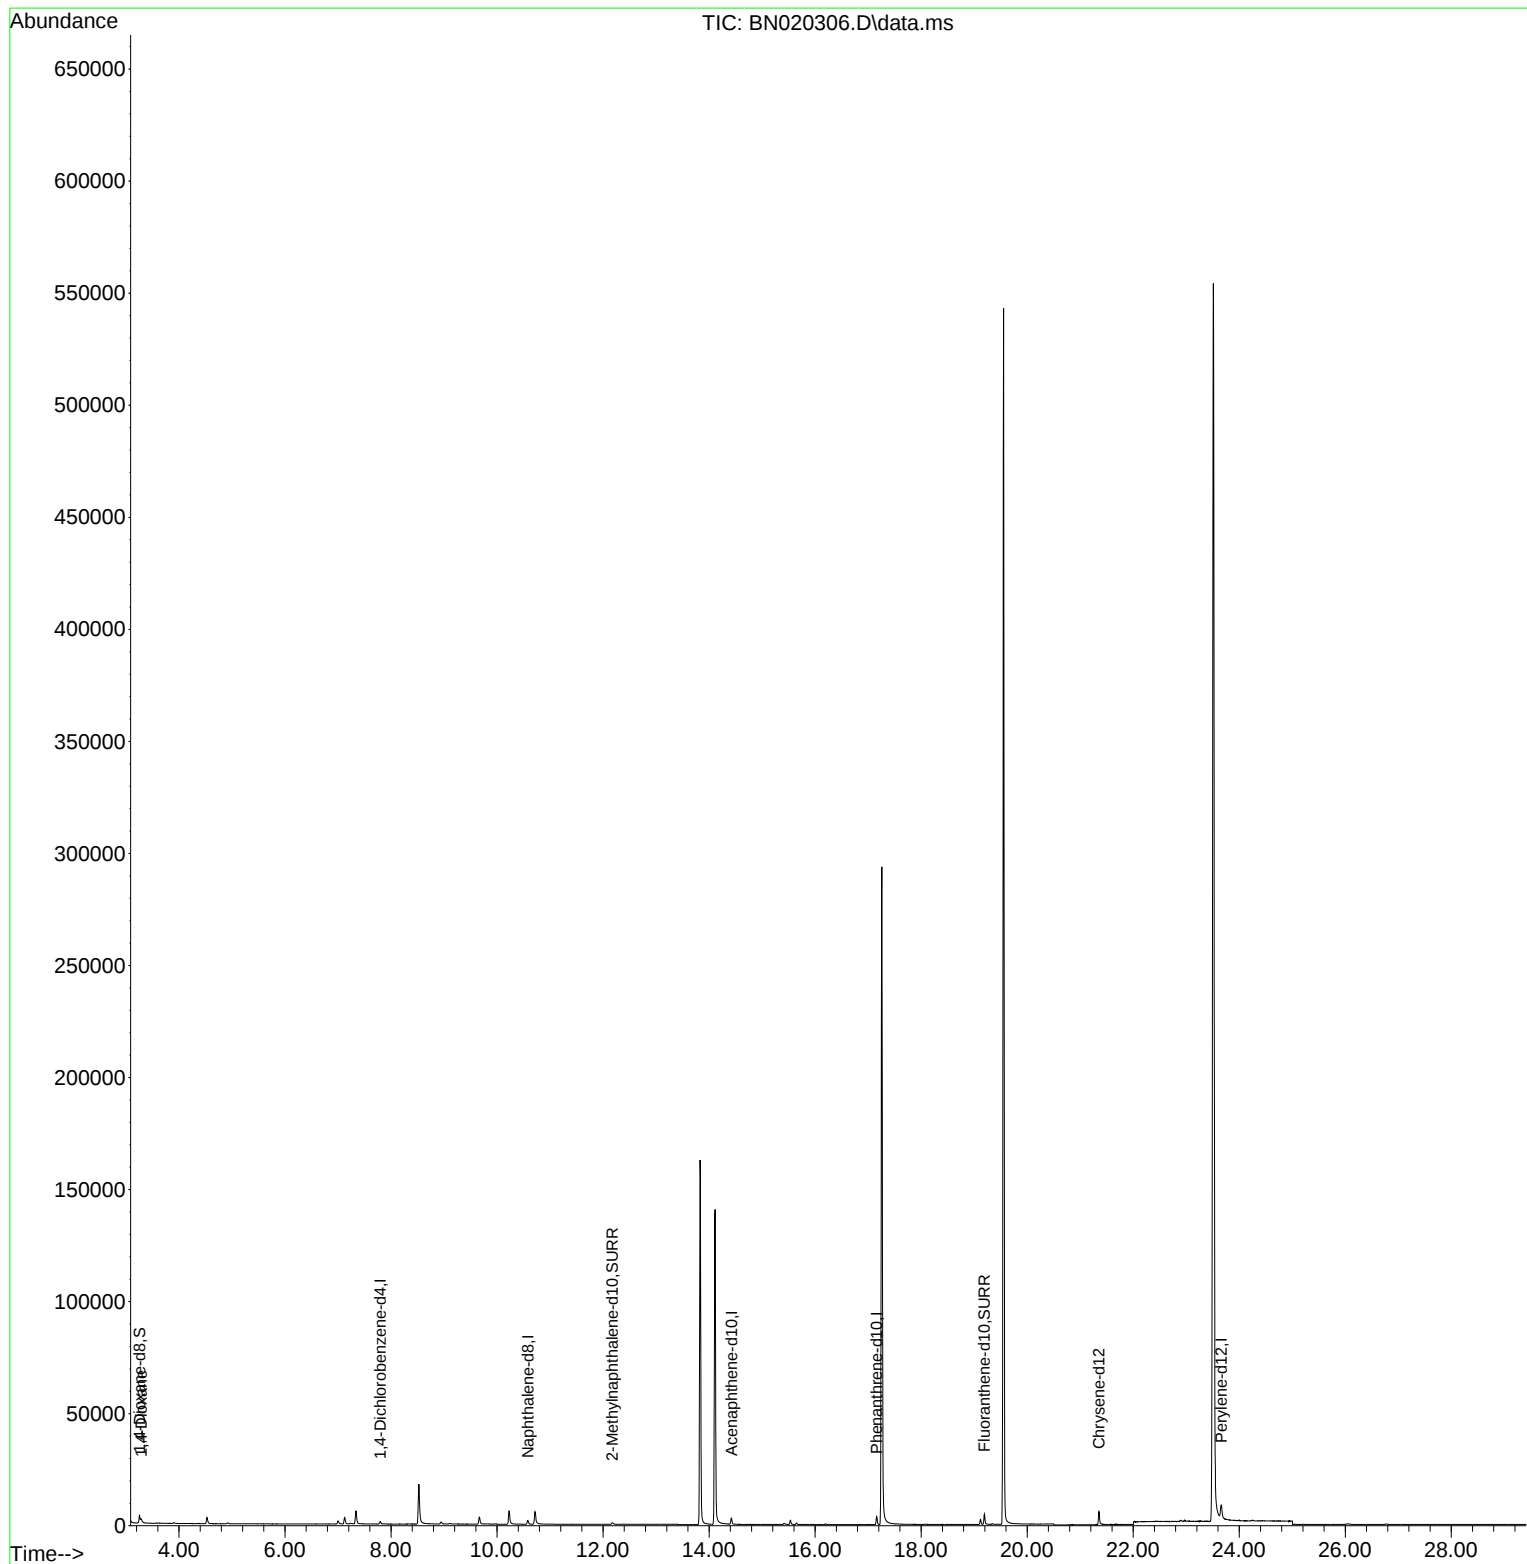

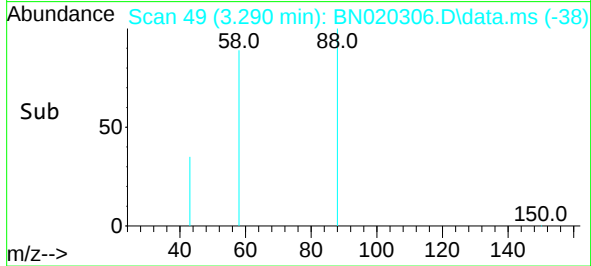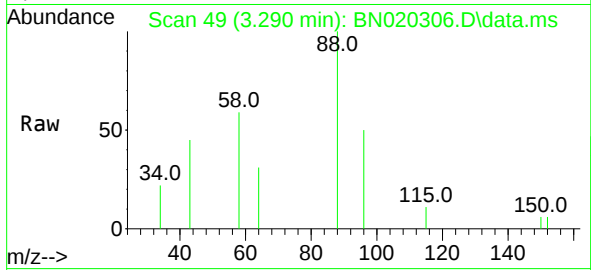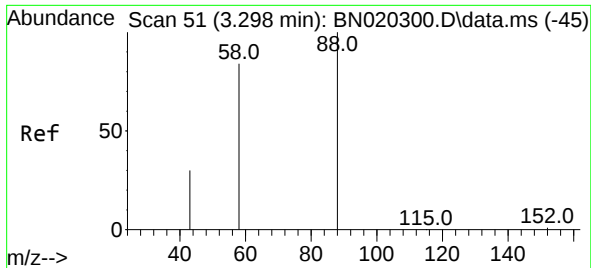

#2
 1,4-Dioxane
 Concen: 1.360 ng/ul m
 RT: 3.290 min Scan# 49
 Delta R.T. -0.004 min
 Lab File: BN020306.D
 Acq: 21 Jun 2022 14:14

Instrument :
 BNA_N
 ClientSampleId :
 YB7L2

Tgt Ion: 88 Resp: 98

Ion	Ratio	Lower	Upper
88	100		
43	45.5	31.6	47.4
58	59.3	23.8	35.6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

