

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
 Data File : BN020311.D
 Acq On : 21 Jun 2022 17:15
 Operator : CG/JU
 Sample : N3313-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

Quant Time: Jun 22 00:41:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:13:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	751	0.400	ng/ul	0.00
4) Naphthalene-d8	10.583	136	2776	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.417	164	2042	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.161	188	5041	0.400	ng/ul	0.00
17) Chrysene-d12	21.351	240	7143	0.400	ng/ul	0.00
23) Perylene-d12	23.660	264	10088	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	3554m	4.144	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.172	152	1674	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.191	212	6510	0.442	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.290	88	897	1.087	ng/ul#	66

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062122\
Data File : BN020311.D
Acq On : 21 Jun 2022 17:15
Operator : CG/JU
Sample : N3313-06
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YB7L4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :mohammad ahmed 06/28/2022


Quant Time: Jun 22 00:41:54 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:13:51 2022
Response via : Initial Calibration

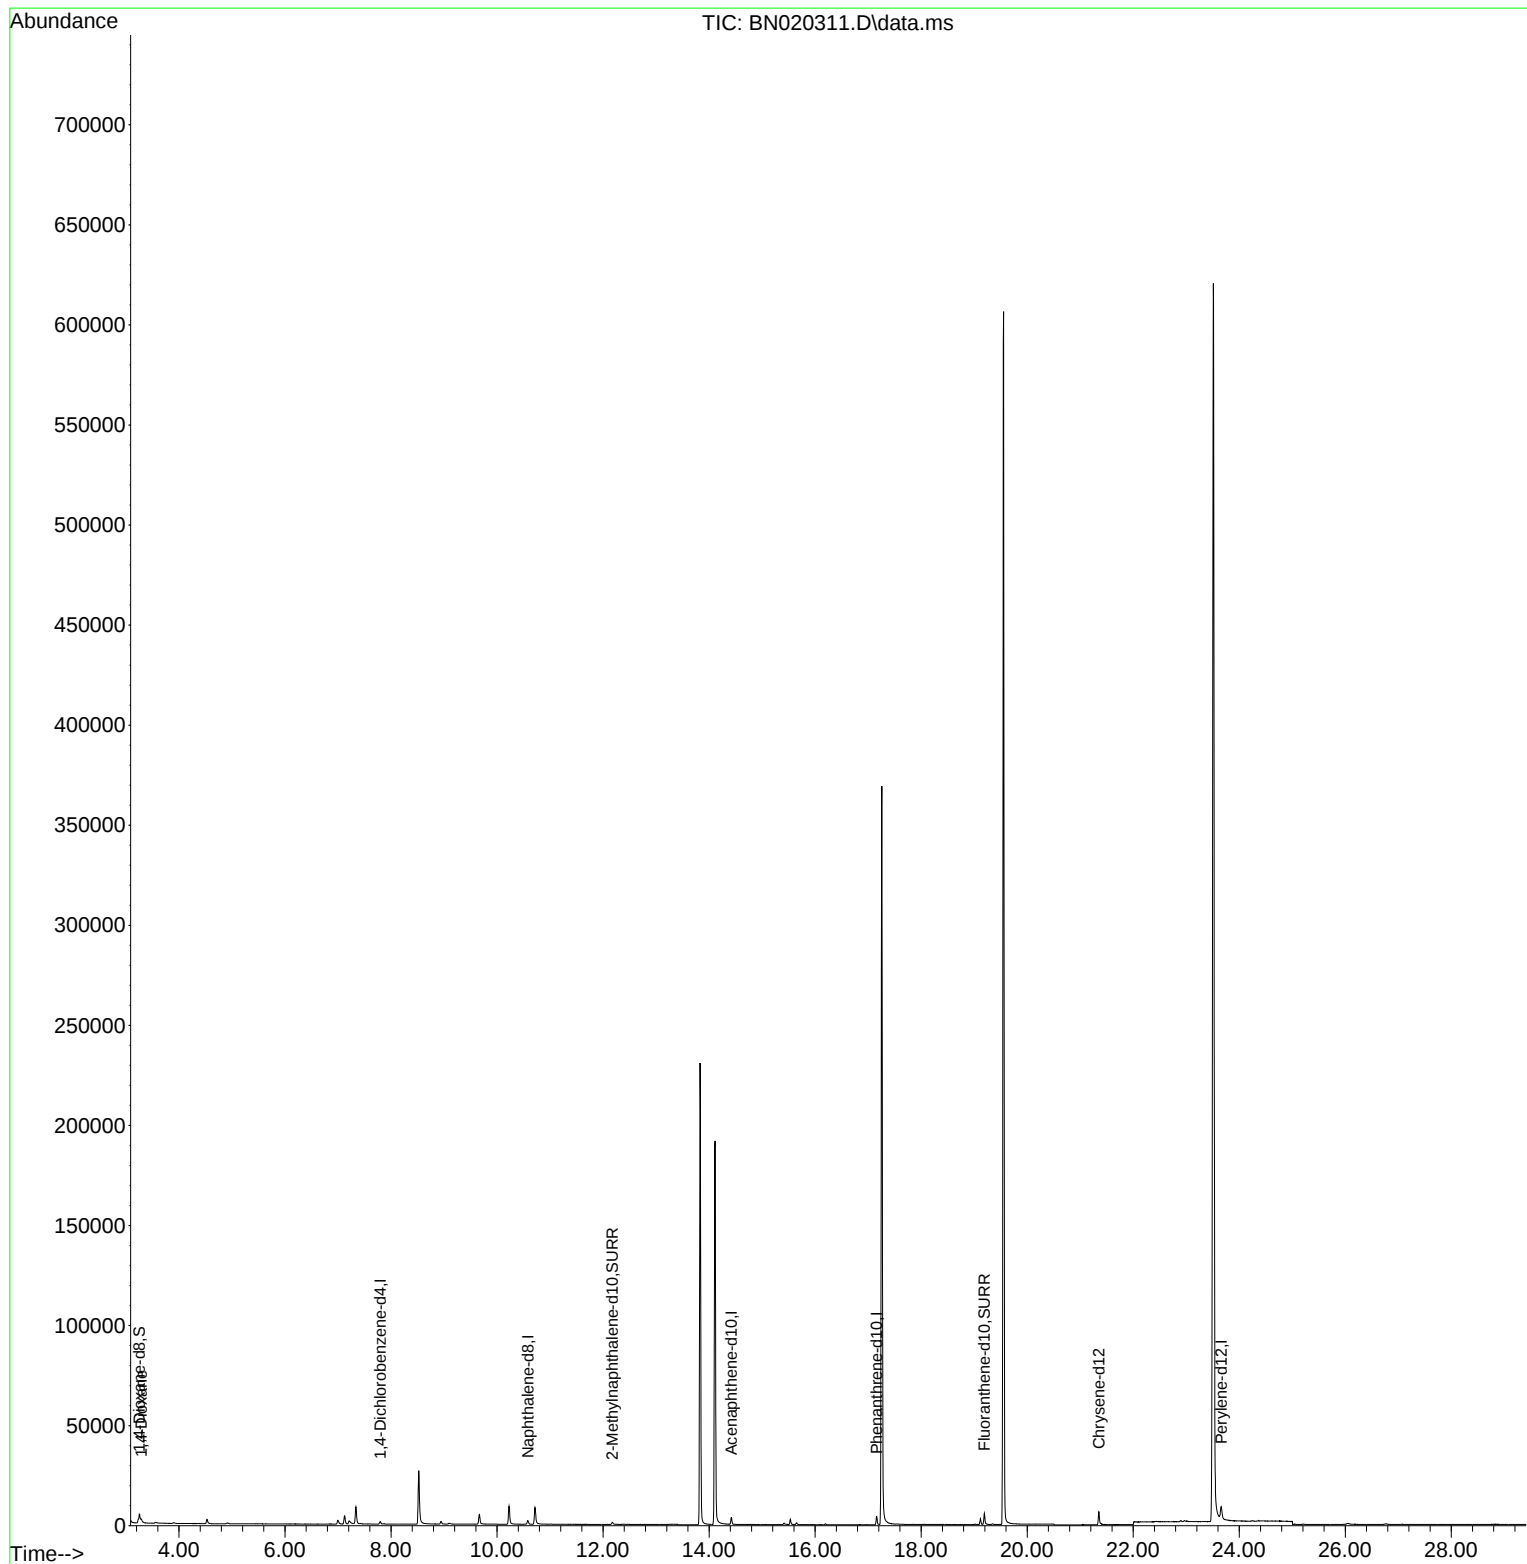

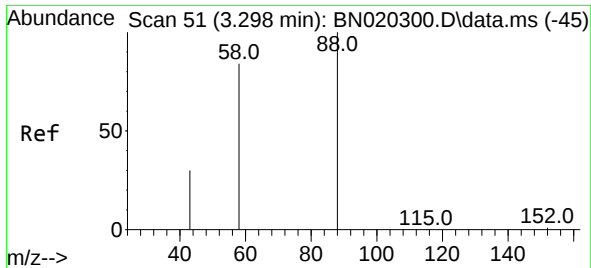

#2
 1,4-Dioxane
 Concen: 1.087 ng/ul
 RT: 3.290 min Scan# 49
 Delta R.T. -0.004 min
 Lab File: BN020311.D
 Acq: 21 Jun 2022 17:15

Instrument :
 BNA_N
 ClientSampleId :
 YB7L4

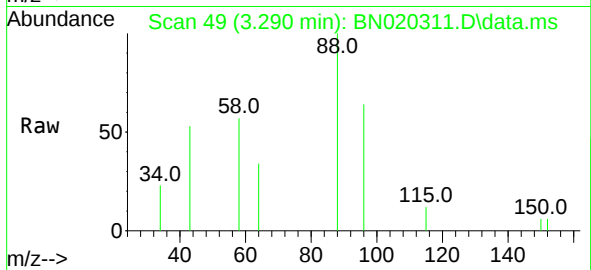

Tgt Ion: 88 Resp: 89
 Ion Ratio Lower Upper
 88 100
 43 52.6 31.6 47.4
 58 57.2 23.8 35.6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :mohammad ahmed 06/28/2022

